

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091223\
Data File : FF013488.D
Signal(s) : FID2B.ch
Acq On : 12 Sep 2023 10:46
Operator : YP\AJ
Sample : PB155476BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 01:48:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083123.M
Quant Title :
QLast Update : Fri Sep 01 02:22:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.974	2343828	19.924 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.383	85636	0.873 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091223\
Data File : FF013488.D
Signal(s) : FID2B.ch
Acq On : 12 Sep 2023 10:46
Operator : YP\AJ
Sample : PB155476BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 01:48:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083123.M
Quant Title :
QLast Update : Fri Sep 01 02:22:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

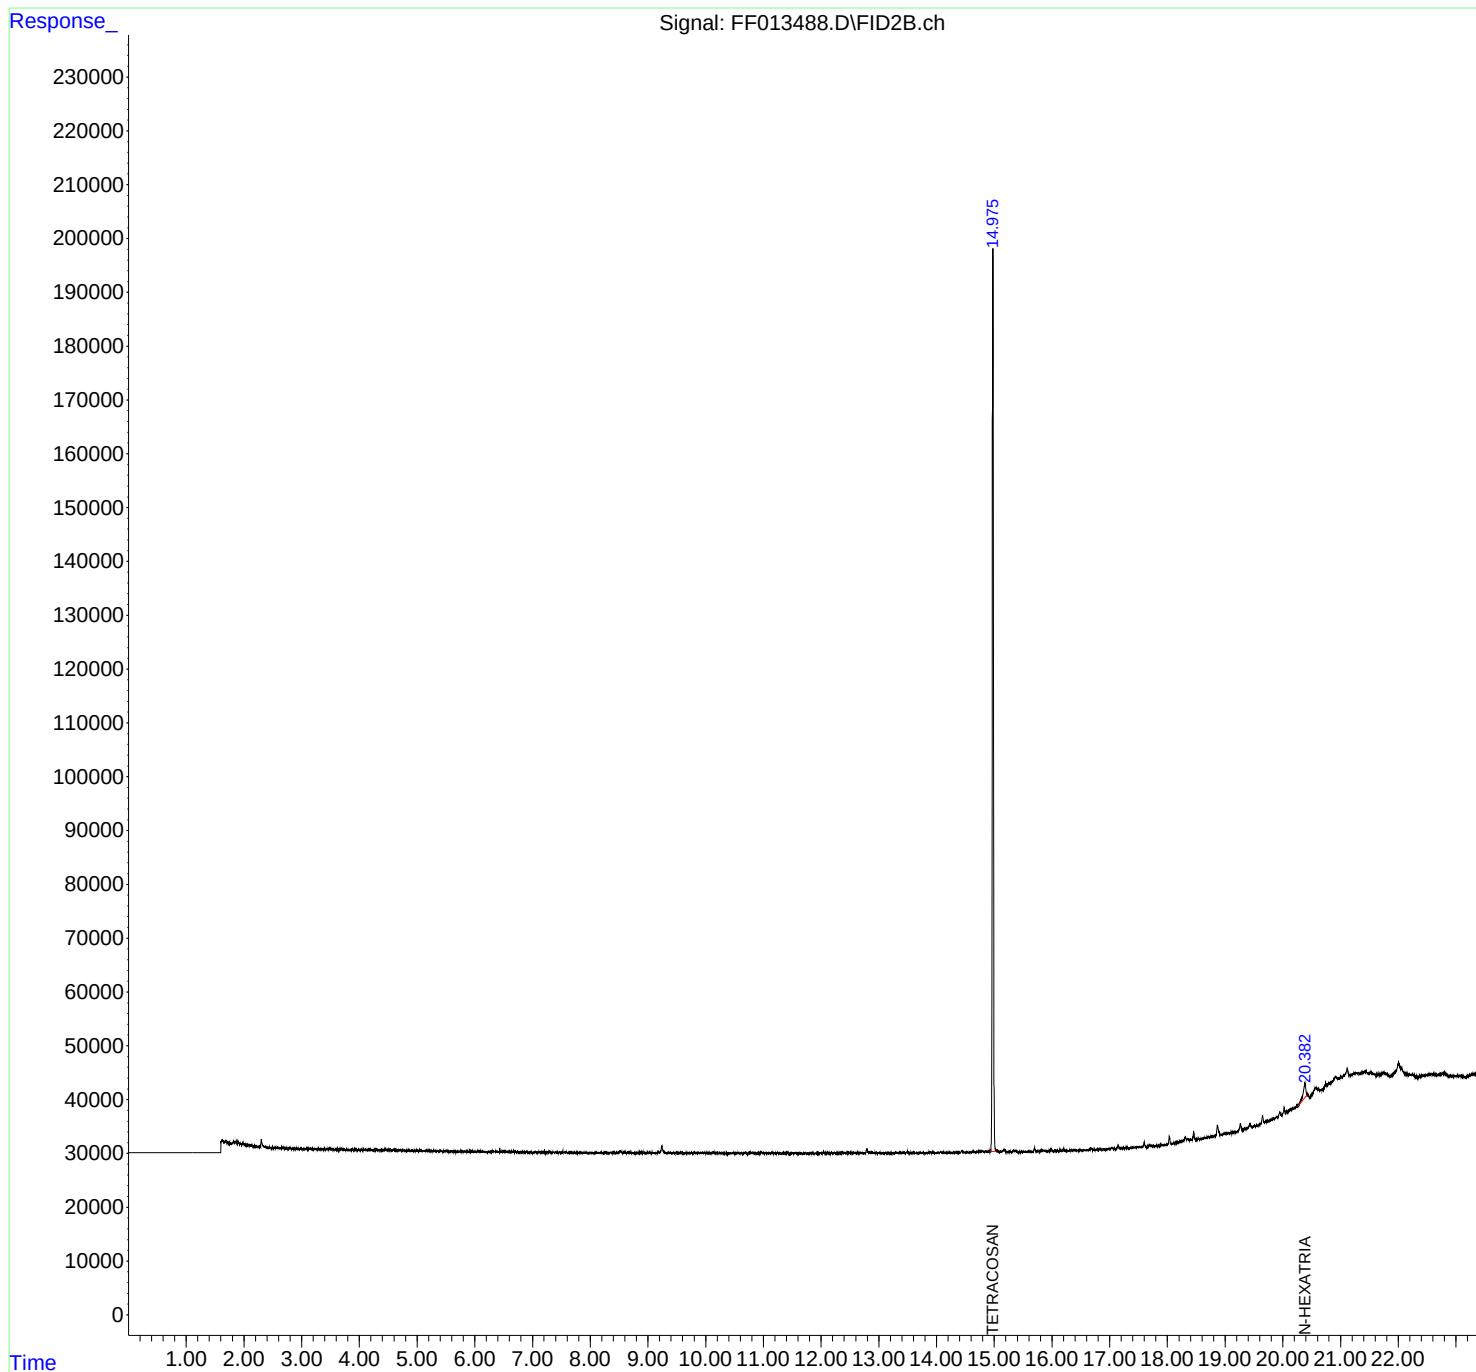


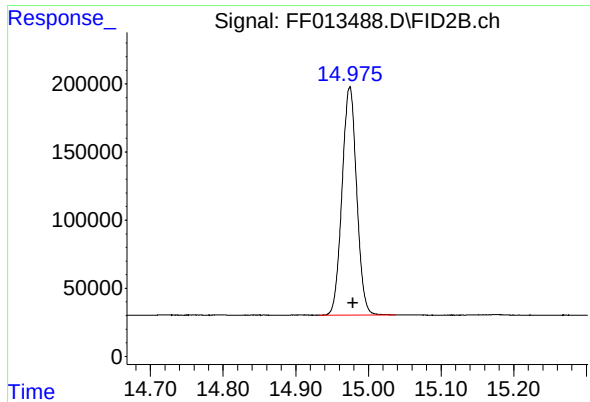

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.974 min
Delta R.T.: -0.005 min
Response: 2343828
Conc: 19.92 ug/ml

Instrument :
FID_F
ClientSampleId :

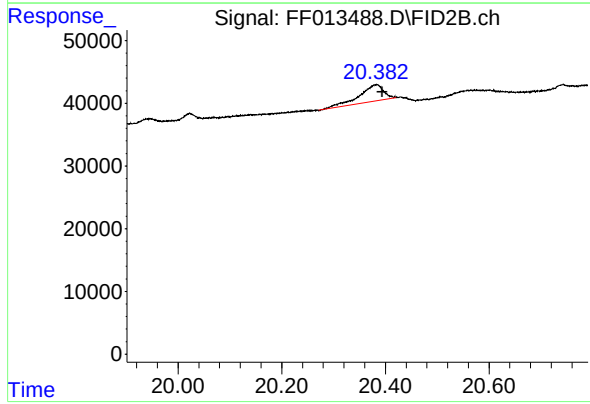

#16 N-HEXATRIACONTANE

R.T.: 20.383 min
Delta R.T.: -0.012 min
Response: 85636
Conc: 0.87 ug/ml