

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091223\
 Data File : FF013489.D
 Signal(s) : FID2B.ch
 Acq On : 12 Sep 2023 11:17
 Operator : YP\AJ
 Sample : 04346-19
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RR-DIES-WP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/13/2023
 Supervised By :Ankita Jodhani 09/13/2023

Integration File: autoint1.e
 Quant Time: Sep 13 01:48:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083123.M
 Quant Title :
 QLast Update : Fri Sep 01 02:22:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.975	2102270	17.870 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091223\
Data File : FF013489.D
Signal(s) : FID2B.ch
Acq On : 12 Sep 2023 11:17
Operator : YP\AJ
Sample : 04346-19
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
RR-DIES-WP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/13/2023
Supervised By :Ankita Jodhani 09/13/2023

Integration File: autoint1.e
Quant Time: Sep 13 01:48:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083123.M
Quant Title :
QLast Update : Fri Sep 01 02:22:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

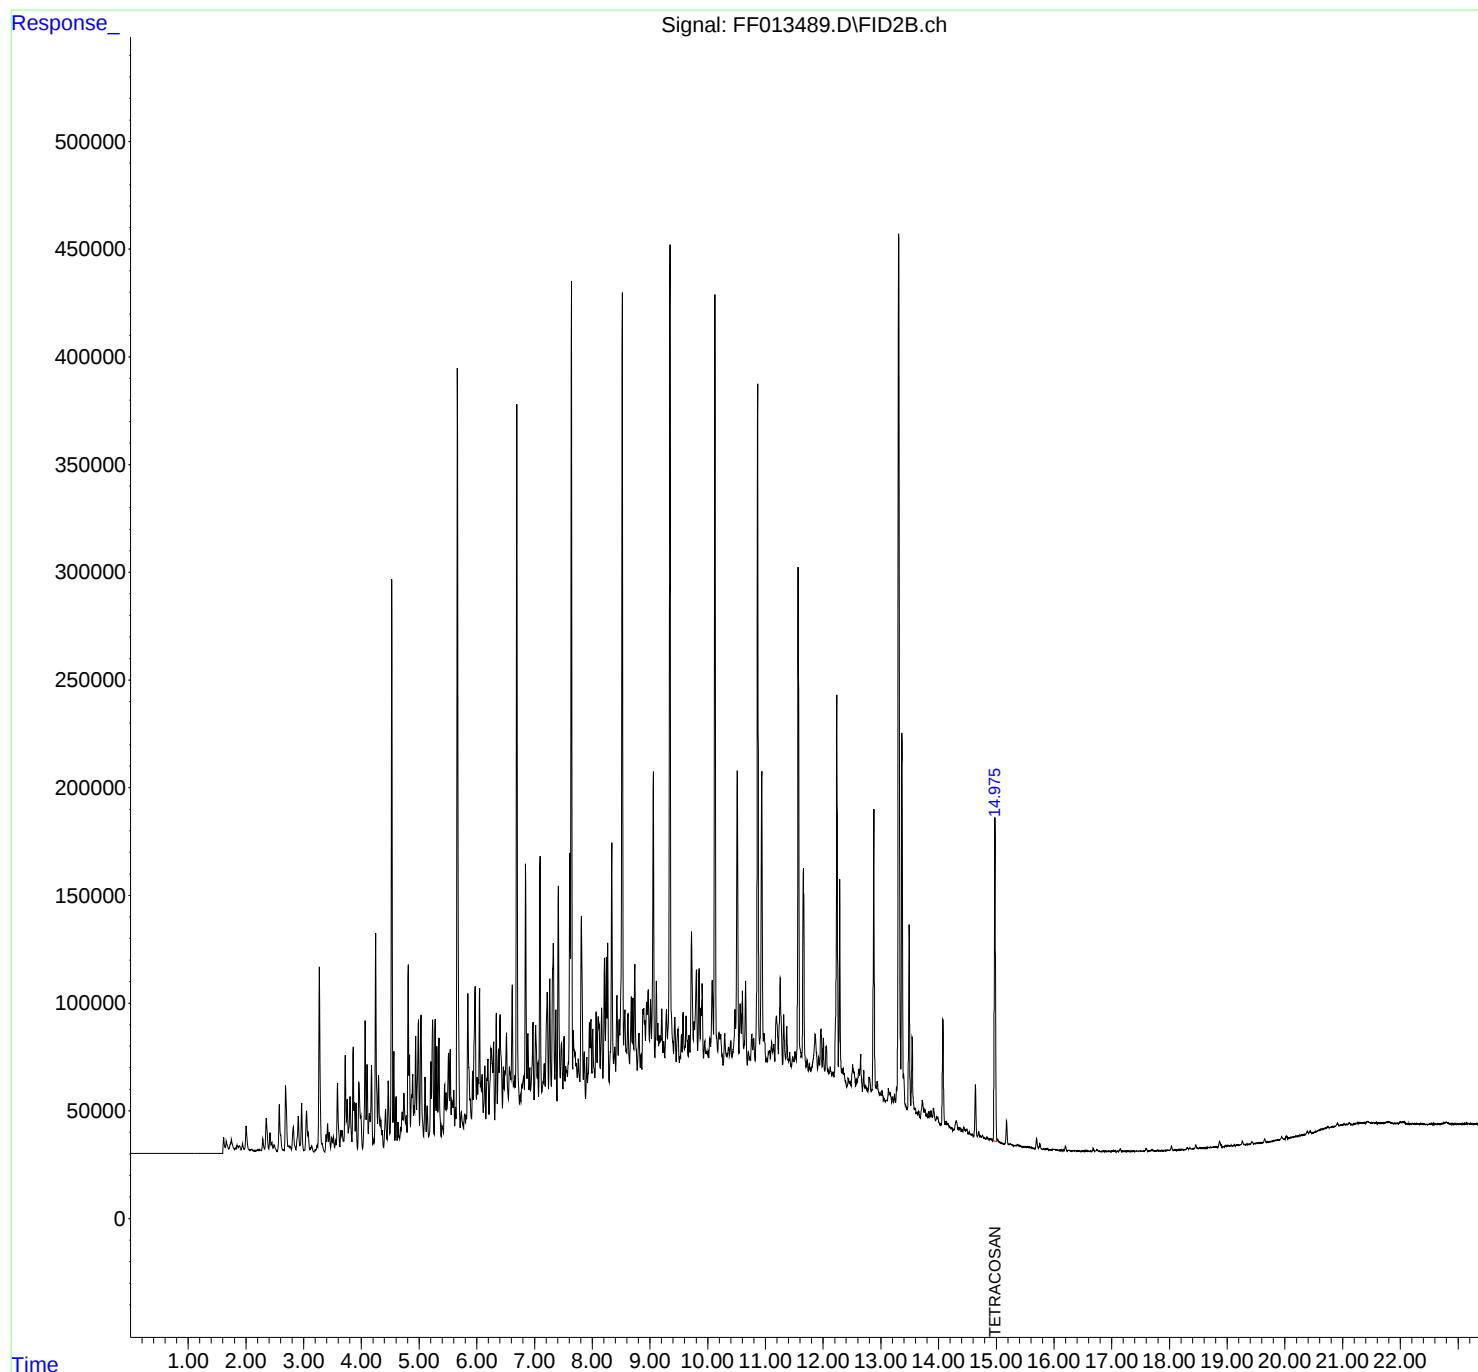

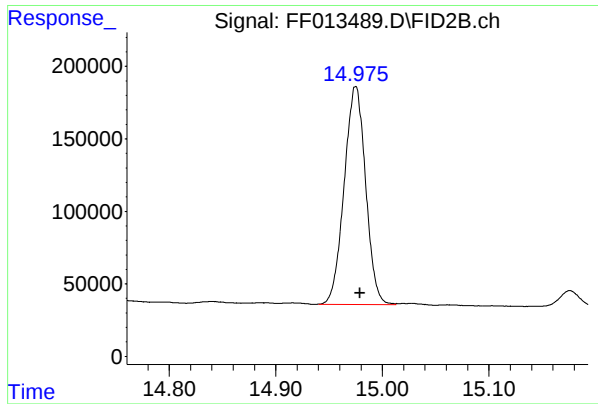

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.975 min
Delta R.T.: -0.004 min
Response: 2102270
Conc: 17.87 ug/ml

Instrument :

FID_F

ClientSampleId :

RR-DIES-WP

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 09/13/2023
Supervised By :Ankita Jodhani 09/13/2023