

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091319\
Data File : FF005545.D
Signal(s) : FID2B.ch
Acq On : 13 Sep 2019 08:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 14 03:44:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.621	1841347	17.207 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.536	271952	2.194 ug/ml
15)	N-TETRATRIACONTANE	19.324	108468	0.900 ug/ml
16)	N-HEXATRIACONTANE	20.113	113160	0.943 ug/ml
18)	N-TETRACONTANE	21.696	2047952	16.108 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091319\
Data File : FF005545.D
Signal(s) : FID2B.ch
Acq On : 13 Sep 2019 08:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 14 03:44:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

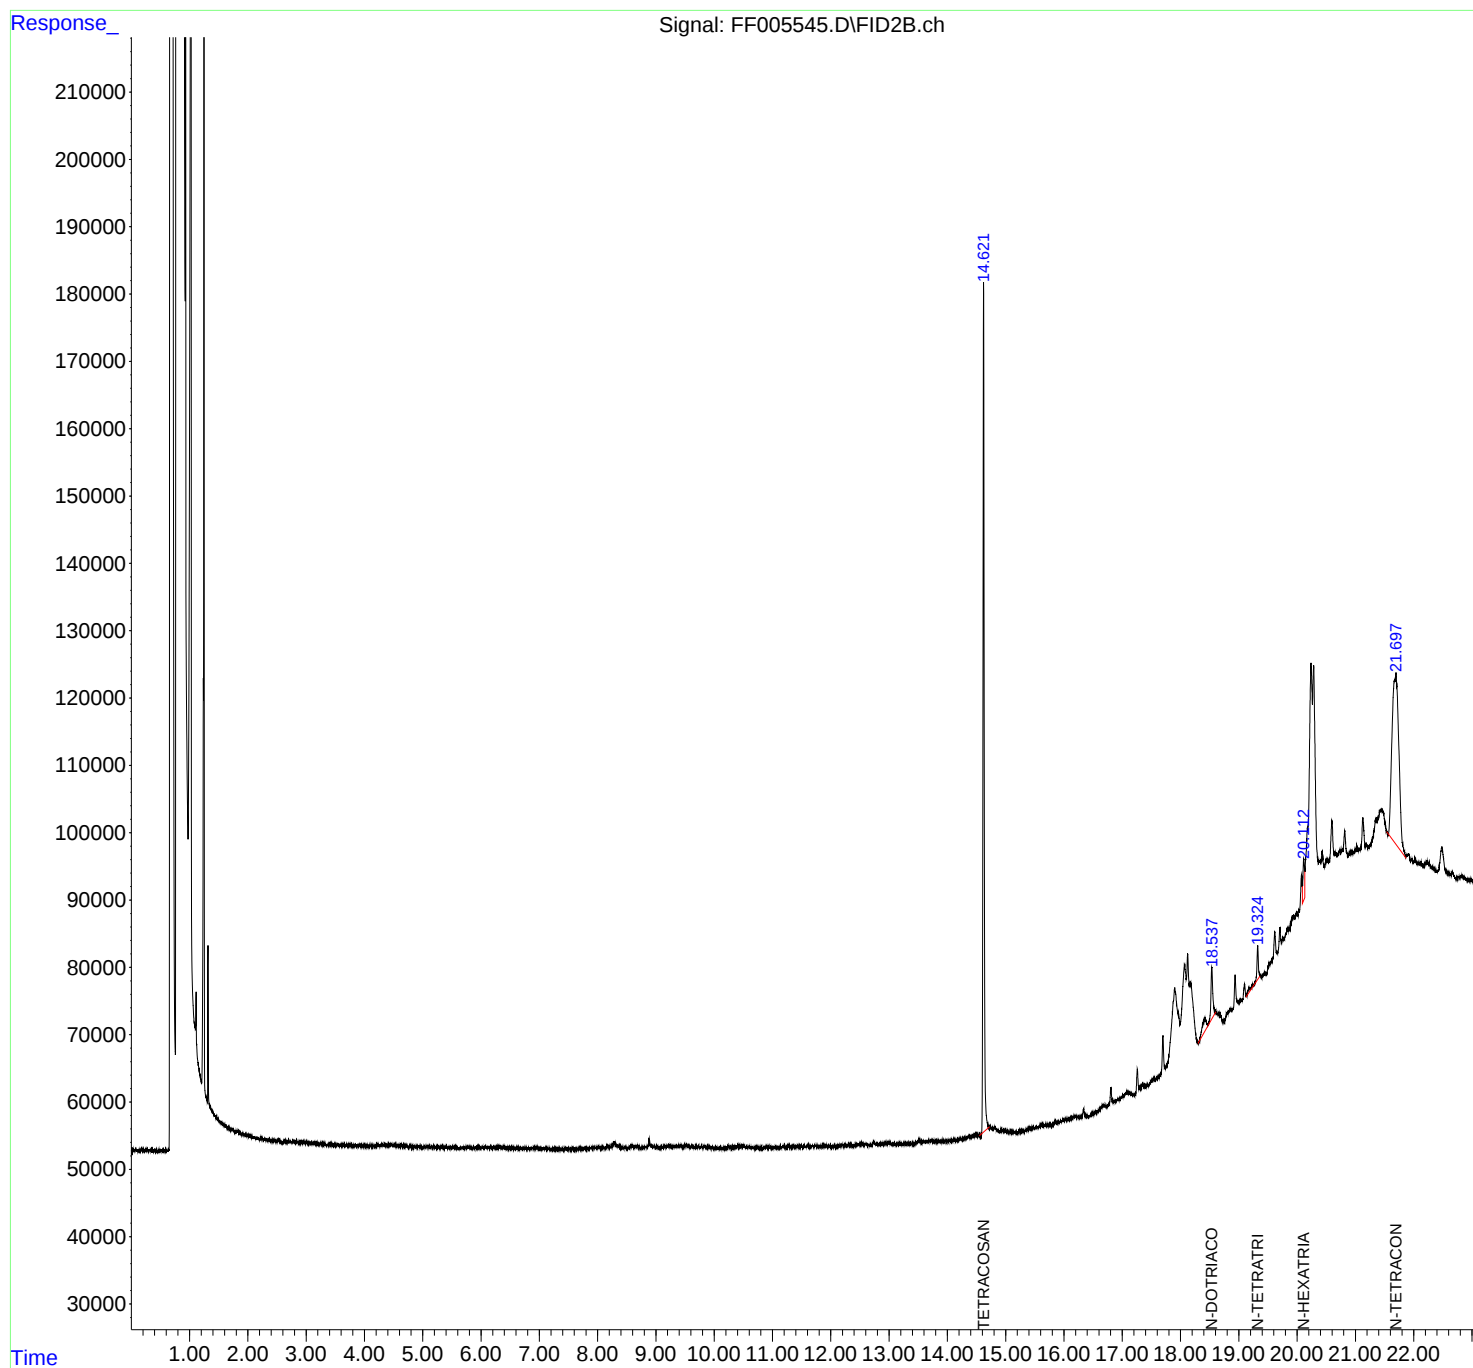

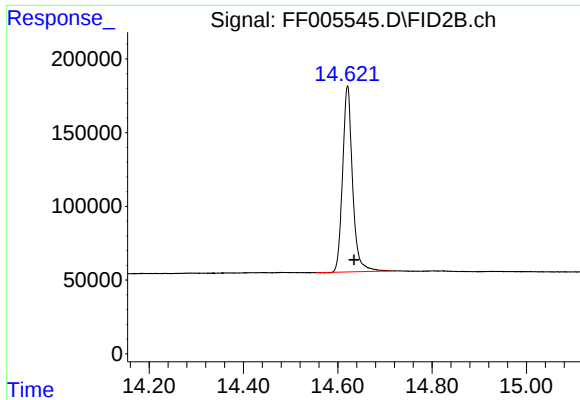


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.621 min
Delta R.T.: -0.014 min
Response: 1841347
Conc: 17.21 ug/ml

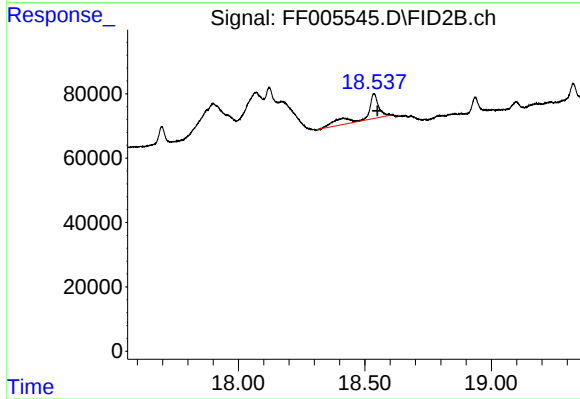


#14 N-DOTRIACONTANE

R.T.: 18.536 min
Delta R.T.: -0.013 min
Response: 271952
Conc: 2.19 ug/ml

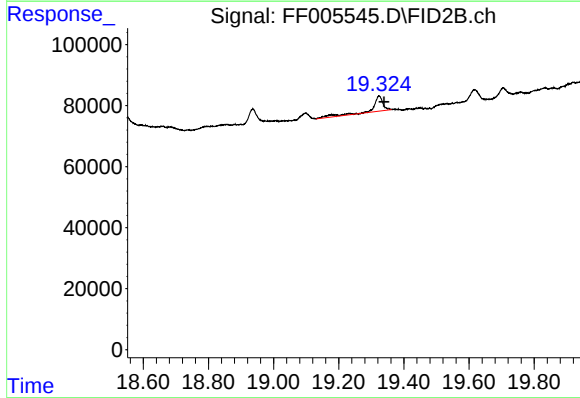


#15 N-TETRATRIACONTANE

R.T.: 19.324 min
Delta R.T.: -0.015 min
Response: 108468
Conc: 0.90 ug/ml

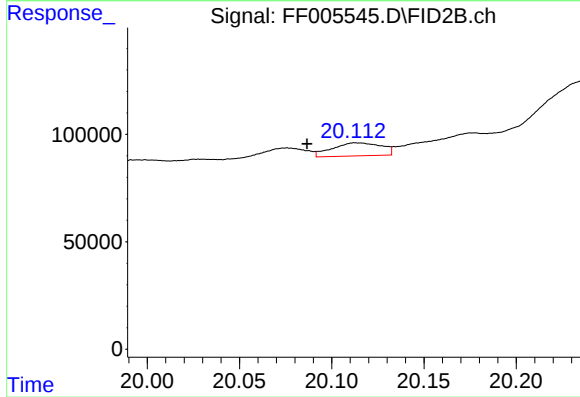

#16 N-HEXATRIACONTANE

R.T.: 20.113 min
Delta R.T.: 0.027 min
Response: 113160
Conc: 0.94 ug/ml

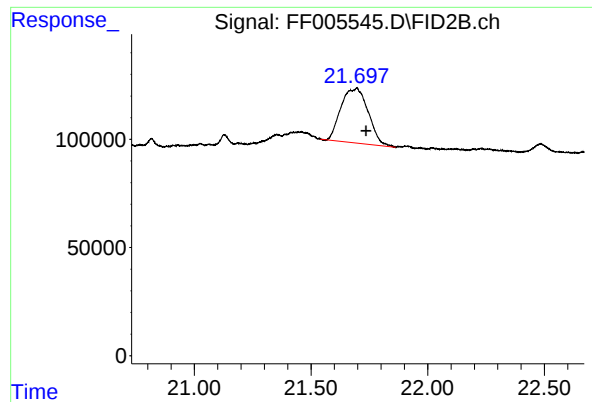

#18 N-TETRACONTANE

R.T.: 21.696 min
Delta R.T.: -0.040 min
Response: 2047952
Conc: 16.11 ug/ml