

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091319\
Data File : FF005551.D
Signal(s) : FID2B.ch
Acq On : 13 Sep 2019 12:01
Operator : DD\AJ
Sample : K4850-04 50X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 14 03:46:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.375	315311	2.200 ug/ml
4) N-TETRADECANE	8.145	339745	2.410 ug/ml
6) N-OCTADECANE	11.284f	170789	1.269 ug/ml
7) N-EICOSANE	12.494	166118	1.267 ug/ml
8) N-DOCOSANE	13.745	204605	1.625 ug/ml
10) N-TETRACOSANE	14.804	695854	5.690 ug/ml
11) N-HEXACOSANE	15.854	80748	0.675 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091319\
Data File : FF005551.D
Signal(s) : FID2B.ch
Acq On : 13 Sep 2019 12:01
Operator : DD\AJ
Sample : K4850-04 50X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 14 03:46:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

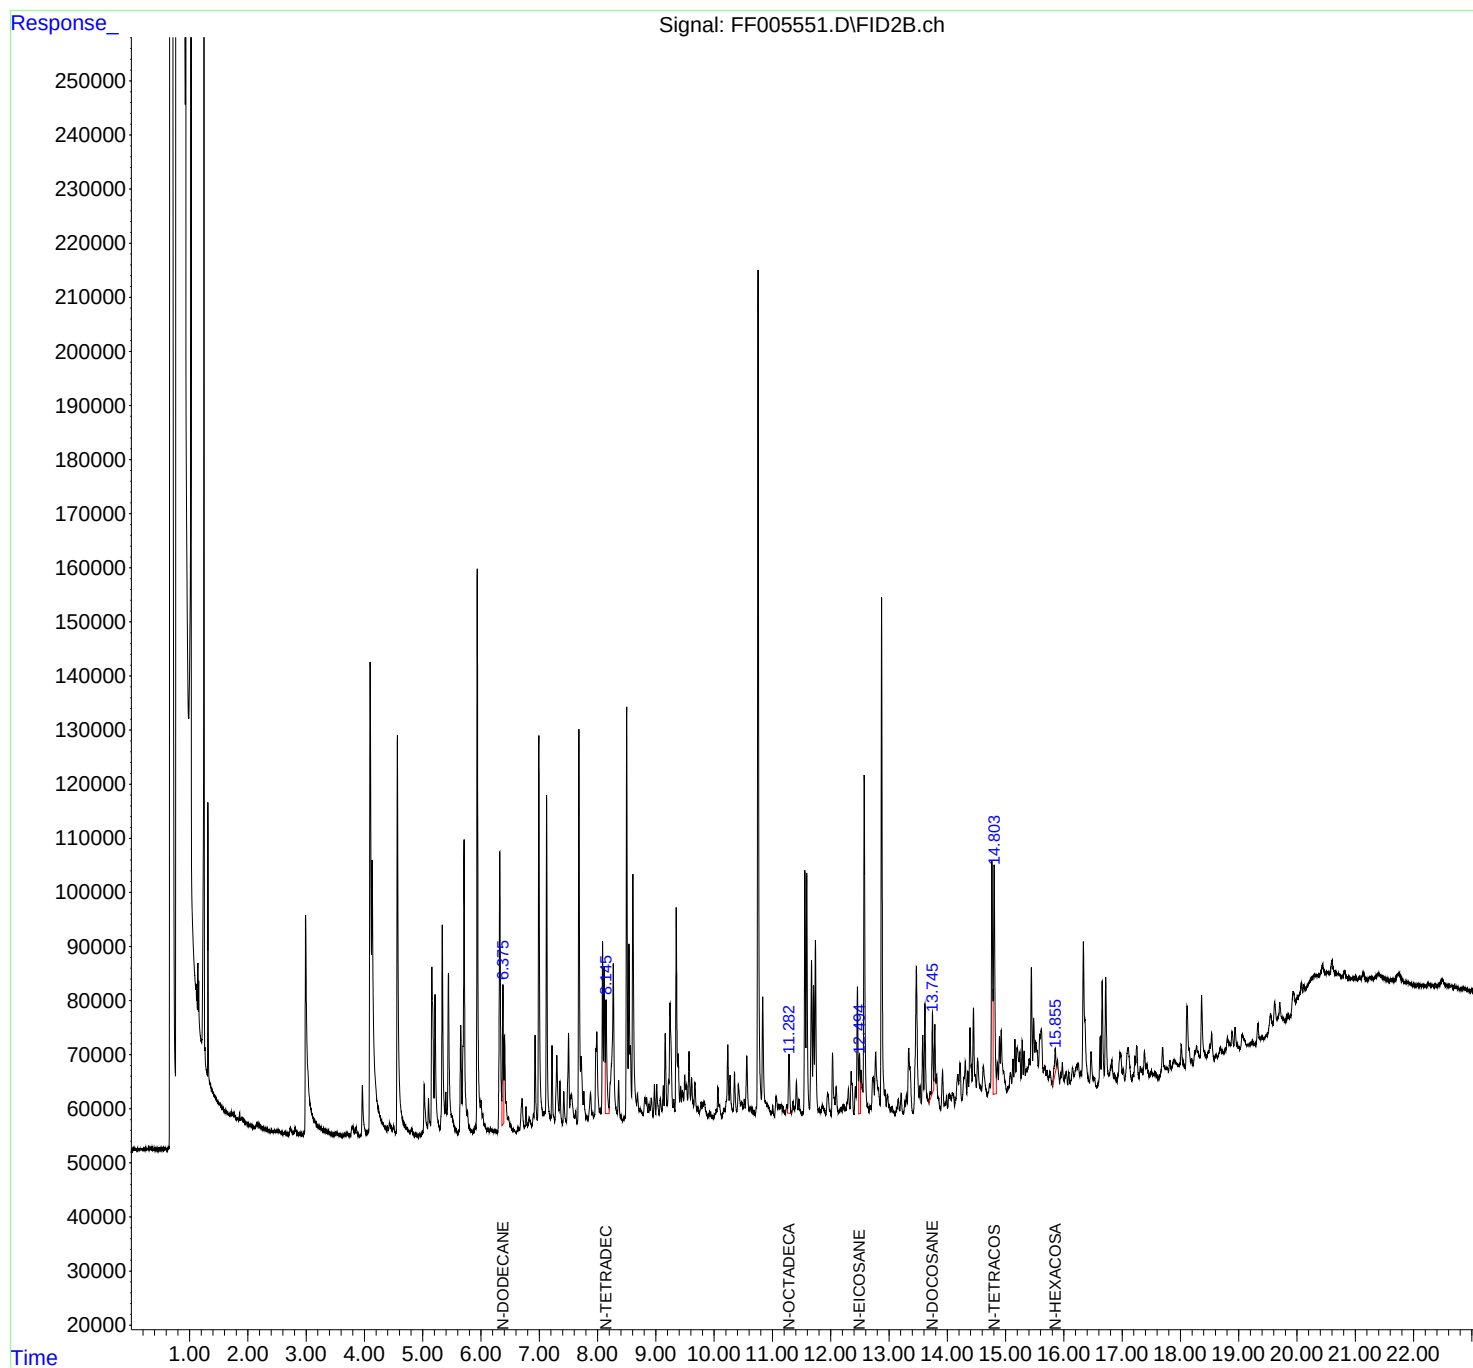

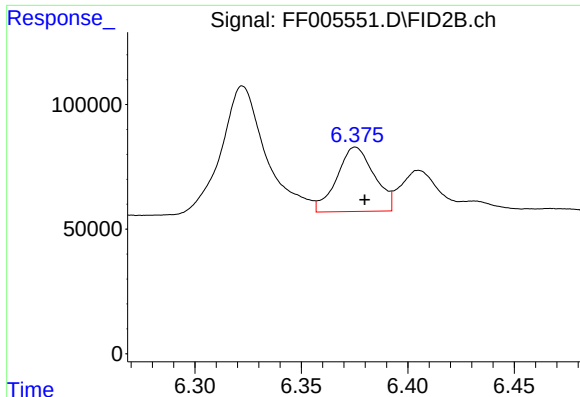


#3 N-DODECANE

R.T.: 6.375 min
Delta R.T.: -0.004 min
Response: 315311
Conc: 2.20 ug/ml

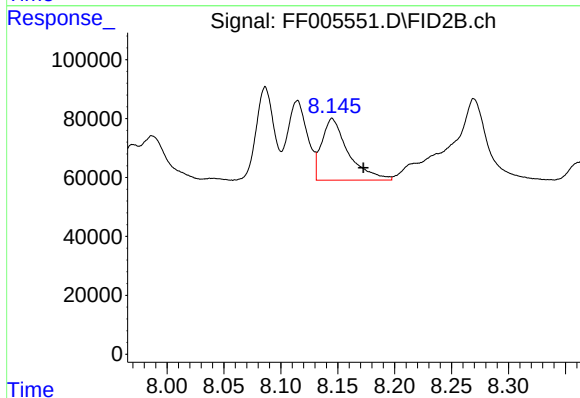


#4 N-TETRADECANE

R.T.: 8.145 min
Delta R.T.: -0.027 min
Response: 339745
Conc: 2.41 ug/ml

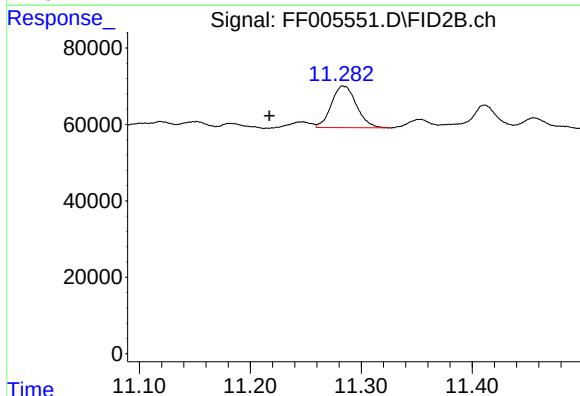


#6 N-OCTADECANE

R.T.: 11.284 min
Delta R.T.: 0.067 min
Response: 170789
Conc: 1.27 ug/ml

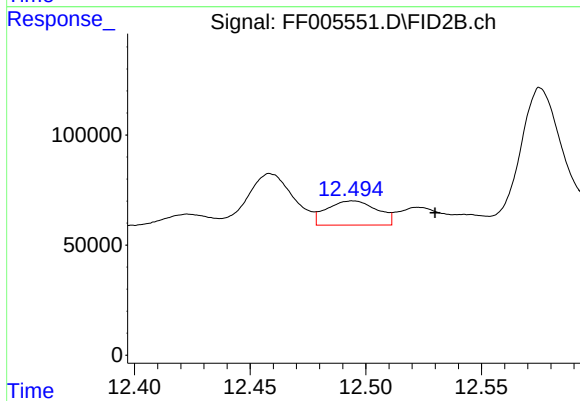


#7 N-EICOSANE

R.T.: 12.494 min
Delta R.T.: -0.036 min
Response: 166118
Conc: 1.27 ug/ml

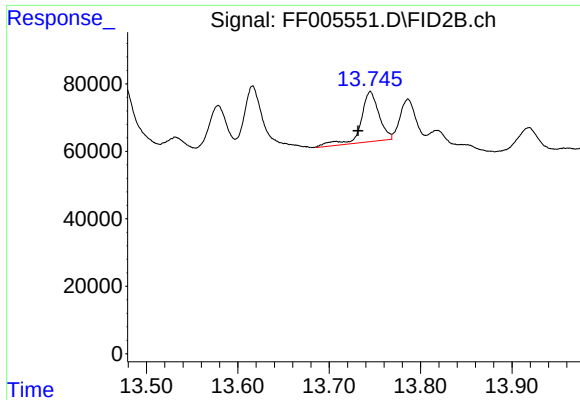


#8 N-DOCOSANE

R.T.: 13.745 min
Delta R.T.: 0.013 min
Response: 204605
Conc: 1.63 ug/ml

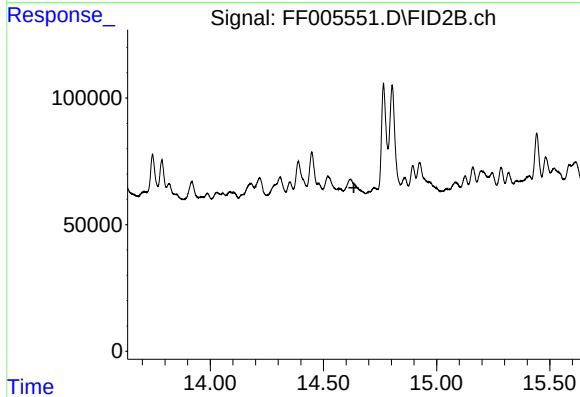


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.635 min
Response: 0
Conc: N.D.

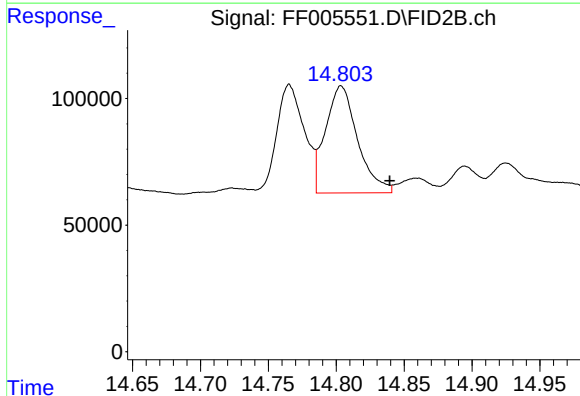

#10 N-TETRACOSANE

R.T.: 14.804 min
Delta R.T.: -0.036 min
Response: 695854
Conc: 5.69 ug/ml

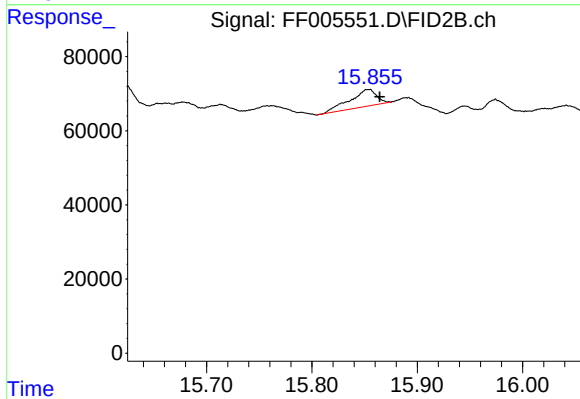

#11 N-HEXACOSANE

R.T.: 15.854 min
Delta R.T.: -0.011 min
Response: 80748
Conc: 0.67 ug/ml