

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091324AL\
Data File : FF014513.D
Signal(s) : FID2B.ch
Acq On : 13 Sep 2024 21:06
Operator : YP\AJ
Sample : P3964-04DL 5X
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SINK-1DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2024
Supervised By :Ankita Jodhani 09/16/2024

Integration File: autoint1.e
Quant Time: Sep 14 04:23:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 091124.M
Quant Title : GC Extractables
QLast Update : Wed Sep 11 08:07:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.247	451765	4.247 ug/mlm
Spiked Amount	50.000	Recovery =	8.49%
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091324AL\
Data File : FF014513.D
Signal(s) : FID2B.ch
Acq On : 13 Sep 2024 21:06
Operator : YP\AJ
Sample : P3964-04DL 5X
Misc :
ALS Vial : 73 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SINK-1DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2024
Supervised By :Ankita Jodhani 09/16/2024

Integration File: autoint1.e
Quant Time: Sep 14 04:23:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 091124.M
Quant Title : GC Extractables
QLast Update : Wed Sep 11 08:07:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

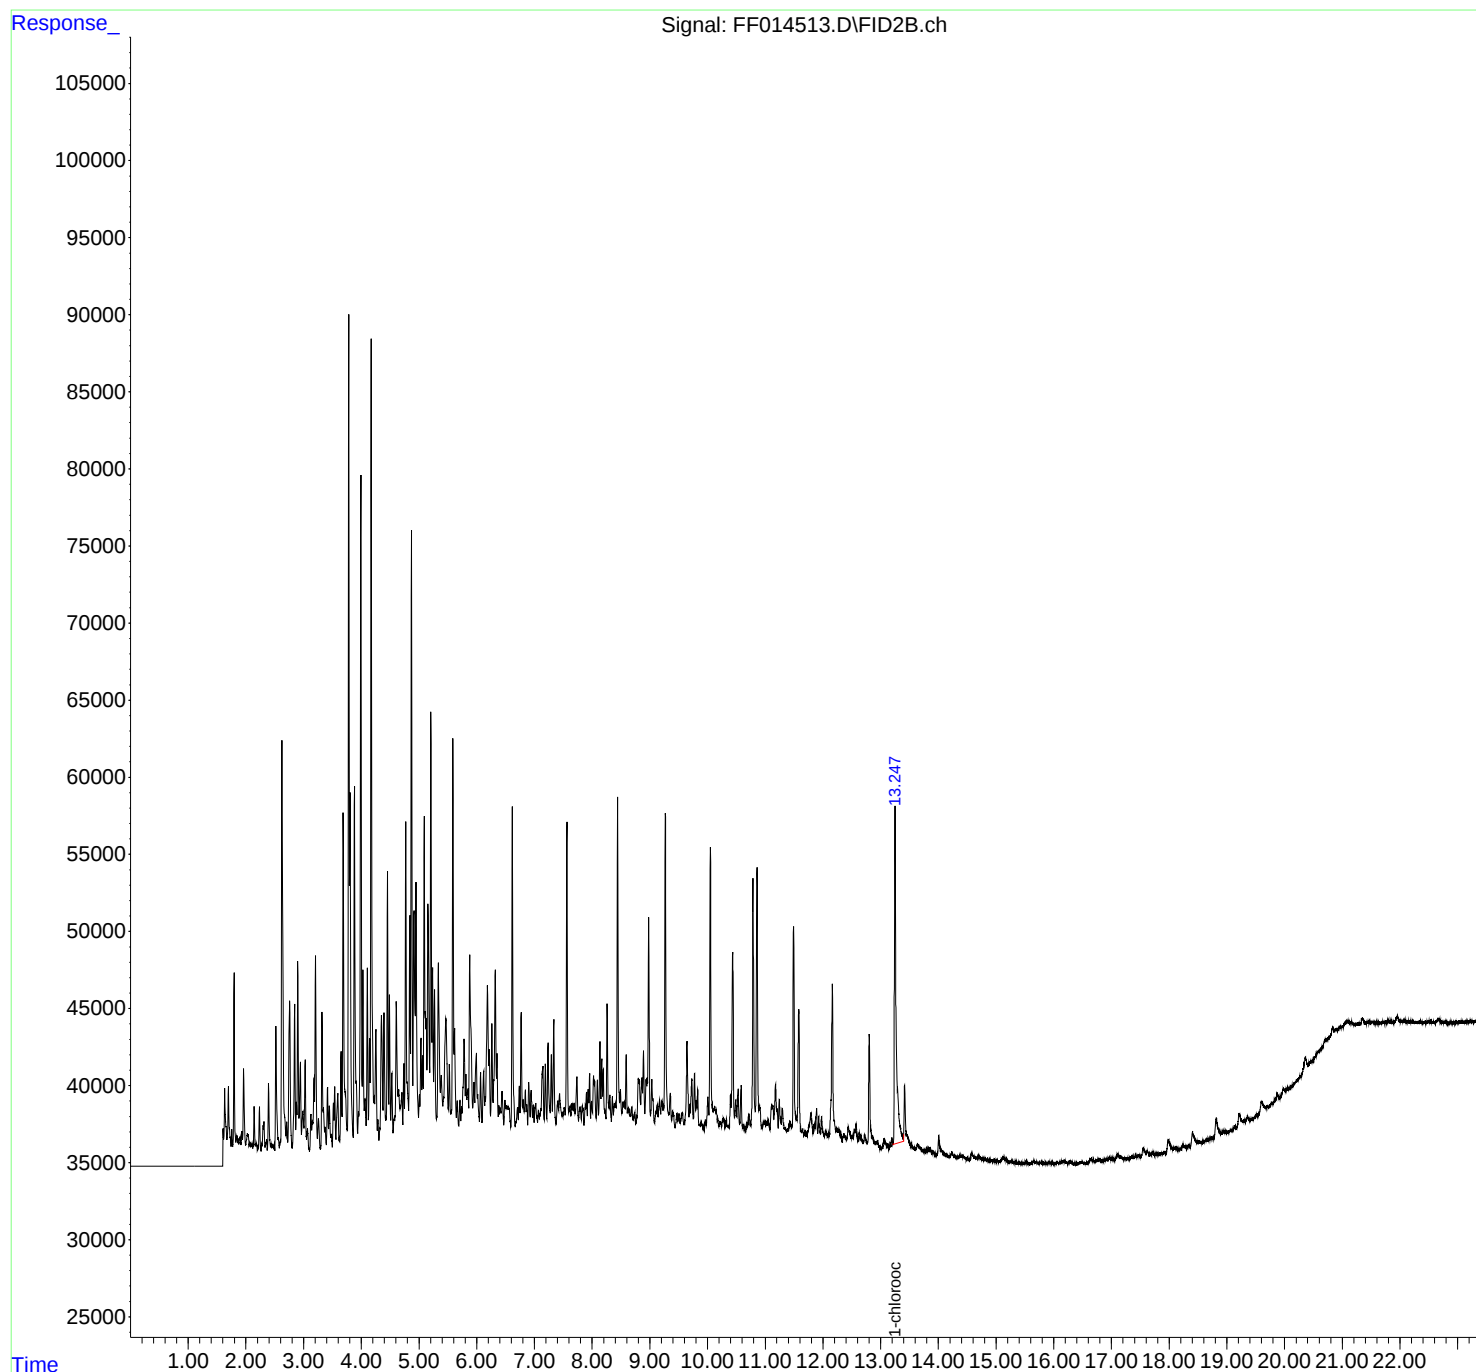

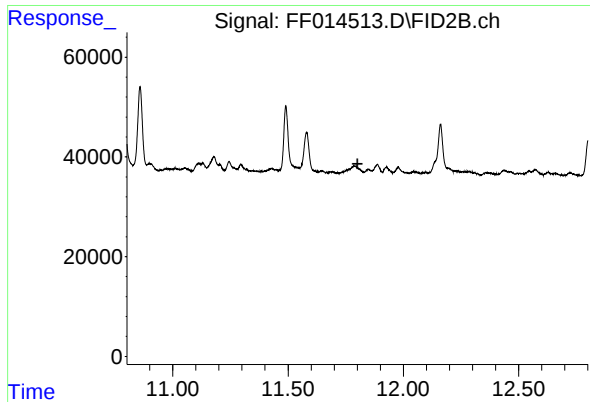


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.801 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
SINK-1DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/16/2024
Supervised By :Ankita Jodhani 09/16/2024

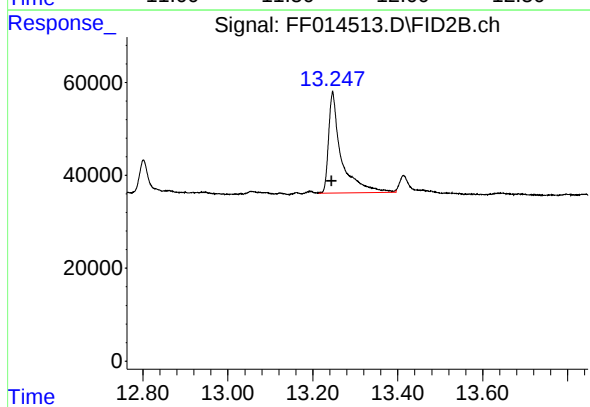

#12 1-chlorooctadecane (SURR)

R.T.: 13.247 min
Delta R.T.: 0.002 min
Response: 451765
Conc: 4.25 ug/ml m