

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091422\
 Data File : FF011446.D
 Signal(s) : FID2B.ch
 Acq On : 14 Sep 2022 16:51
 Operator : YP\AJ
 Sample : N4613-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 15 05:14:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	1812977	16.174 ug/ml
Target Compounds			
5) N-HEXADECANE	9.942	44977	0.339 ug/ml
7) N-EICOSANE	12.685	59049	0.449 ug/ml
8) N-DOCOSANE	13.890	95528	0.747 ug/ml
10) N-TETRACOSANE	14.985	74378	0.584 ug/ml
11) N-HEXACOSANE	16.007	113207	0.906 ug/ml
12) N-OCTACOSANE	16.953	175992	1.437 ug/ml
13) N-TRIACONTANE	17.836	184780	1.532 ug/ml
14) N-DOTRIACONTANE	18.667	115264	0.974 ug/ml
15) N-TETRATRIACONTANE	19.457	66684	0.584 ug/ml
16) N-HEXATRIACONTANE	20.196	277099	2.603 ug/ml
17) N-OCTATRIACONTANE	20.895	397102	3.817 ug/ml
18) N-TETRACONTANE	21.695	133306	1.263 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091422\
Data File : FF011446.D
Signal(s) : FID2B.ch
Acq On : 14 Sep 2022 16:51
Operator : YP\AJ
Sample : N4613-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 15 05:14:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

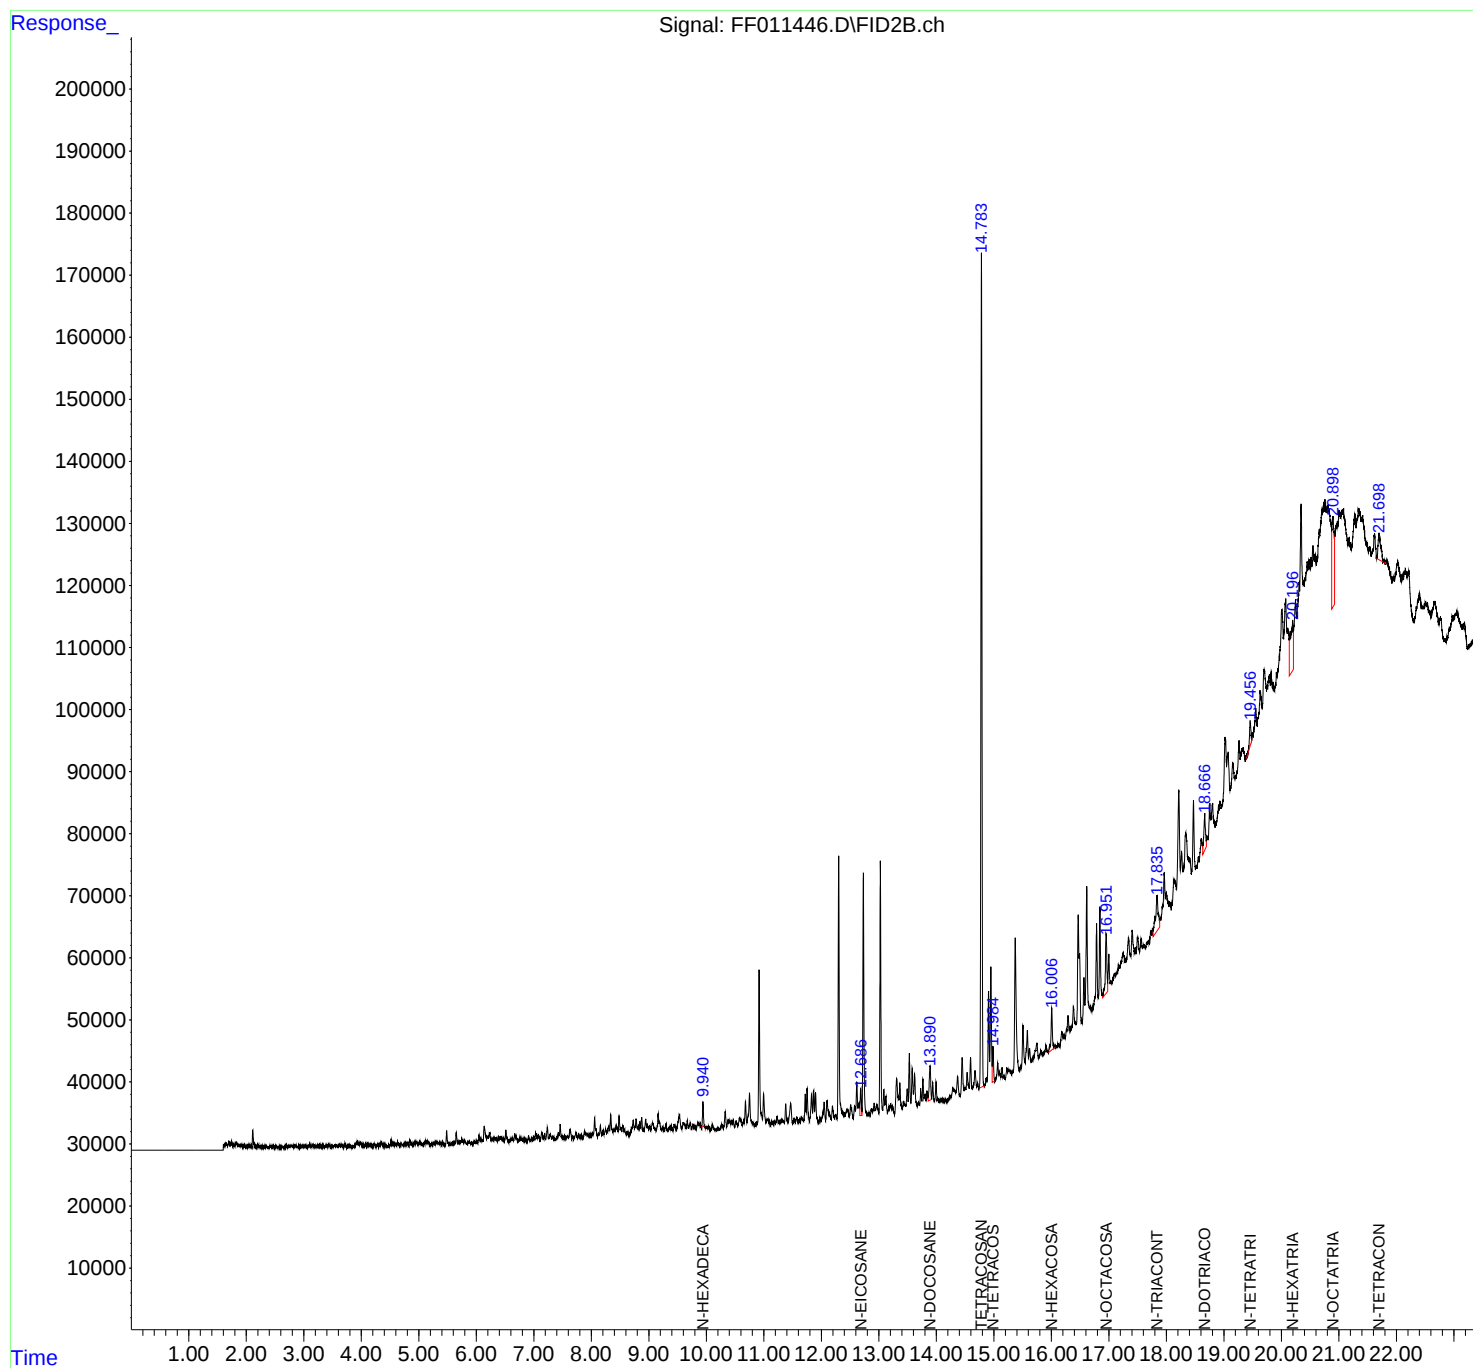


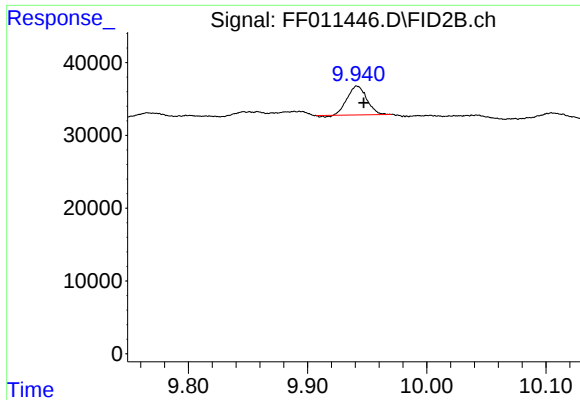

#5 N-HEXADECANE


R.T.: 9.942 min
Delta R.T.: -0.006 min
Response: 44977
Conc: 0.34 ug/ml

Instrument :
FID_F
ClientSampleId :

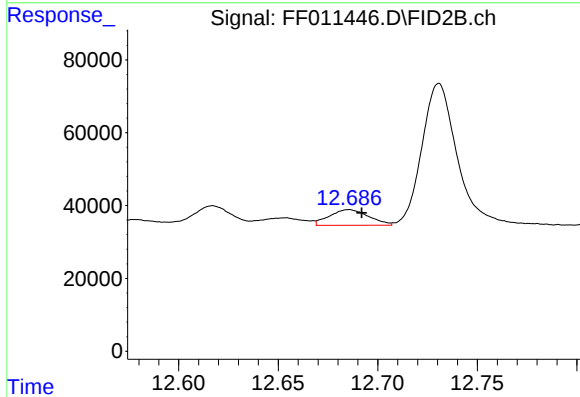


#7 N-EICOSANE

R.T.: 12.685 min
Delta R.T.: -0.007 min
Response: 59049
Conc: 0.45 ug/ml

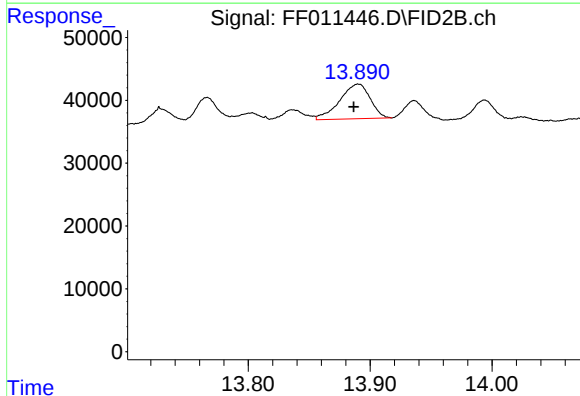


#8 N-DOCOSANE

R.T.: 13.890 min
Delta R.T.: 0.004 min
Response: 95528
Conc: 0.75 ug/ml

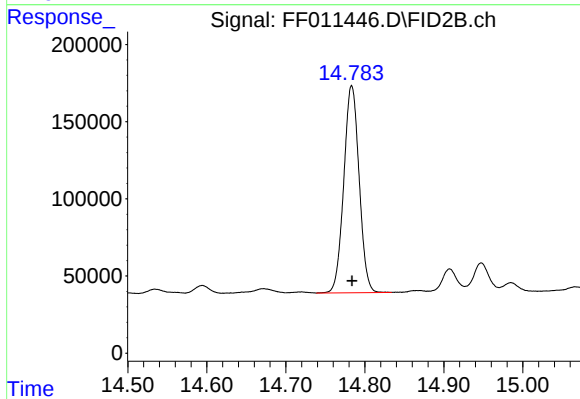

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.783 min
Delta R.T.: 0.000 min
Response: 1812977
Conc: 16.17 ug/ml

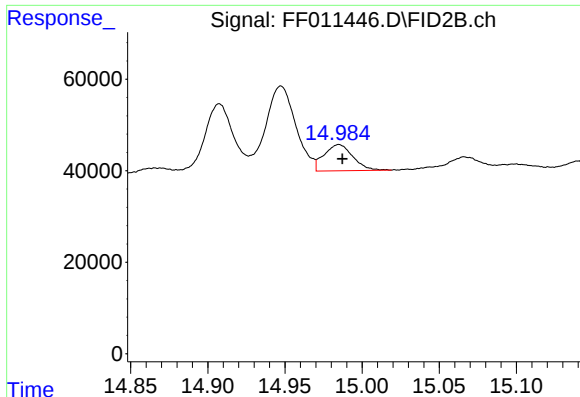

#10 N-TETRACOSANE


R.T.: 14.985 min
Delta R.T.: -0.002 min
Response: 74378
Conc: 0.58 ug/ml

Instrument :
FID_F
ClientSampleId :

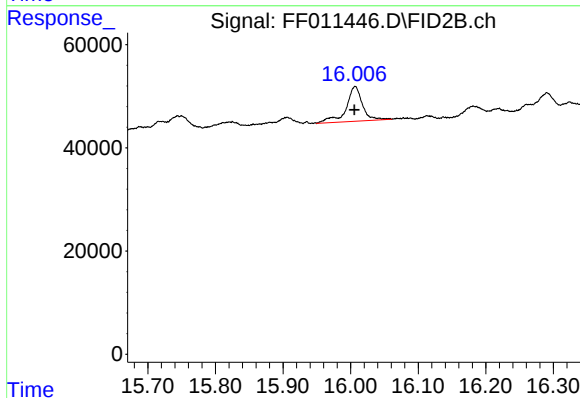


#11 N-HEXACOSANE

R.T.: 16.007 min
Delta R.T.: 0.001 min
Response: 113207
Conc: 0.91 ug/ml

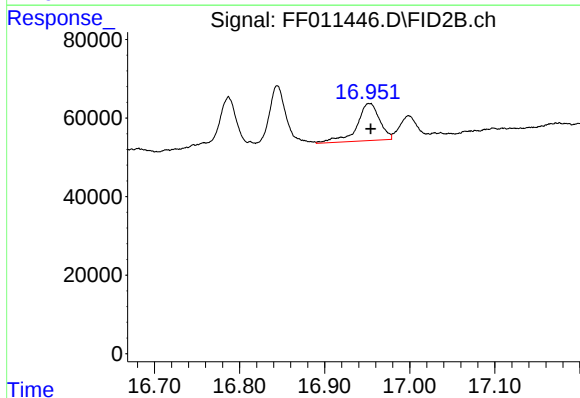


#12 N-OCTACOSANE

R.T.: 16.953 min
Delta R.T.: -0.001 min
Response: 175992
Conc: 1.44 ug/ml

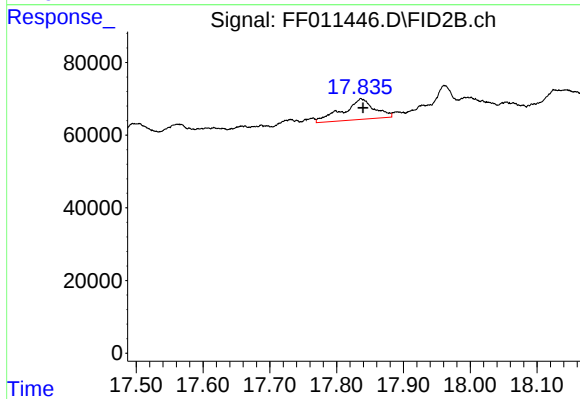

#13 N-TRIACONTANE


R.T.: 17.836 min
Delta R.T.: -0.003 min
Response: 184780
Conc: 1.53 ug/ml

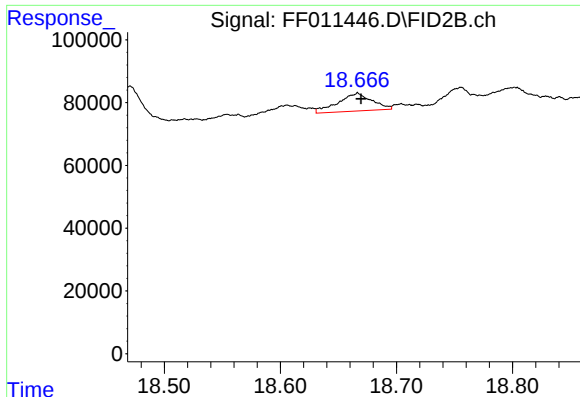

#14 N-DOTRIACONTANE


R.T.: 18.667 min
Delta R.T.: -0.003 min
Response: 115264
Conc: 0.97 ug/ml

Instrument :
FID_F
ClientSampleId :

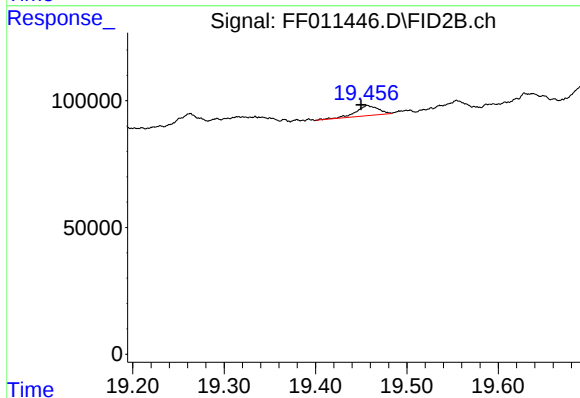


#15 N-TETRATRIACONTANE

R.T.: 19.457 min
Delta R.T.: 0.007 min
Response: 66684
Conc: 0.58 ug/ml

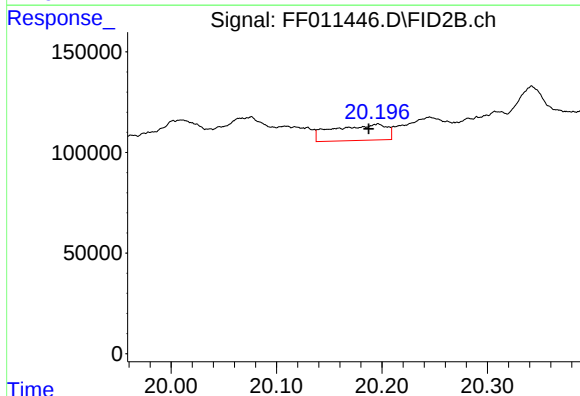


#16 N-HEXATRIACONTANE

R.T.: 20.196 min
Delta R.T.: 0.008 min
Response: 277099
Conc: 2.60 ug/ml

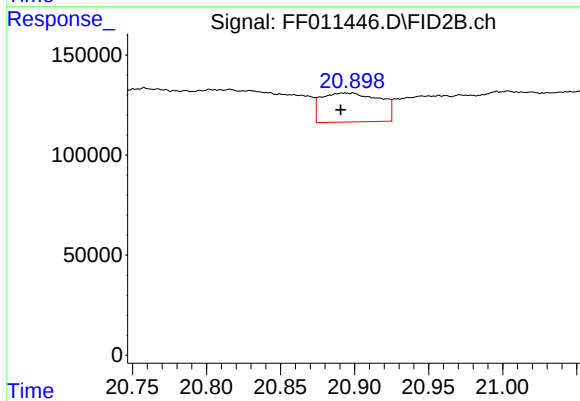

#17 N-OCTATRIACONTANE

R.T.: 20.895 min
Delta R.T.: 0.004 min
Response: 397102
Conc: 3.82 ug/ml

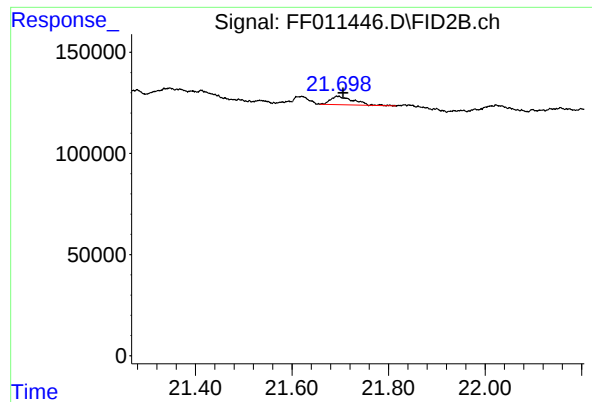

#18 N-TETRACONTANE

R.T.: 21.695 min
Delta R.T.: -0.011 min
Response: 133306
Conc: 1.26 ug/ml

Instrument :

FID_F

ClientSampleId :