

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091422\
 Data File : FF011448.D
 Signal(s) : FID2B.ch
 Acq On : 14 Sep 2022 17:50
 Operator : YP\AJ
 Sample : N4613-03
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 15 05:14:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	3445474	30.739 ug/ml
Target Compounds			
8) N-DOCOSANE	13.883	48246	0.377 ug/ml
10) N-TETRACOSANE	14.985	157601	1.238 ug/ml
11) N-HEXACOSANE	16.004	176350	1.412 ug/ml
12) N-OCTACOSANE	16.952	144121	1.177 ug/ml
13) N-TRIACONTANE	17.838	116212	0.963 ug/ml
14) N-DOTRIACONTANE	18.668	185421	1.567 ug/ml
15) N-TETRATRIACONTANE	19.452	49836	0.437 ug/ml
16) N-HEXATRIACONTANE	20.189	46305	0.435 ug/ml
17) N-OCTATRIACONTANE	20.889	392859	3.777 ug/ml
18) N-TETRACONTANE	21.711	184056	1.744 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091422\
Data File : FF011448.D
Signal(s) : FID2B.ch
Acq On : 14 Sep 2022 17:50
Operator : YP\AJ
Sample : N4613-03
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 15 05:14:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

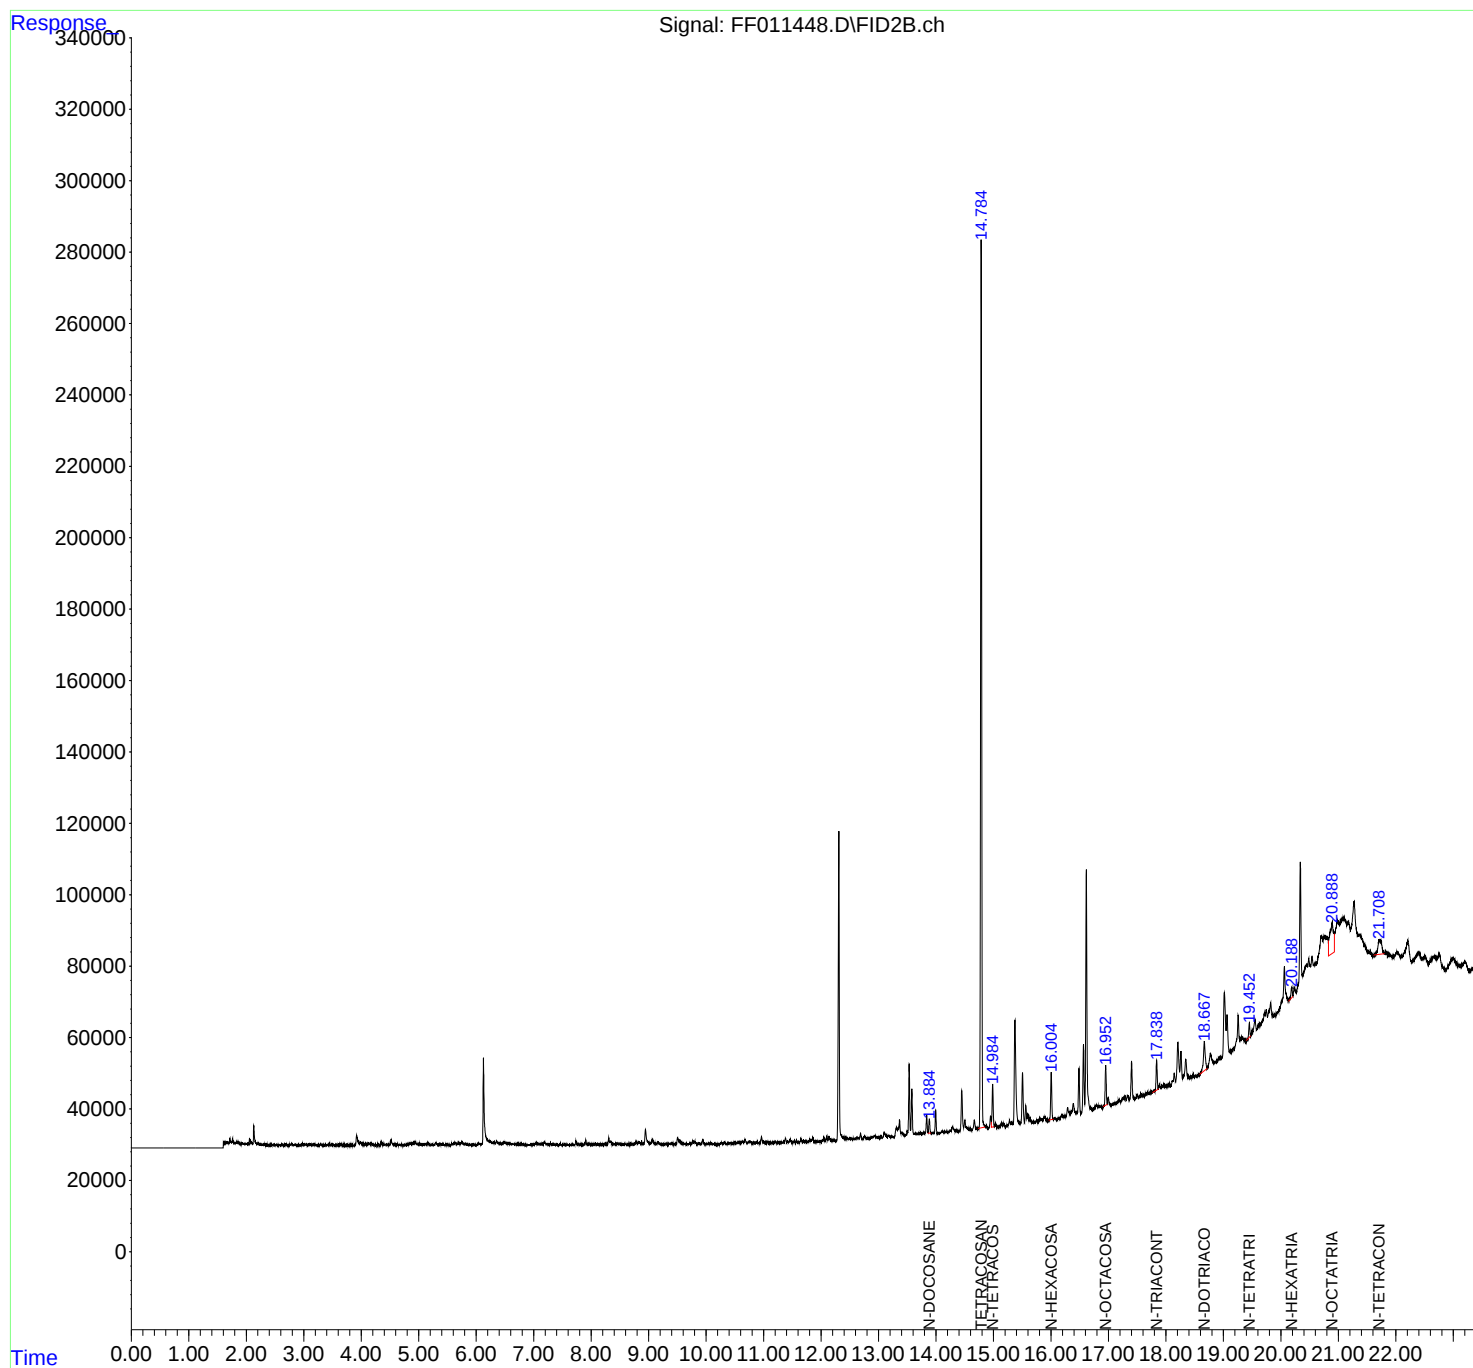


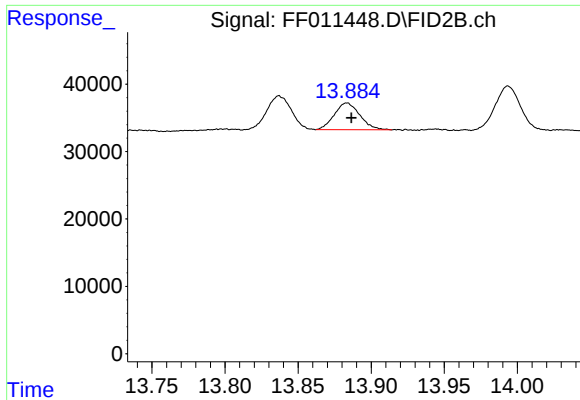

#8 N-DOCOSANE


R.T.: 13.883 min
Delta R.T.: -0.003 min
Response: 48246
Conc: 0.38 ug/ml

Instrument :
FID_F
ClientSampleId :

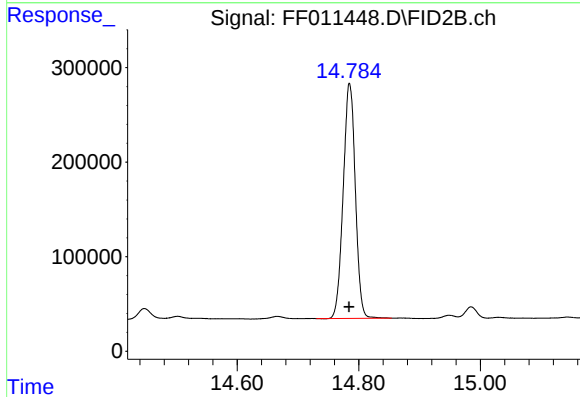


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.785 min
Delta R.T.: 0.001 min
Response: 3445474
Conc: 30.74 ug/ml

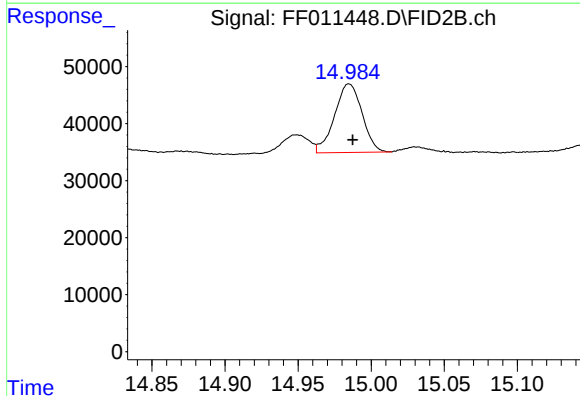


#10 N-TETRACOSANE

R.T.: 14.985 min
Delta R.T.: -0.002 min
Response: 157601
Conc: 1.24 ug/ml

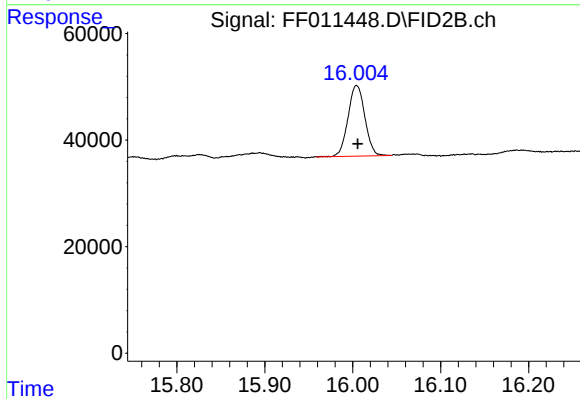

#11 N-HEXACOSANE


R.T.: 16.004 min
Delta R.T.: -0.001 min
Response: 176350
Conc: 1.41 ug/ml

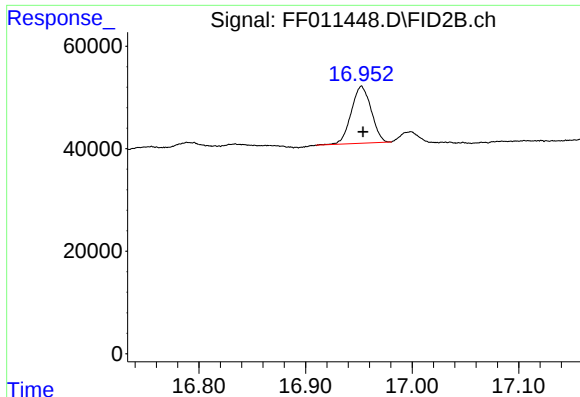

#12 N-OCTACOSANE


R.T.: 16.952 min
Delta R.T.: -0.002 min
Response: 144121
Conc: 1.18 ug/ml

Instrument :
FID_F
ClientSampleId :

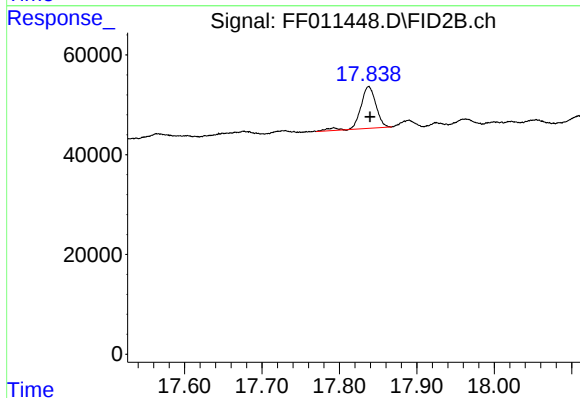


#13 N-TRIACONTANE

R.T.: 17.838 min
Delta R.T.: -0.002 min
Response: 116212
Conc: 0.96 ug/ml

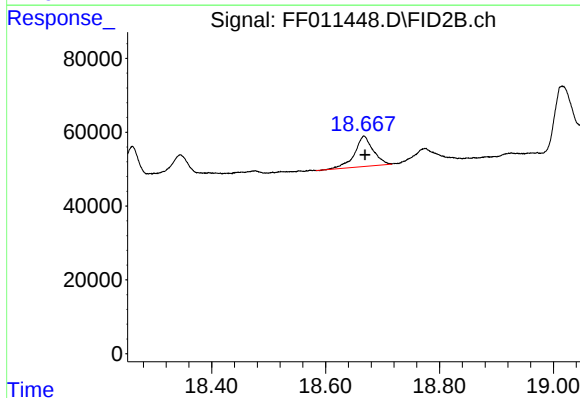


#14 N-DOTRIACONTANE

R.T.: 18.668 min
Delta R.T.: -0.002 min
Response: 185421
Conc: 1.57 ug/ml

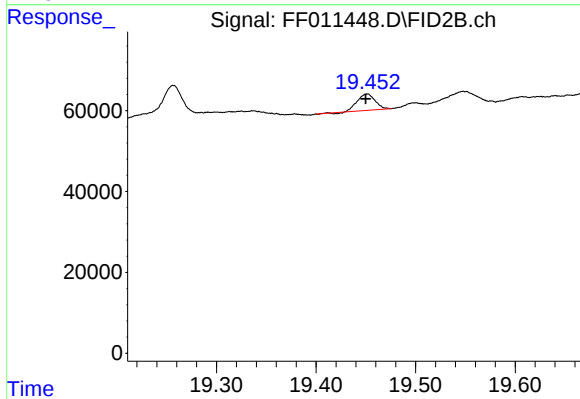

#15 N-TETRATRIACONTANE


R.T.: 19.452 min
Delta R.T.: 0.002 min
Response: 49836
Conc: 0.44 ug/ml

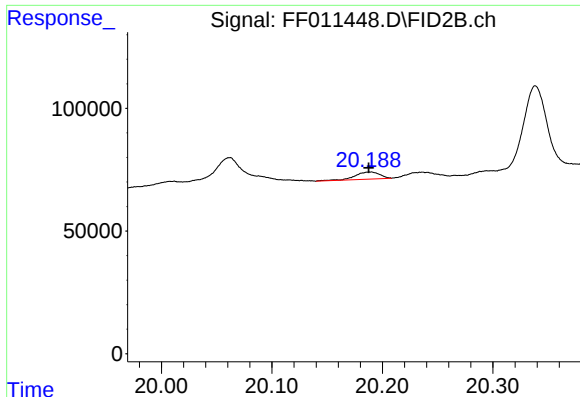

#16 N-HEXATRIACONTANE


R.T.: 20.189 min
Delta R.T.: 0.002 min
Response: 46305
Conc: 0.44 ug/ml

Instrument :
FID_F
ClientSampleId :

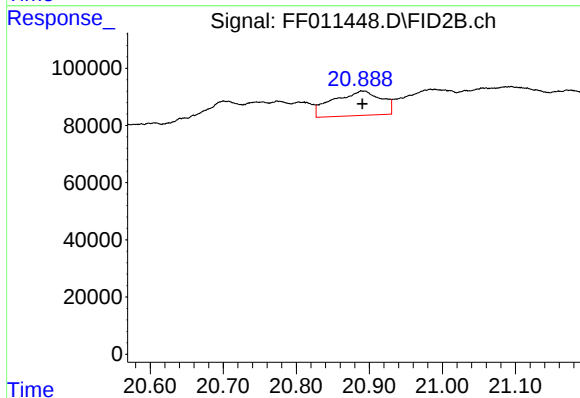

#17 N-OCTATRIACONTANE

R.T.: 20.889 min
Delta R.T.: -0.001 min
Response: 392859
Conc: 3.78 ug/ml

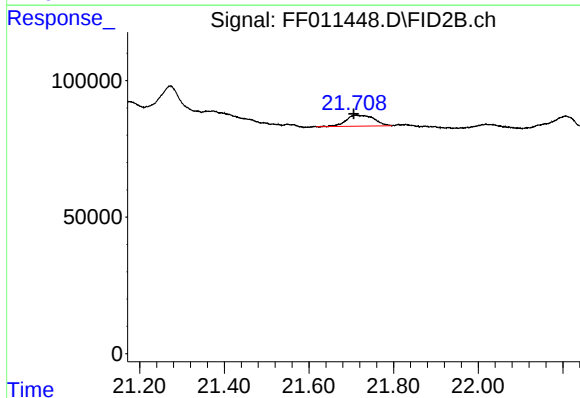

#18 N-TETRACONTANE

R.T.: 21.711 min
Delta R.T.: 0.005 min
Response: 184056
Conc: 1.74 ug/ml