

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091422\
 Data File : FF011449.D
 Signal(s) : FID2B.ch
 Acq On : 14 Sep 2022 18:50
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 15 05:14:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.782	2070003	18.467 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.838	105350	0.873 ug/ml
14) N-DOTRIACONTANE	18.668	159398	1.347 ug/ml
15) N-TETRATRIACONTANE	19.449	116998	1.025 ug/ml
16) N-HEXATRIACONTANE	20.189	25801	0.242 ug/ml
17) N-OCTATRIACONTANE	20.893	179986	1.730 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091422\
Data File : FF011449.D
Signal(s) : FID2B.ch
Acq On : 14 Sep 2022 18:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 15 05:14:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

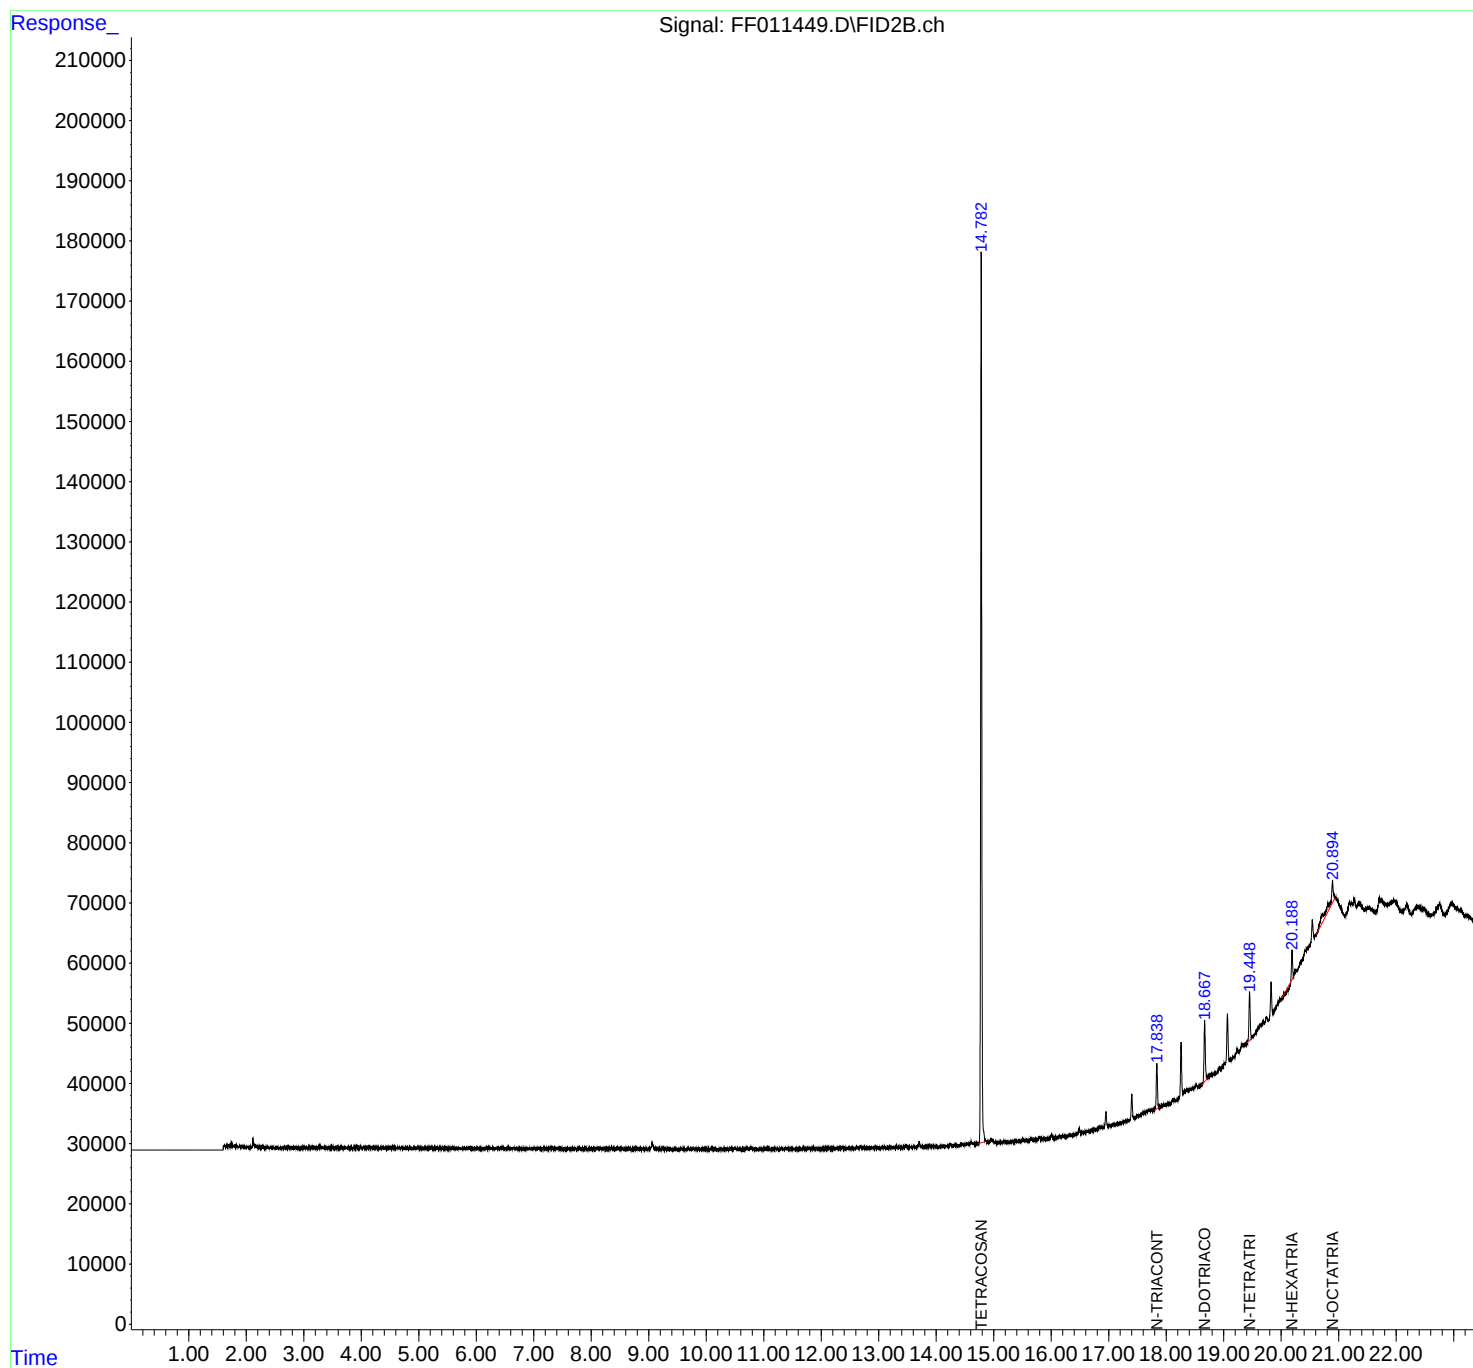


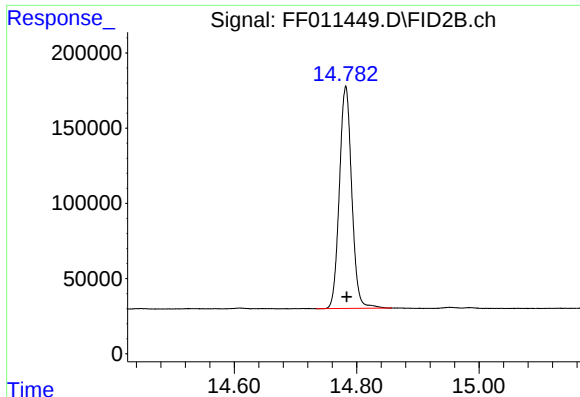

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.782 min
Delta R.T.: -0.001 min
Response: 2070003
Conc: 18.47 ug/ml

Instrument :
FID_F
ClientSampleId :

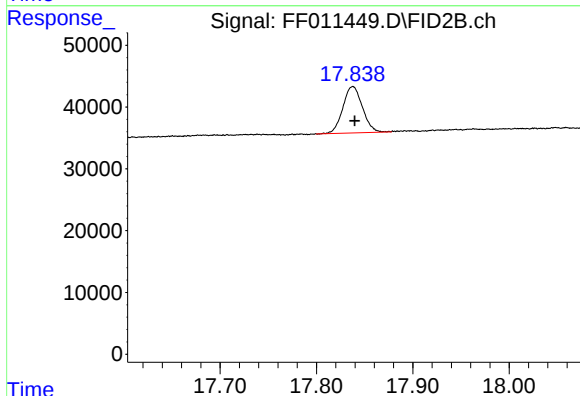


#13 N-TRIACONTANE

R.T.: 17.838 min
Delta R.T.: -0.002 min
Response: 105350
Conc: 0.87 ug/ml

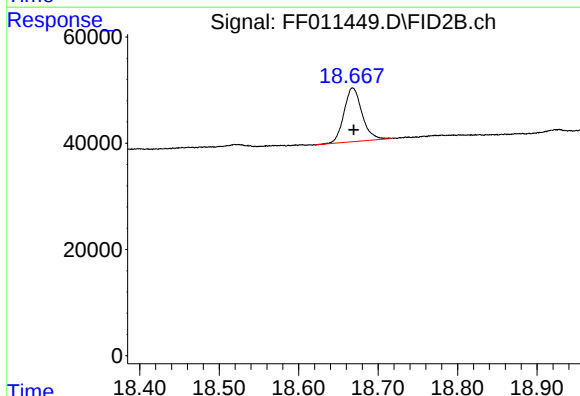


#14 N-DOTRIACONTANE

R.T.: 18.668 min
Delta R.T.: -0.002 min
Response: 159398
Conc: 1.35 ug/ml

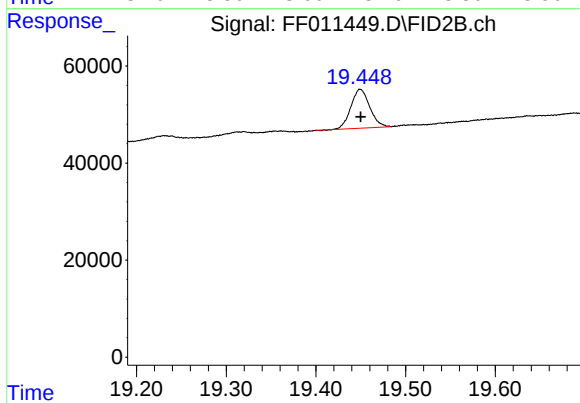

#15 N-TETRATRIACONTANE


R.T.: 19.449 min
Delta R.T.: 0.000 min
Response: 116998
Conc: 1.02 ug/ml

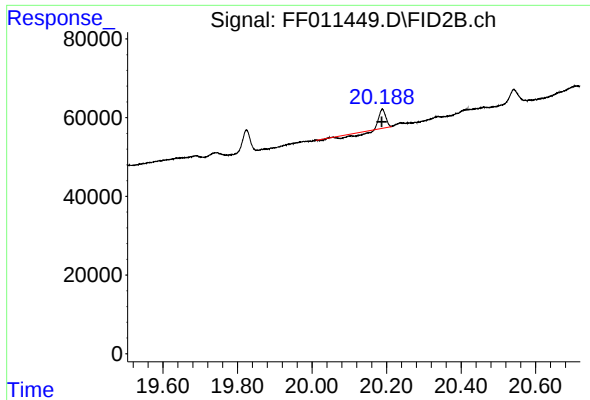

#16 N-HEXATRIACONTANE

R.T.: 20.189 min
Delta R.T.: 0.001 min
Response: 25801
Conc: 0.24 ug/ml

Instrument :
FID_F
ClientSampleId :

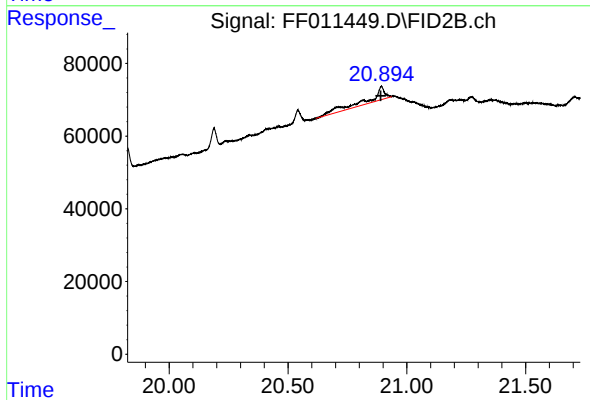

#17 N-OCTATRIACONTANE

R.T.: 20.893 min
Delta R.T.: 0.003 min
Response: 179986
Conc: 1.73 ug/ml