

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091422\
Data File : FF011446.D
Signal(s) : FID2B.ch
Acq On : 14 Sep 2022 16:51
Operator : YP\AJ
Sample : N4613-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SASP2-T-6-(10-18)

Integration File: autoint1.e
Quant Time: Sep 15 05:14:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	1812977	16.174 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091422\
Data File : FF011446.D
Signal(s) : FID2B.ch
Acq On : 14 Sep 2022 16:51
Operator : YP\AJ
Sample : N4613-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SASP2-T-6-(10-18)

Integration File: autoint1.e
Quant Time: Sep 15 05:14:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

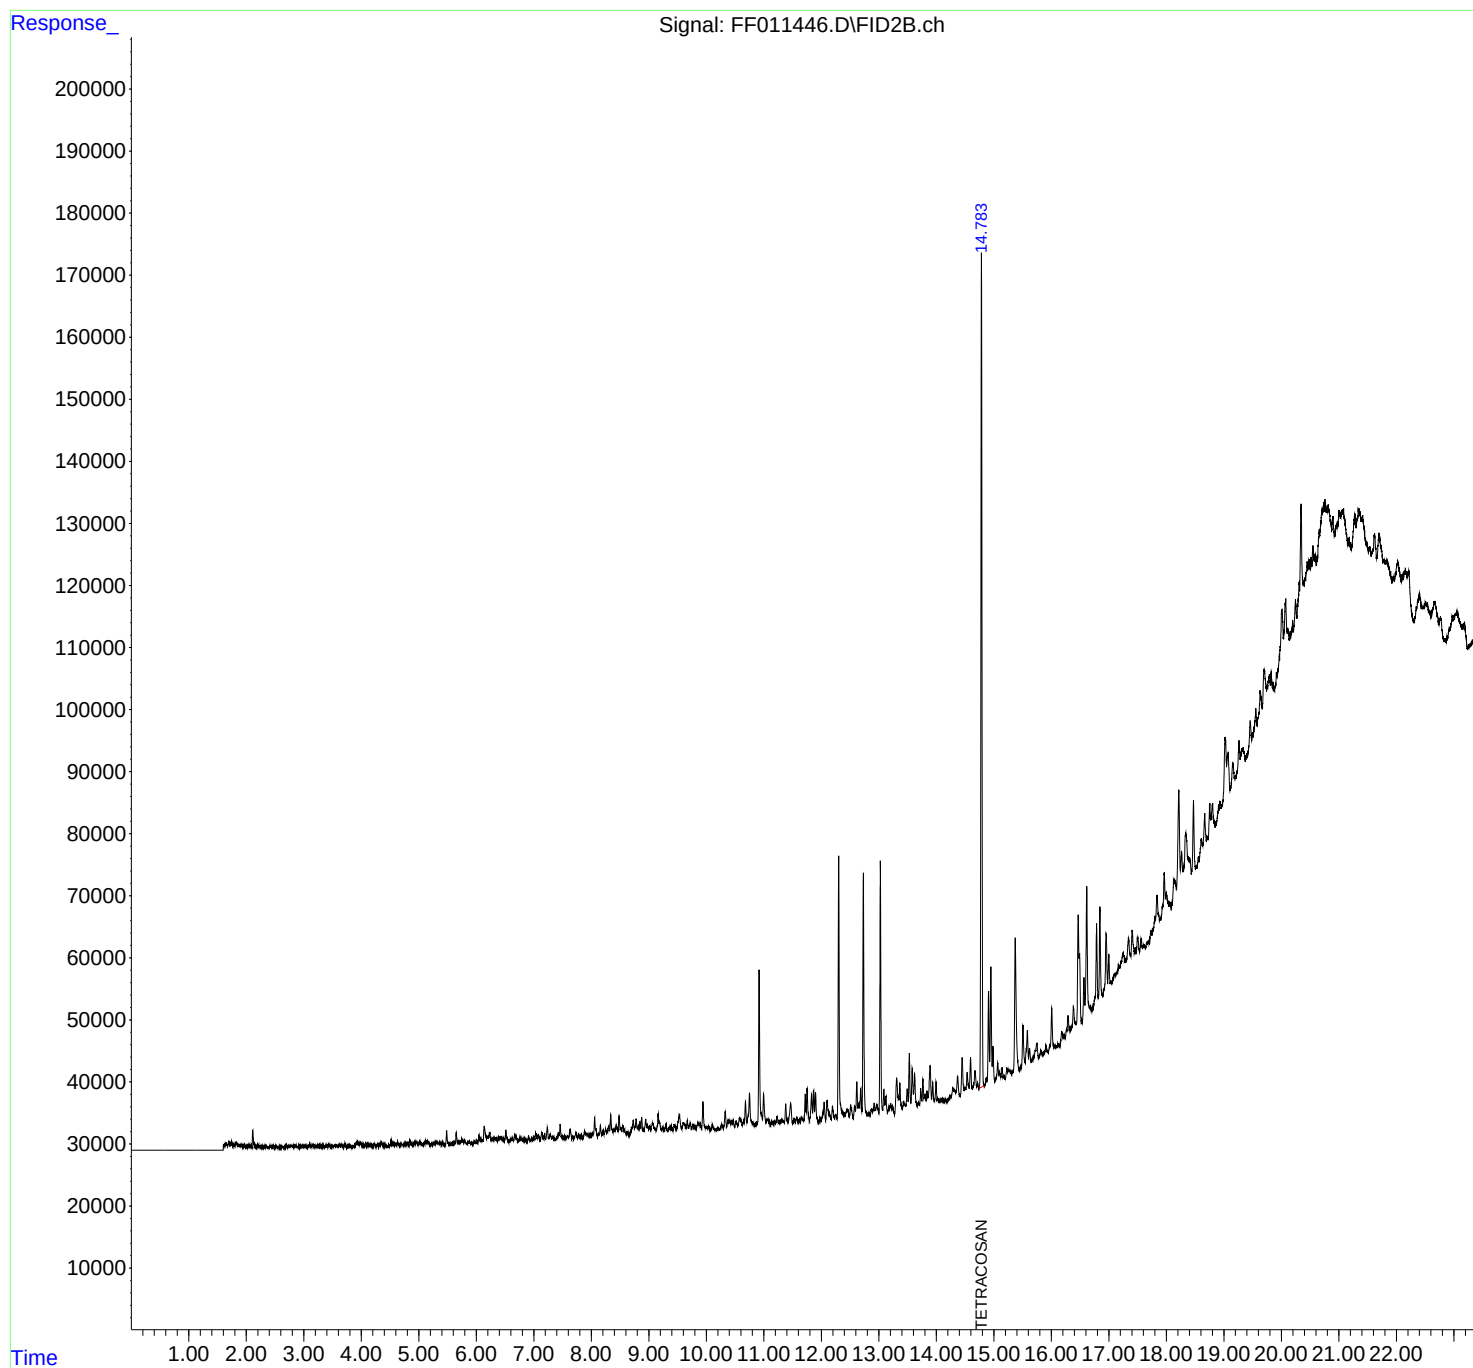

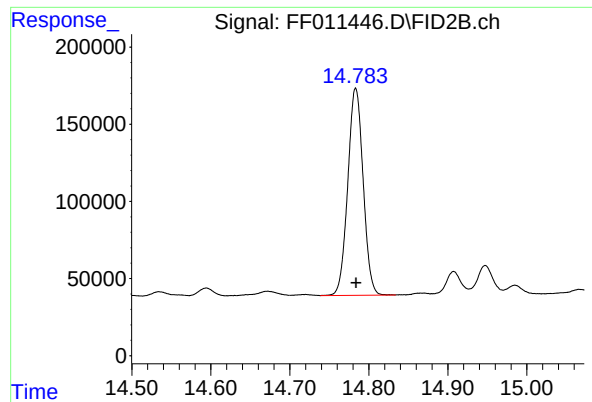

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.783 min
Delta R.T.: 0.000 min
Response: 1812977
Conc: 16.17 ug/ml

Instrument :
FID_F
ClientSampleId :
SASP2-T-6-(10-18)