

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
Data File : FF011451.D
Signal(s) : FID2B.ch
Acq On : 15 Sep 2022 10:16
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 03:29:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7)	N-EICOSANE	12.671	81771	0.622 ug/ml
8)	N-DOCOSANE	13.877	76317	0.597 ug/ml
10)	N-TETRACOSANE	14.981	58849	0.462 ug/ml
11)	N-HEXACOSANE	16.001	50115	0.401 ug/ml
12)	N-OCTACOSANE	16.949	67369	0.550 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
Data File : FF011451.D
Signal(s) : FID2B.ch
Acq On : 15 Sep 2022 10:16
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 03:29:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

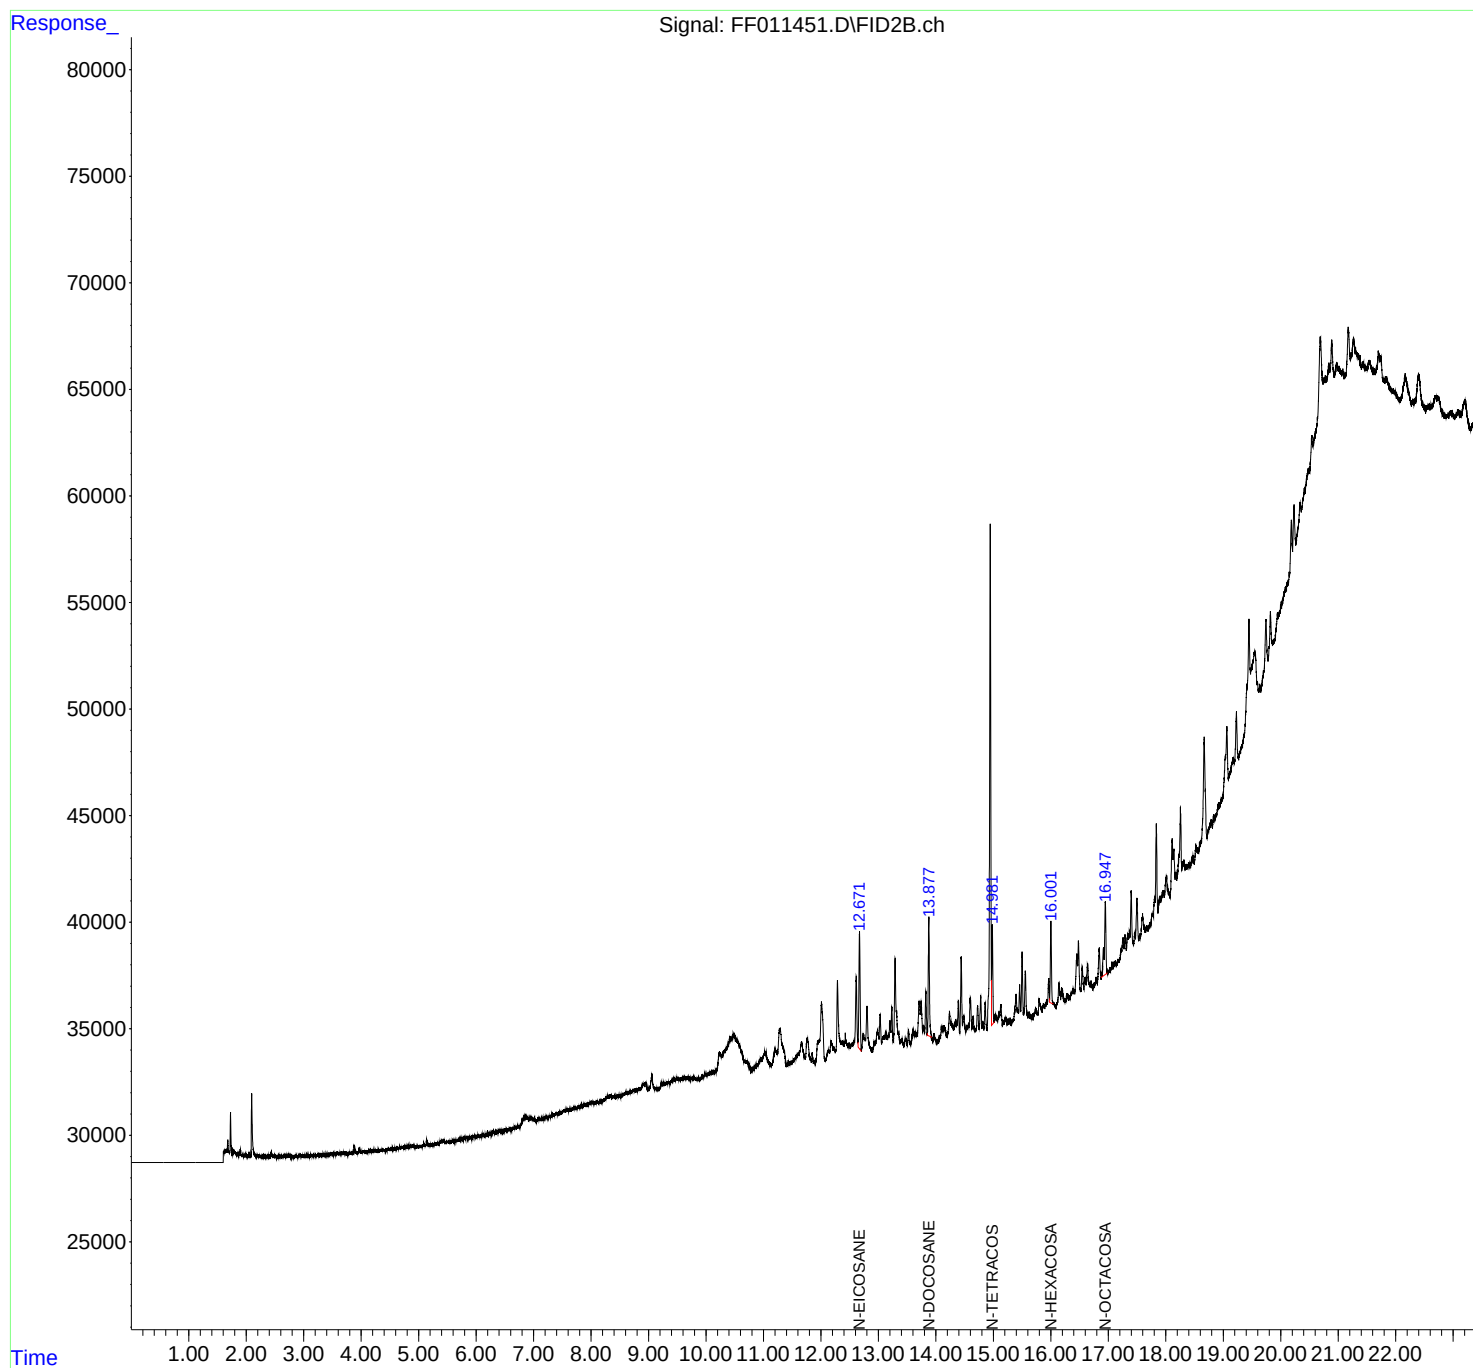


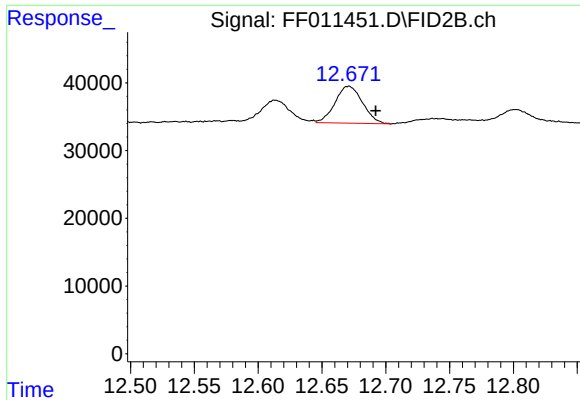

#7 N-EICOSANE


R.T.: 12.671 min
Delta R.T.: -0.021 min
Response: 81771
Conc: 0.62 ug/ml

Instrument :
FID_F
ClientSampleId :

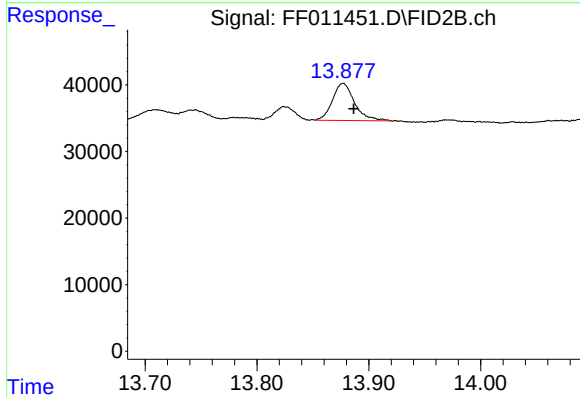


#8 N-DOCOSANE

R.T.: 13.877 min
Delta R.T.: -0.010 min
Response: 76317
Conc: 0.60 ug/ml

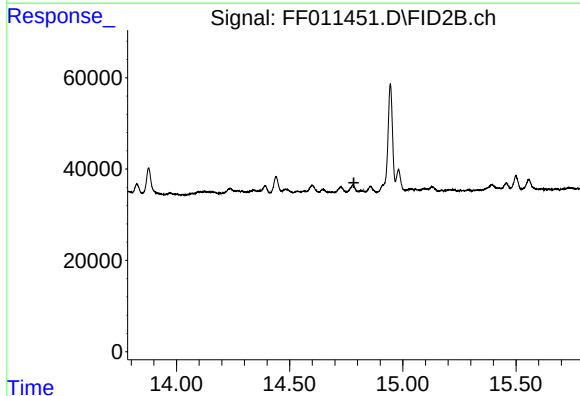


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.784 min
Response: 0
Conc: N.D.

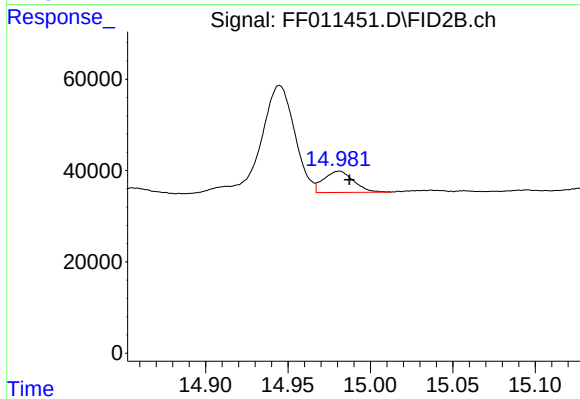

#10 N-TETRACOSANE


R.T.: 14.981 min
Delta R.T.: -0.006 min
Response: 58849
Conc: 0.46 ug/ml

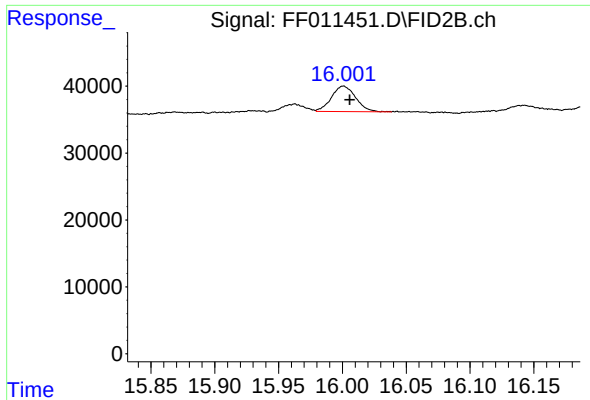

#11 N-HEXACOSANE

R.T.: 16.001 min
Delta R.T.: -0.005 min
Response: 50115
Conc: 0.40 ug/ml

Instrument :
FID_F
ClientSampleId :

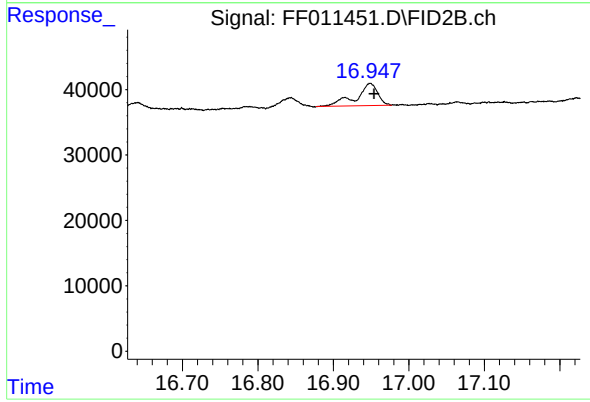

#12 N-OCTACOSANE

R.T.: 16.949 min
Delta R.T.: -0.005 min
Response: 67369
Conc: 0.55 ug/ml