

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
Data File : FF011455.D
Signal(s) : FID2B.ch
Acq On : 15 Sep 2022 12:14
Operator : YP\AJ
Sample : N4597-02 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 03:30:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	377483	3.368 ug/ml
Target Compounds			
7) N-EICOSANE	12.729	1434126	10.903 ug/ml
8) N-DOCOSANE	13.891	137908	1.079 ug/ml
10) N-TETRACOSANE	14.944	707189	5.554 ug/ml
12) N-OCTACOSANE	16.945	176666	1.442 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
Data File : FF011455.D
Signal(s) : FID2B.ch
Acq On : 15 Sep 2022 12:14
Operator : YP\AJ
Sample : N4597-02 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 03:30:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

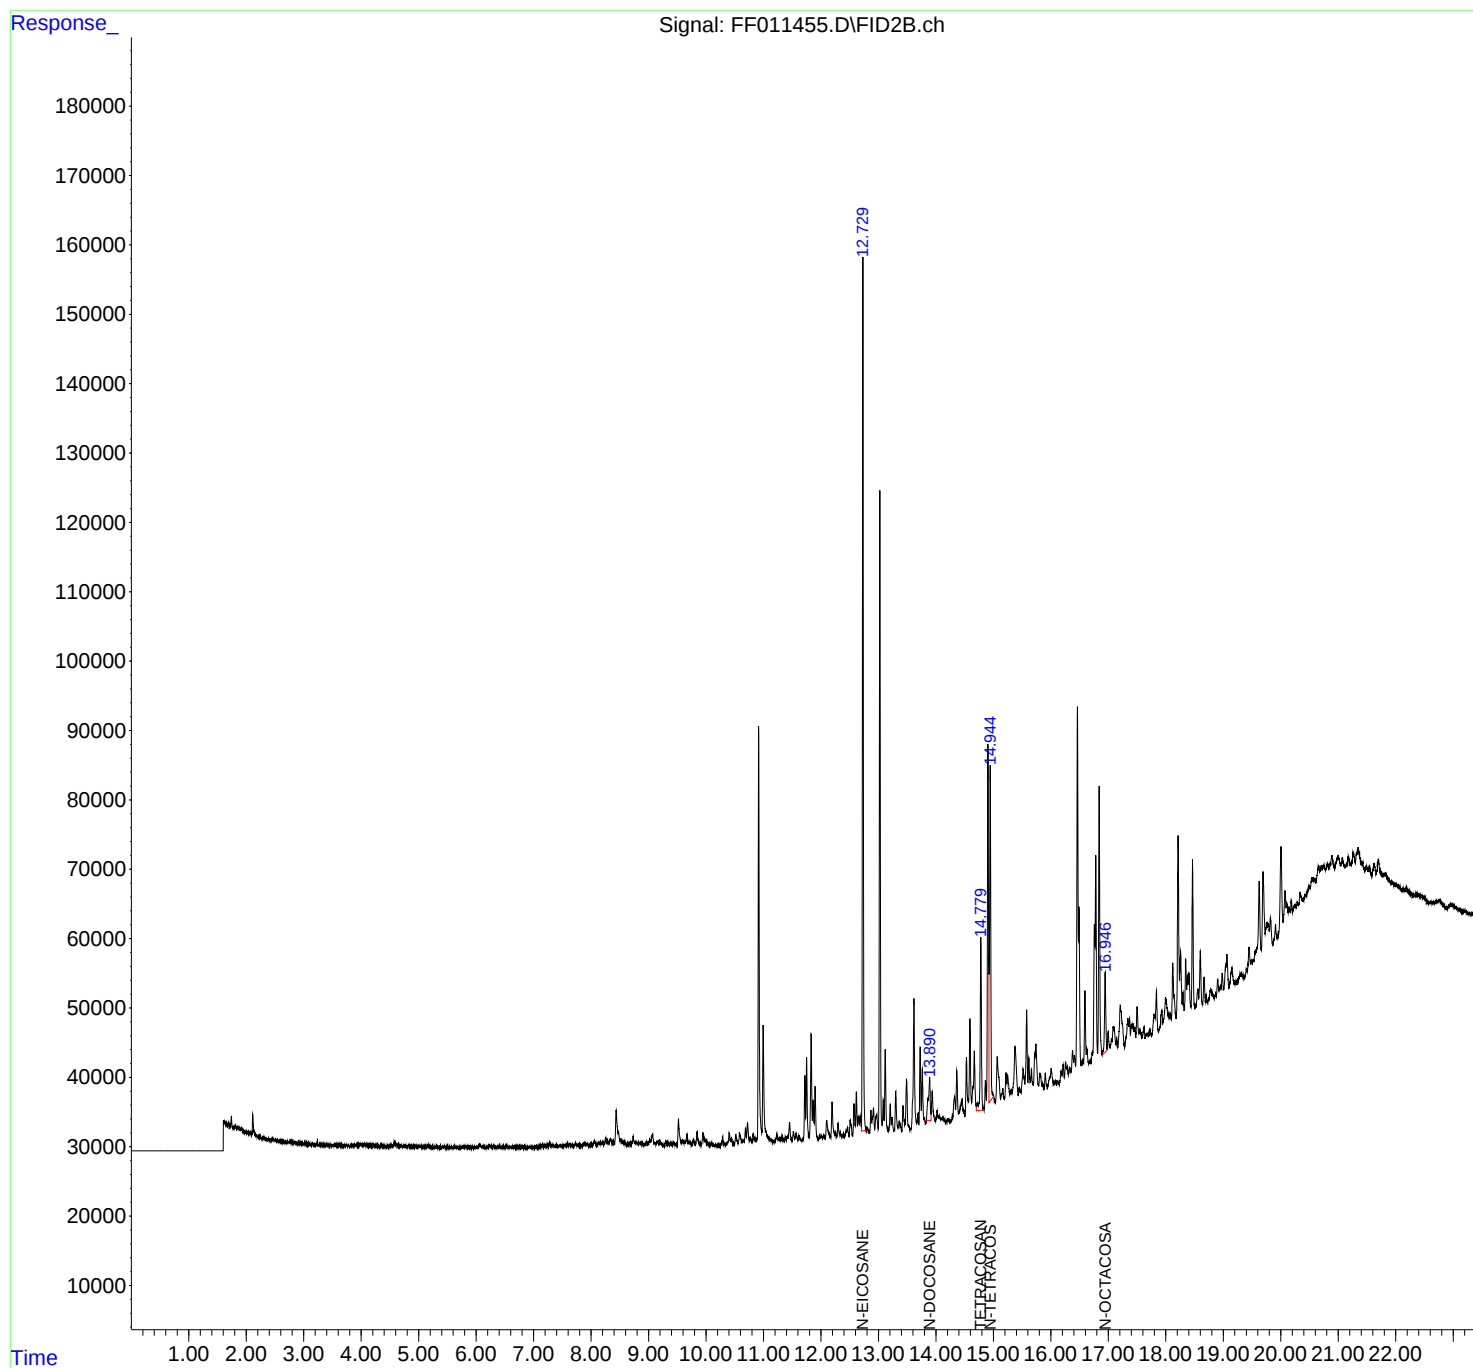


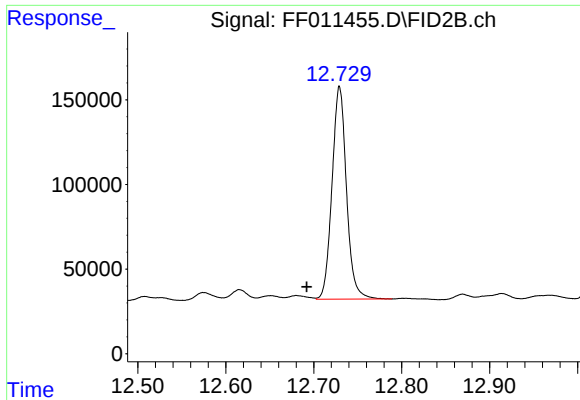

#7 N-EICOSANE


R.T.: 12.729 min
Delta R.T.: 0.037 min
Response: 1434126
Conc: 10.90 ug/ml

Instrument :
FID_F
ClientSampleId :

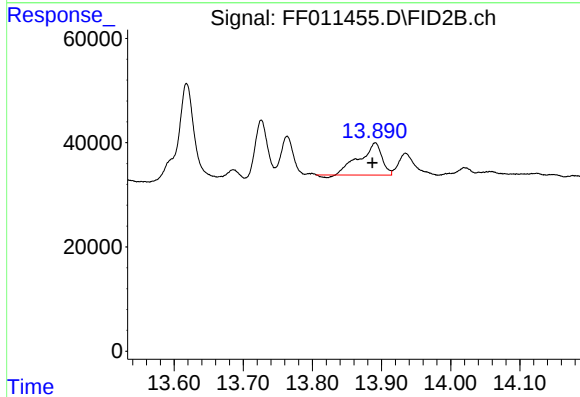


#8 N-DOCOSANE

R.T.: 13.891 min
Delta R.T.: 0.004 min
Response: 137908
Conc: 1.08 ug/ml

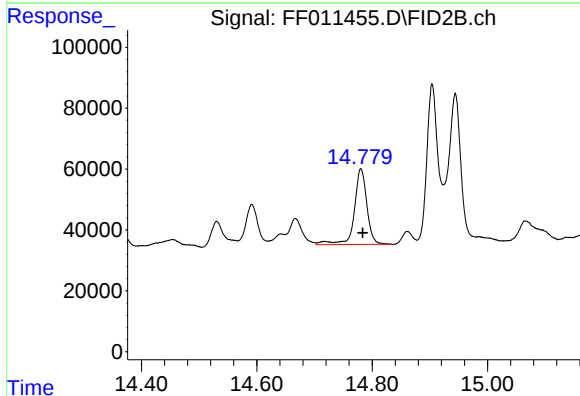


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.780 min
Delta R.T.: -0.003 min
Response: 377483
Conc: 3.37 ug/ml

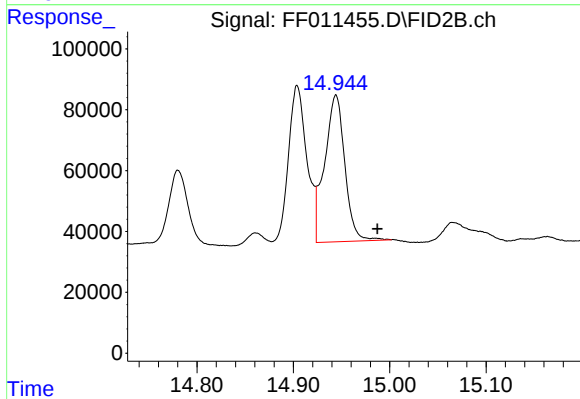

#10 N-TETRACOSANE

R.T.: 14.944 min
Delta R.T.: -0.043 min
Response: 707189
Conc: 5.55 ug/ml

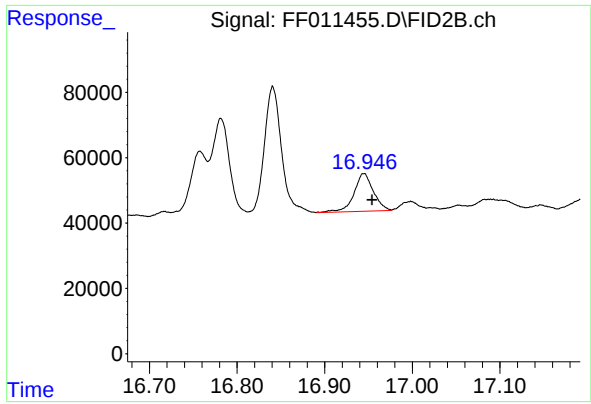

#12 N-OCTACOSANE

R.T.: 16.945 min
Delta R.T.: -0.009 min
Response: 176666
Conc: 1.44 ug/ml

Instrument :

FID_F

ClientSampleId :