

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
 Data File : FF011457.D
 Signal(s) : FID2B.ch
 Acq On : 15 Sep 2022 13:13
 Operator : YP\AJ
 Sample : N4597-06 2X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 16 03:30:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.781	843654	7.527 ug/ml
Target Compounds			
6) N-OCTADECANE	11.453f	83932	0.631 ug/ml
7) N-EICOSANE	12.681	104976	0.798 ug/ml
8) N-DOCOSANE	13.891	292659	2.290 ug/ml
10) N-TETRACOSANE	14.945	1383449	10.865 ug/ml
11) N-HEXACOSANE	16.007	160502	1.285 ug/ml
12) N-OCTACOSANE	16.944	436383	3.563 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
Data File : FF011457.D
Signal(s) : FID2B.ch
Acq On : 15 Sep 2022 13:13
Operator : YP\AJ
Sample : N4597-06 2X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 03:30:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

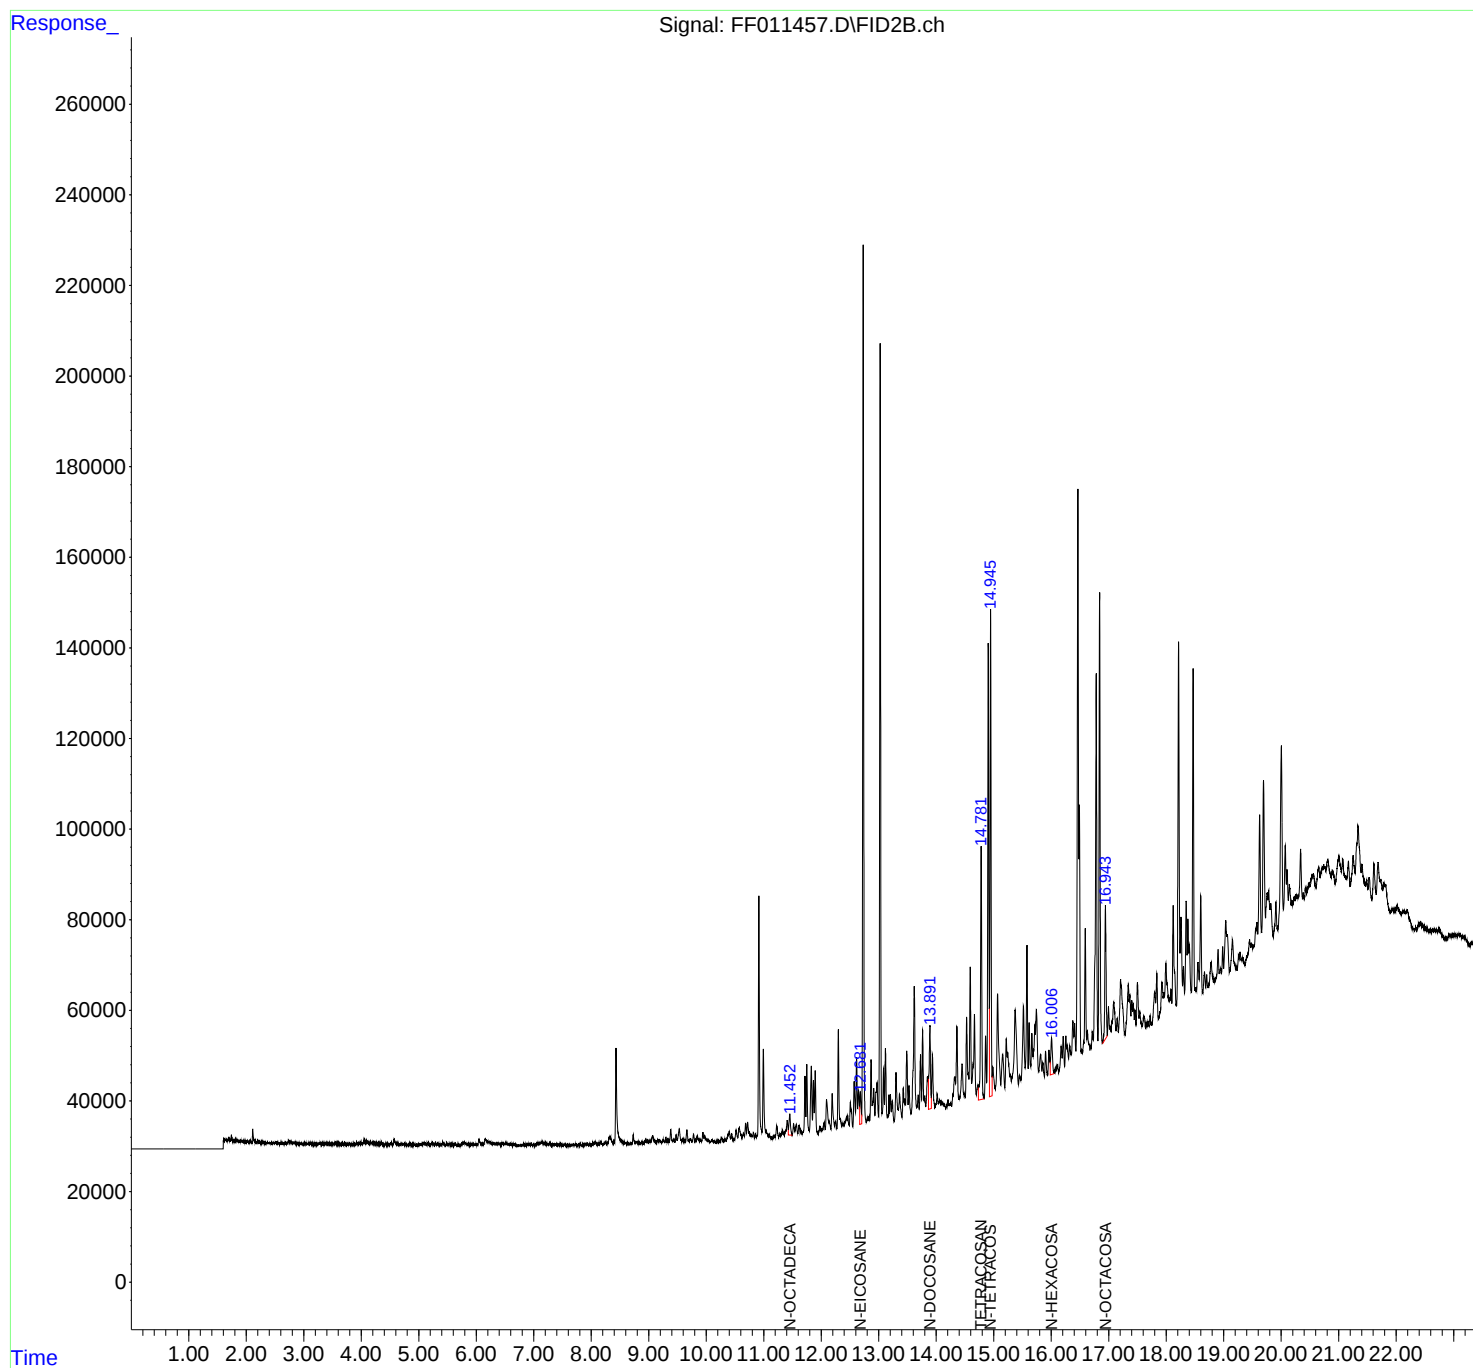


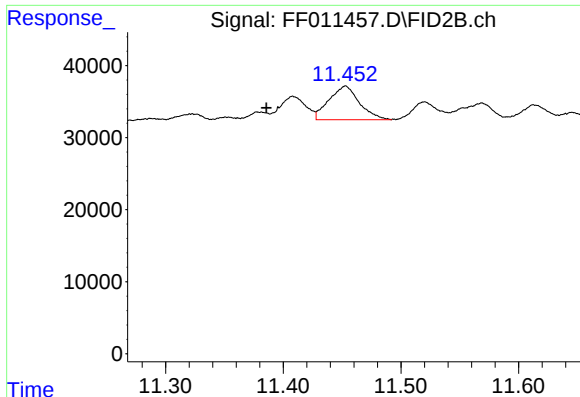

#6 N-OCTADECANE


R.T.: 11.453 min
Delta R.T.: 0.067 min
Response: 83932
Conc: 0.63 ug/ml

Instrument :
FID_F
ClientSampleId :

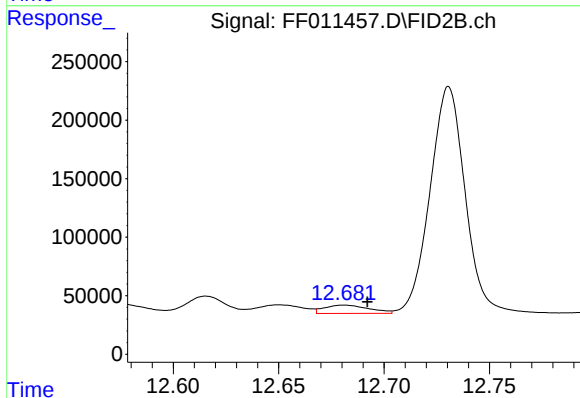


#7 N-EICOSANE

R.T.: 12.681 min
Delta R.T.: -0.011 min
Response: 104976
Conc: 0.80 ug/ml

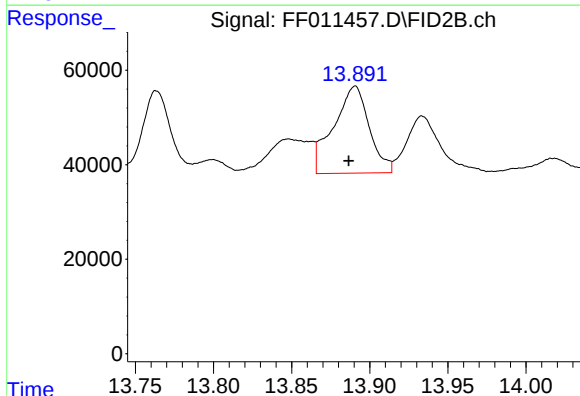


#8 N-DOCOSANE

R.T.: 13.891 min
Delta R.T.: 0.004 min
Response: 292659
Conc: 2.29 ug/ml

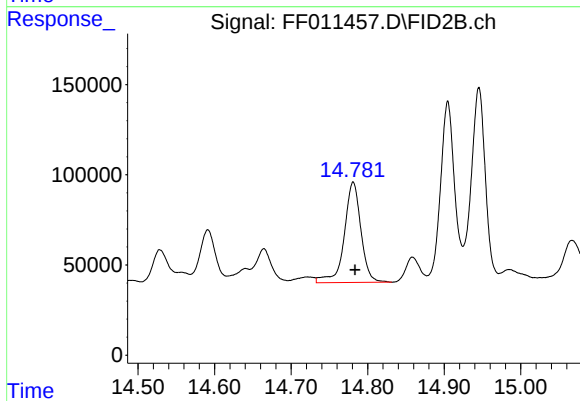

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.781 min
Delta R.T.: -0.003 min
Response: 843654
Conc: 7.53 ug/ml

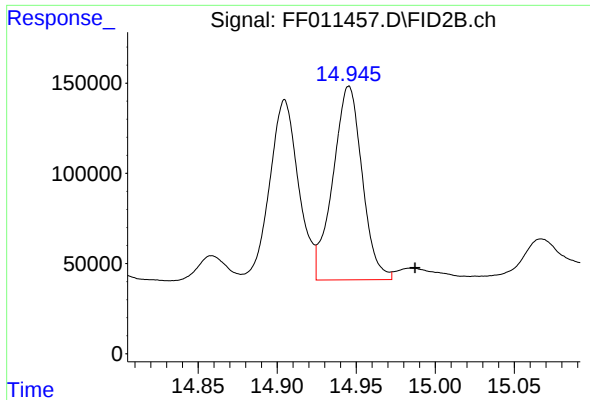

#10 N-TETRACOSANE


R.T.: 14.945 min
Delta R.T.: -0.042 min
Response: 1383449
Conc: 10.87 ug/ml

Instrument :
FID_F
ClientSampleId :

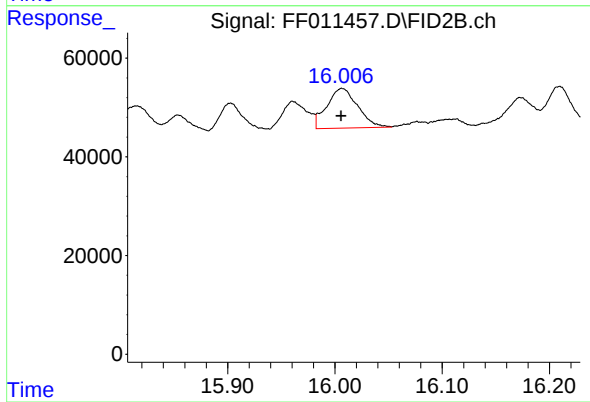

#11 N-HEXACOSANE

R.T.: 16.007 min
Delta R.T.: 0.000 min
Response: 160502
Conc: 1.29 ug/ml

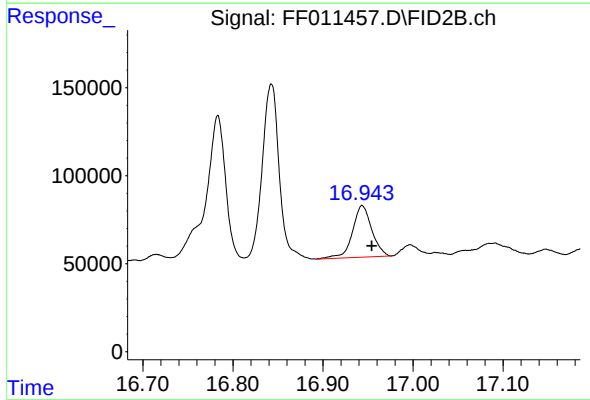

#12 N-OCTACOSANE

R.T.: 16.944 min
Delta R.T.: -0.010 min
Response: 436383
Conc: 3.56 ug/ml