

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
 Data File : FF011458.D
 Signal(s) : FID2B.ch
 Acq On : 15 Sep 2022 13:43
 Operator : YP\AJ
 Sample : N4613-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 16 03:30:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.782	1975512	17.624 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.984	91493	0.719 ug/ml
11) N-HEXACOSANE	16.003	102227	0.818 ug/ml
12) N-OCTACOSANE	16.951	81814	0.668 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
Data File : FF011458.D
Signal(s) : FID2B.ch
Acq On : 15 Sep 2022 13:43
Operator : YP\AJ
Sample : N4613-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 03:30:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

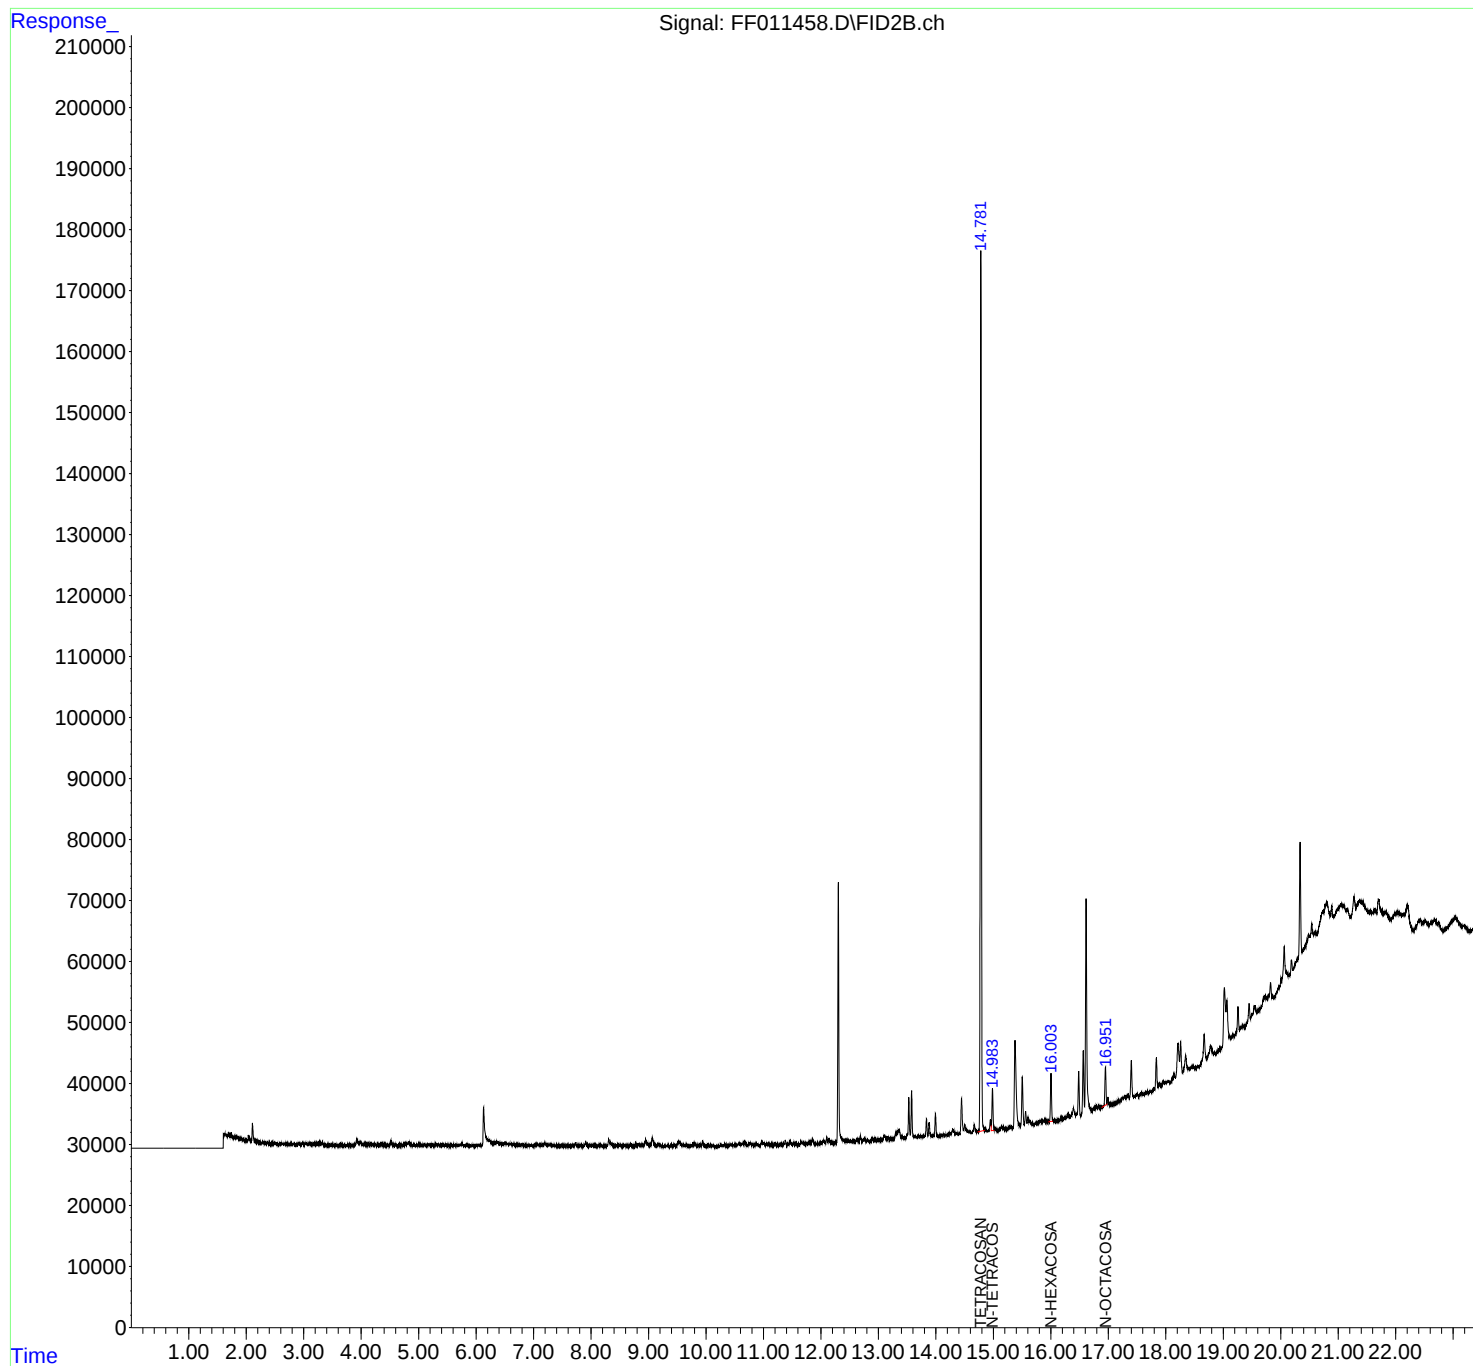


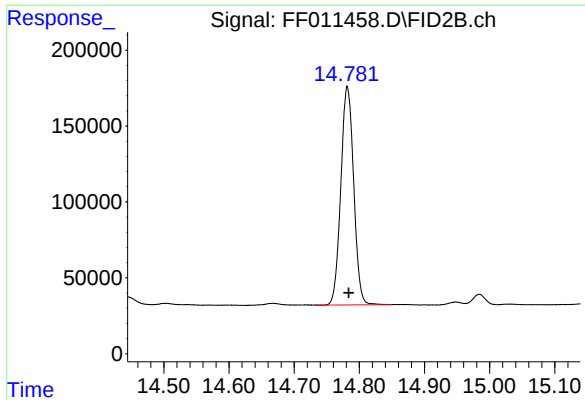

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.782 min
Delta R.T.: -0.002 min
Response: 1975512
Conc: 17.62 ug/ml

Instrument :
FID_F
ClientSampleId :

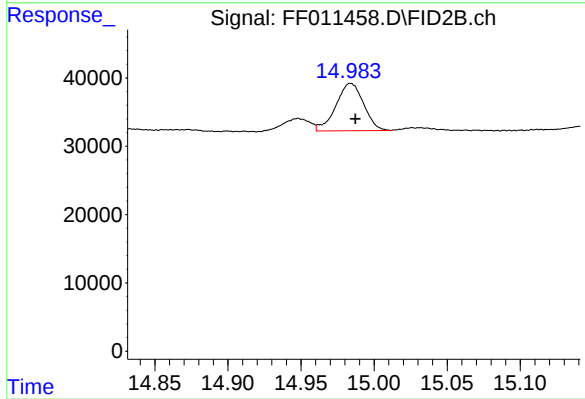


#10 N-TETRACOSANE

R.T.: 14.984 min
Delta R.T.: -0.003 min
Response: 91493
Conc: 0.72 ug/ml

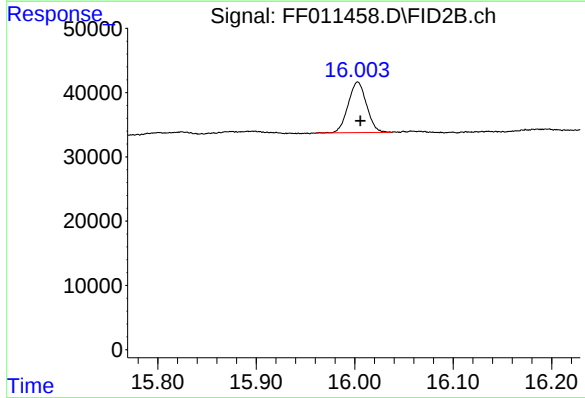

#11 N-HEXACOSANE

R.T.: 16.003 min
Delta R.T.: -0.003 min
Response: 102227
Conc: 0.82 ug/ml

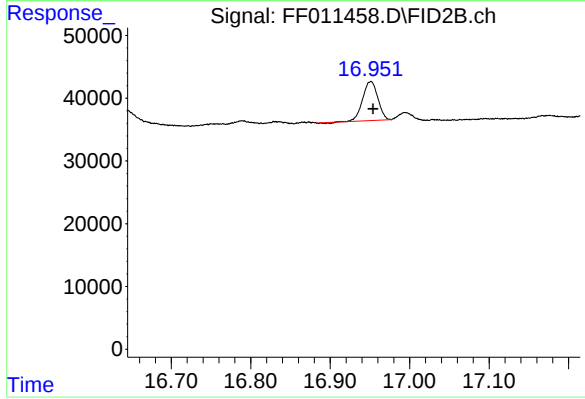

#12 N-OCTACOSANE

R.T.: 16.951 min
Delta R.T.: -0.003 min
Response: 81814
Conc: 0.67 ug/ml