

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
Data File : FF011467.D
Signal(s) : FID2B.ch
Acq On : 15 Sep 2022 20:16
Operator : YP\AJ
Sample : N4630-19 125X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 03:31:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.951	37783	0.297 ug/ml
12)	N-OCTACOSANE	16.954	79590	0.650 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
Data File : FF011467.D
Signal(s) : FID2B.ch
Acq On : 15 Sep 2022 20:16
Operator : YP\AJ
Sample : N4630-19 125X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 03:31:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

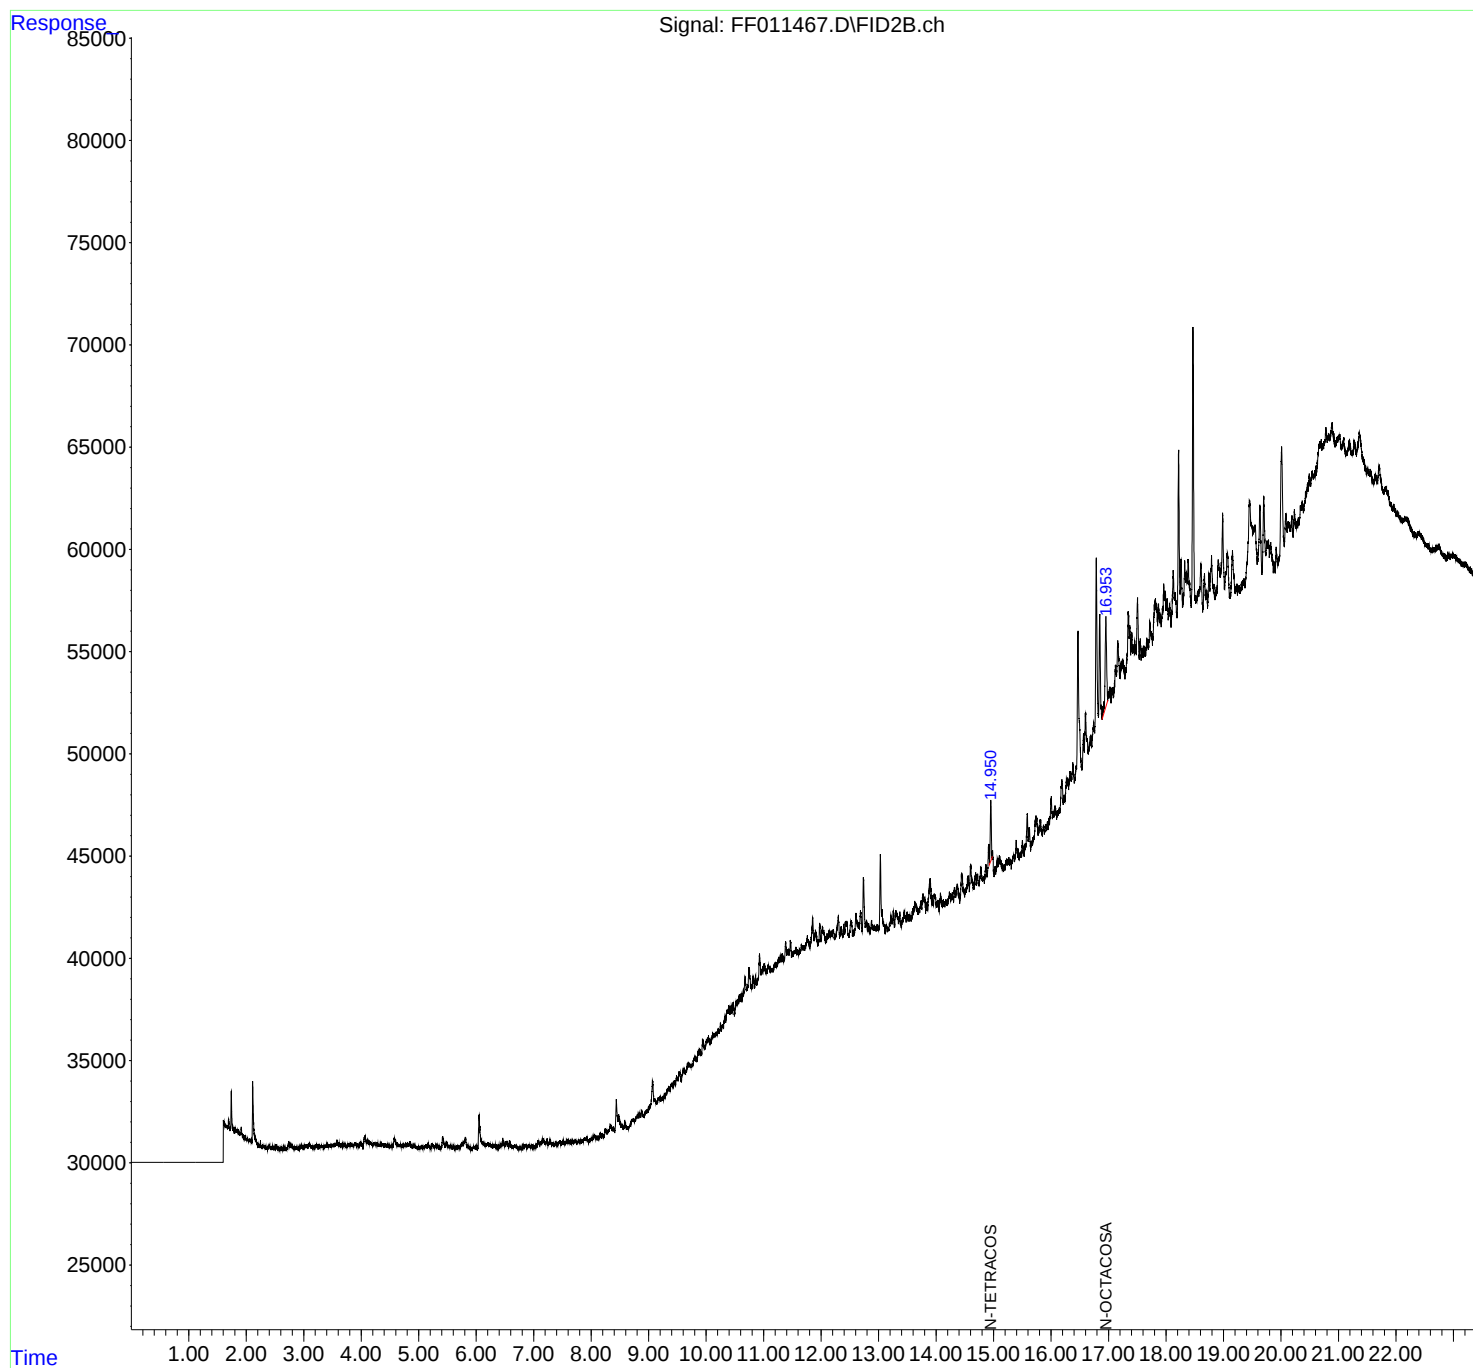


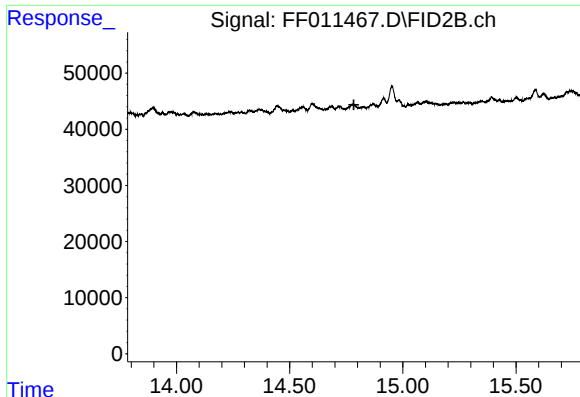

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.784 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

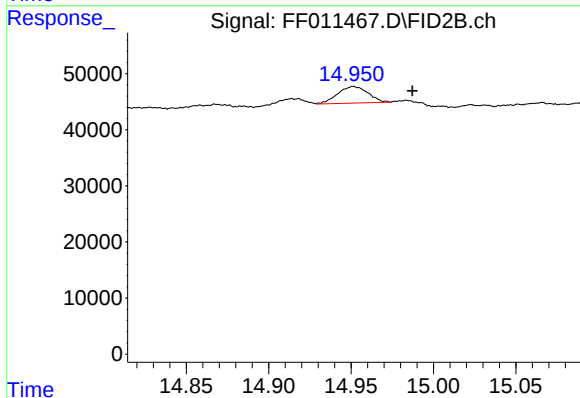

#10 N-TETRACOSANE

R.T.: 14.951 min
Delta R.T.: -0.036 min
Response: 37783
Conc: 0.30 ug/ml

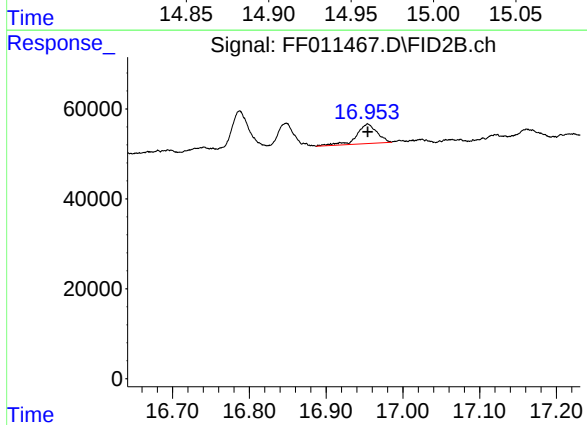

#12 N-OCTACOSANE

R.T.: 16.954 min
Delta R.T.: 0.000 min
Response: 79590
Conc: 0.65 ug/ml