

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
Data File : FF011454.D
Signal(s) : FID2B.ch
Acq On : 15 Sep 2022 11:44
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 16 03:30:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.514	2351930	17.961 ug/ml
12)	N-OCTACOSANE	16.952	2198586	17.949 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091522\
Data File : FF011454.D
Signal(s) : FID2B.ch
Acq On : 15 Sep 2022 11:44
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 16 03:30:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

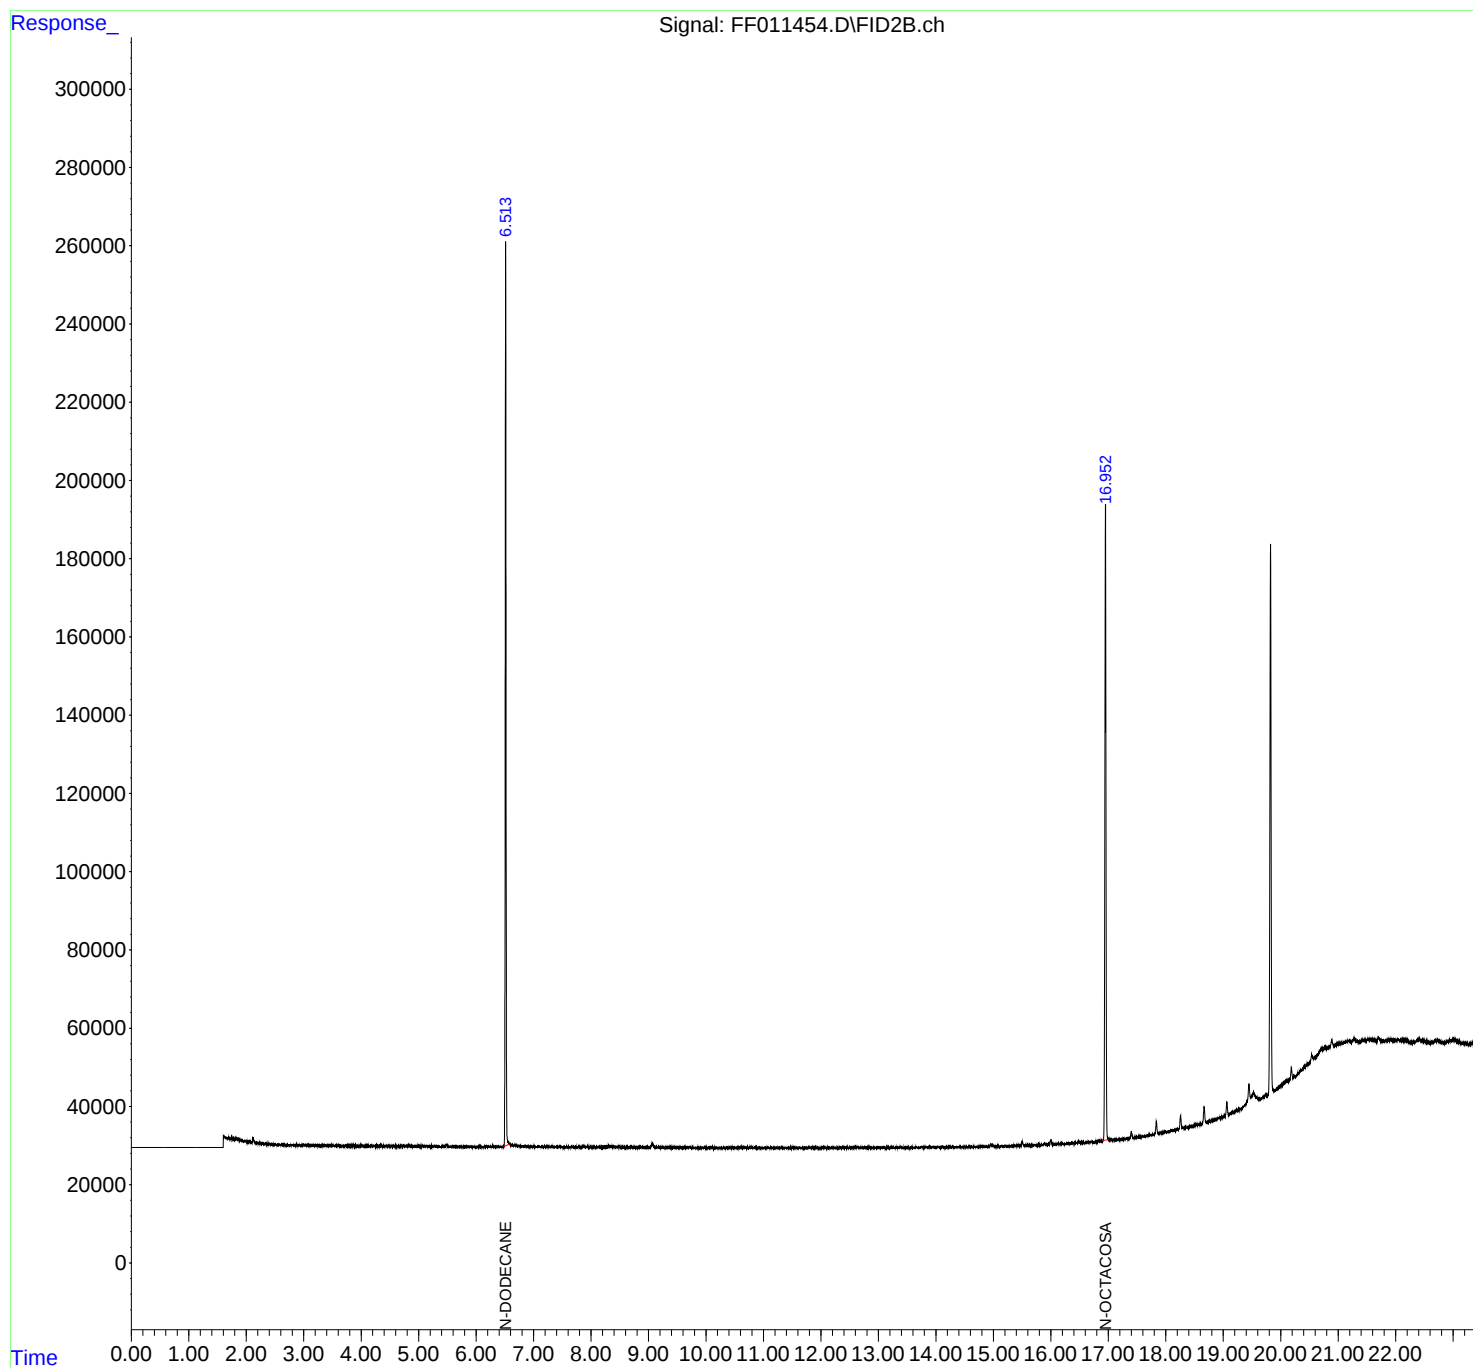


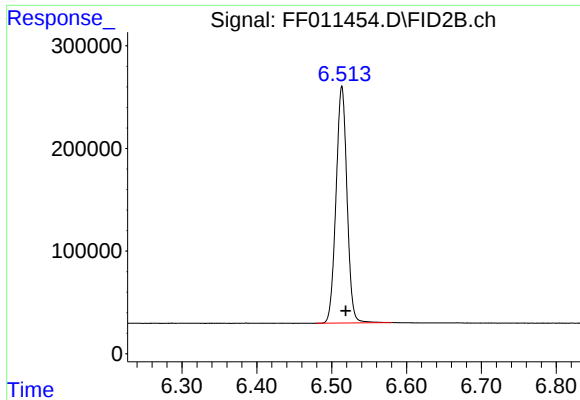

#3 N-DODECANE


R.T.: 6.514 min
Delta R.T.: -0.005 min
Response: 2351930
Conc: 17.96 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

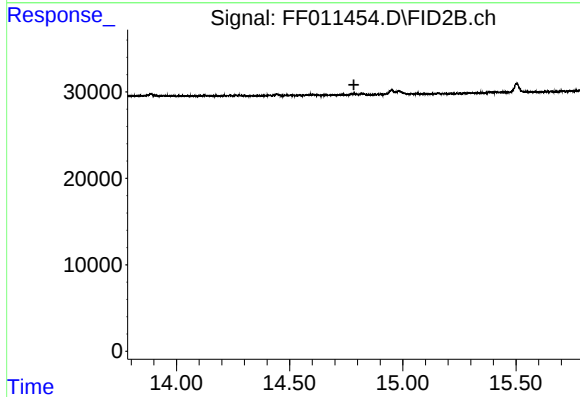

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.784 min
Response: 0
Conc: N.D.

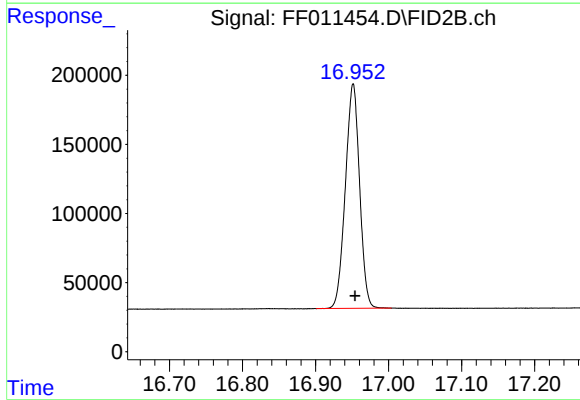

#12 N-OCTACOSANE

R.T.: 16.952 min
Delta R.T.: -0.003 min
Response: 2198586
Conc: 17.95 ug/ml