

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
Data File : FF005565.D
Signal(s) : FID2B.ch
Acq On : 16 Sep 2019 08:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 17 01:06:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.628	1922279	17.964 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.545	137215	1.107 ug/ml
15) N-TETRATRIACONTANE	19.345	11606	0.096 ug/ml
16) N-HEXATRIACONTANE	20.110	147811	1.232 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
Data File : FF005565.D
Signal(s) : FID2B.ch
Acq On : 16 Sep 2019 08:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 17 01:06:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

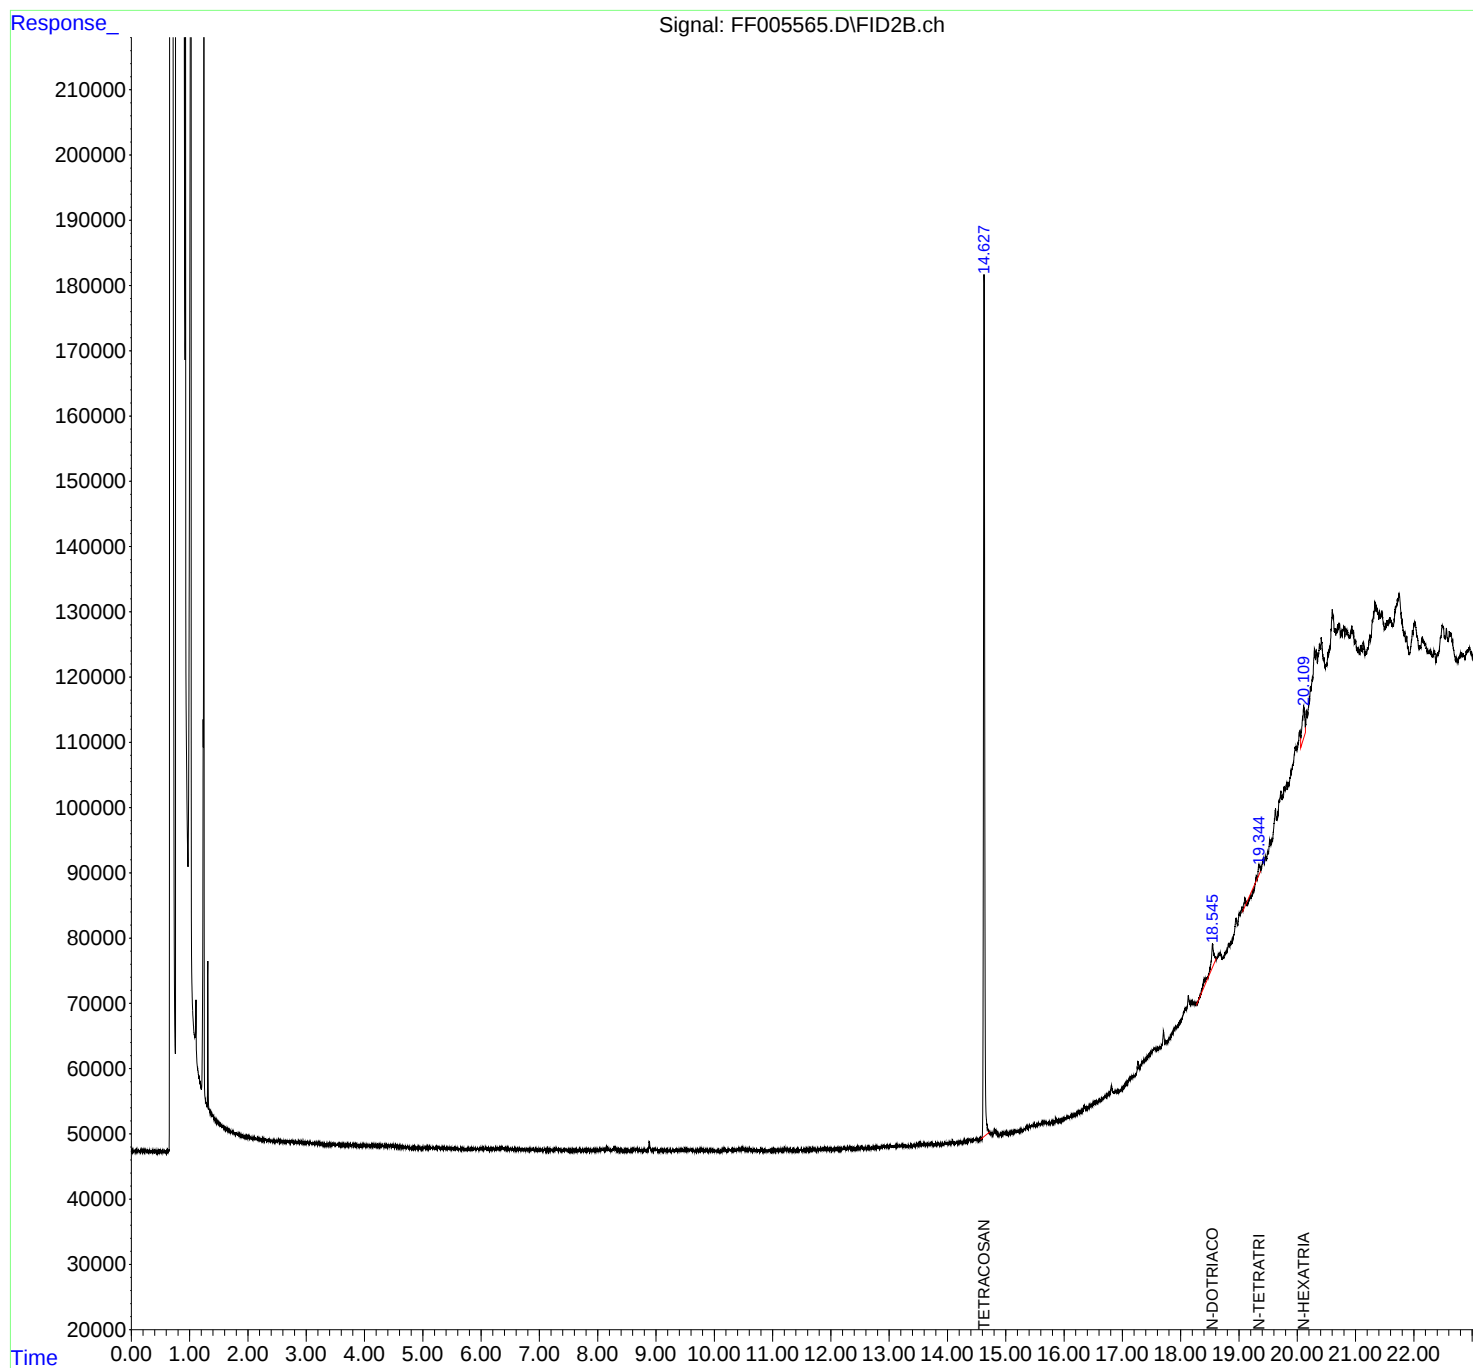


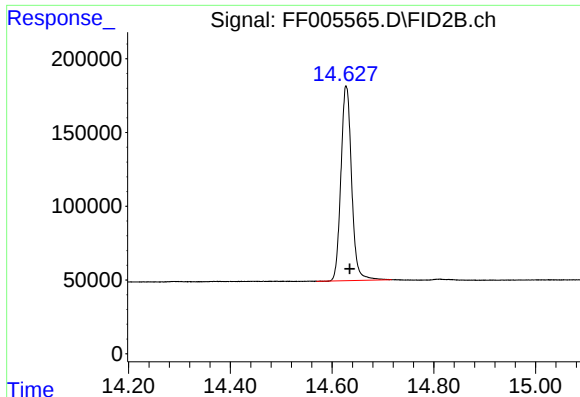

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.628 min
Delta R.T.: -0.007 min
Response: 1922279
Conc: 17.96 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

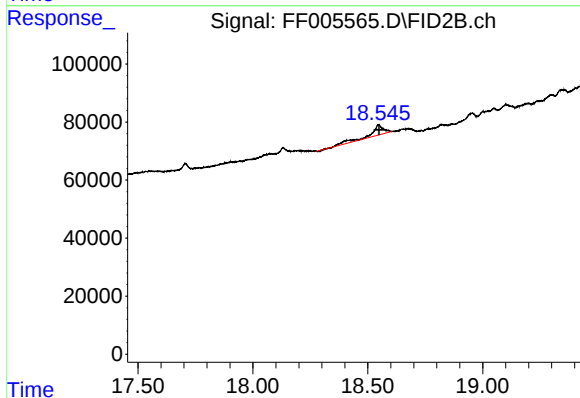


#14 N-DOTRIACONTANE

R.T.: 18.545 min
Delta R.T.: -0.004 min
Response: 137215
Conc: 1.11 ug/ml

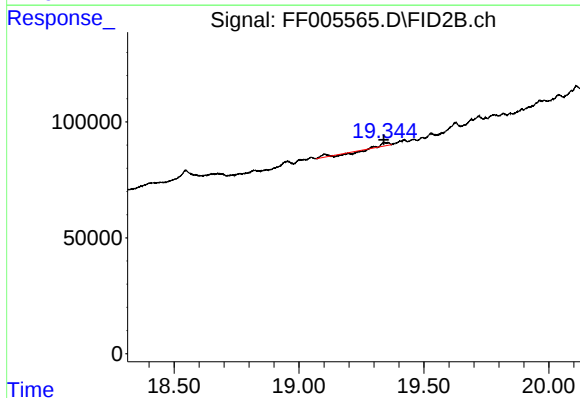

#15 N-TETRATRIACONTANE

R.T.: 19.345 min
Delta R.T.: 0.006 min
Response: 11606
Conc: 0.10 ug/ml

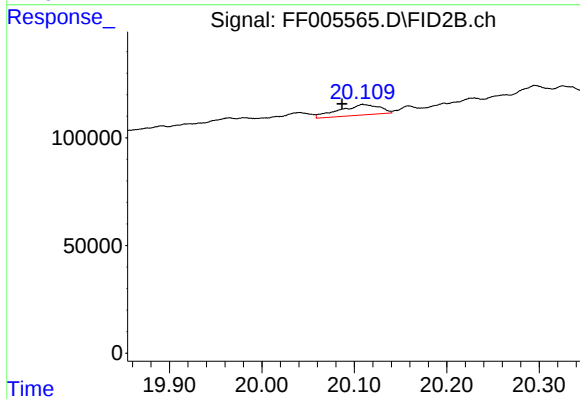

#16 N-HEXATRIACONTANE

R.T.: 20.110 min
Delta R.T.: 0.023 min
Response: 147811
Conc: 1.23 ug/ml