

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
 Data File : FF005571.D
 Signal(s) : FID2B.ch
 Acq On : 16 Sep 2019 13:08
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Sep 17 01:08:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	2027537	18.947 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.547	86793	0.700 ug/ml
15) N-TETRATRIACONTANE	19.338	90035	0.747 ug/ml
16) N-HEXATRIACONTANE	20.086	22795	0.190 ug/ml
17) N-OCTATRIACONTANE	20.832	1244455	11.406 ug/ml
18) N-TETRACONTANE	21.734	210401	1.655 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
Data File : FF005571.D
Signal(s) : FID2B.ch
Acq On : 16 Sep 2019 13:08
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 17 01:08:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

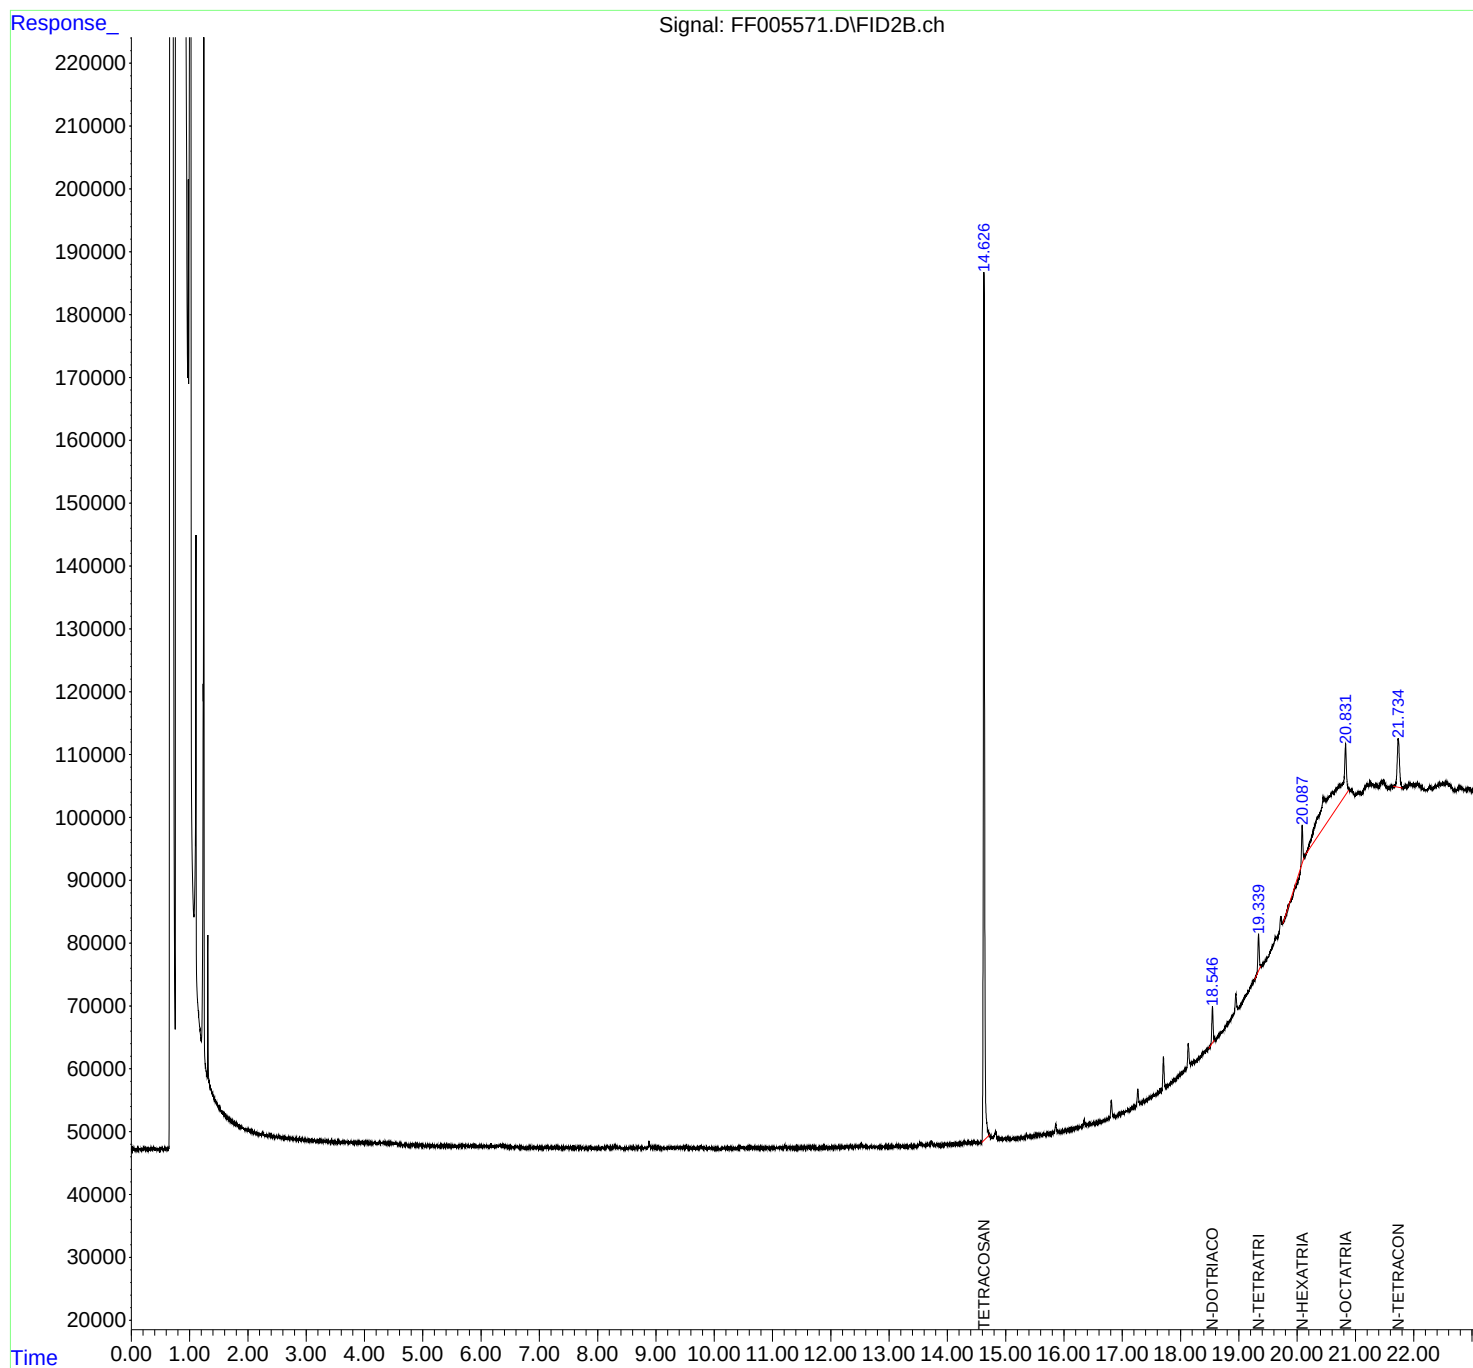


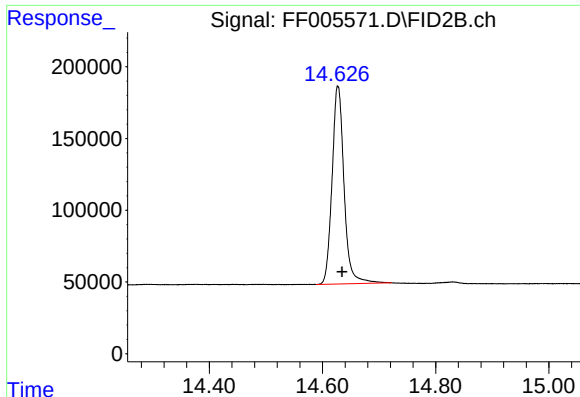

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.627 min
Delta R.T.: -0.007 min
Response: 2027537
Conc: 18.95 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

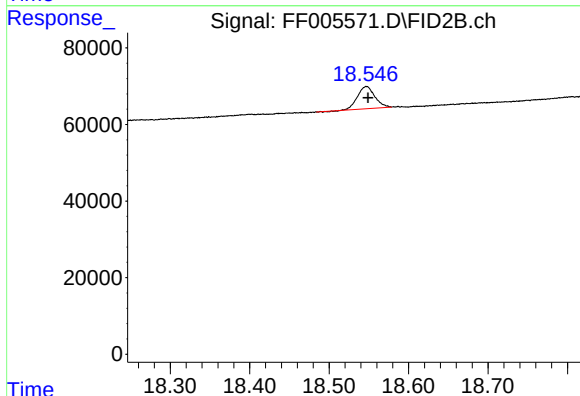


#14 N-DOTRIACONTANE

R.T.: 18.547 min
Delta R.T.: -0.002 min
Response: 86793
Conc: 0.70 ug/ml

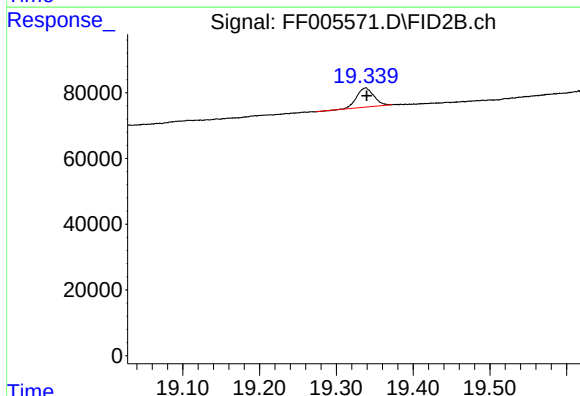


#15 N-TETRATRIACONTANE

R.T.: 19.338 min
Delta R.T.: -0.001 min
Response: 90035
Conc: 0.75 ug/ml

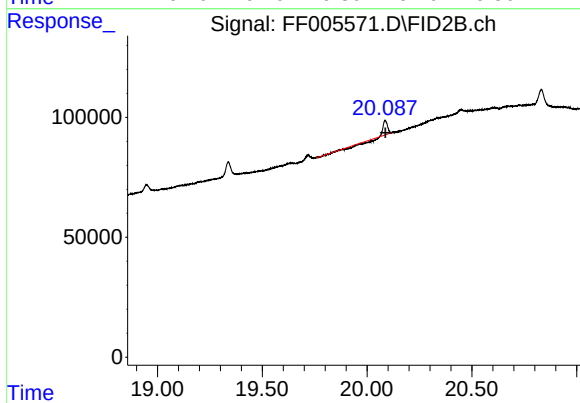

#16 N-HEXATRIACONTANE


R.T.: 20.086 min
Delta R.T.: 0.000 min
Response: 22795
Conc: 0.19 ug/ml

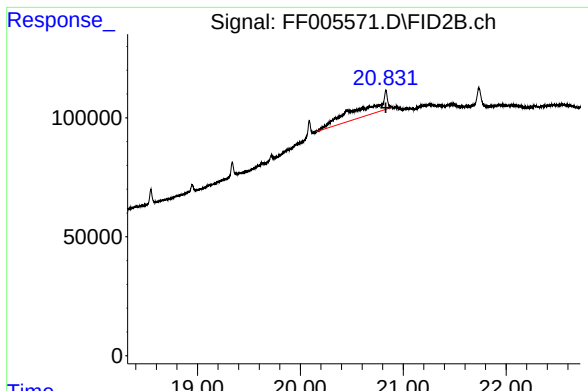

#17 N-OCTATRIACONTANE

R.T.: 20.832 min
Delta R.T.: 0.000 min
Response: 1244455
Conc: 11.41 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

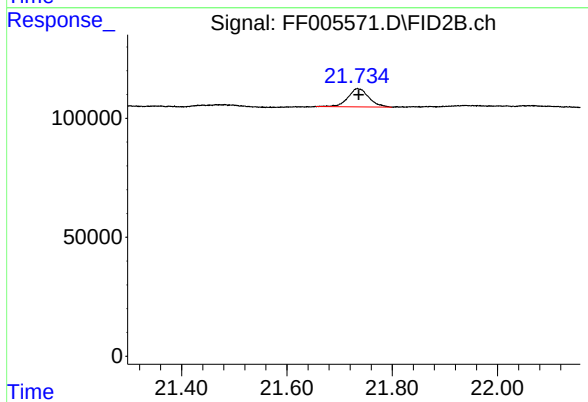

#18 N-TETRACONTANE

R.T.: 21.734 min
Delta R.T.: -0.003 min
Response: 210401
Conc: 1.65 ug/ml