

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
Data File : FF005576.D
Signal(s) : FID2B.ch
Acq On : 16 Sep 2019 17:01
Operator : DD\AJ
Sample : K4863-04 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSA-4-6

Integration File: autoint1.e
Quant Time: Sep 17 01:10:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
12) N-OCTACOSANE	16.833	195174	1.636 ug/ml
13) N-TRIACONTANE	17.707	118362	0.978 ug/ml
14) N-DOTRIACONTANE	18.553	110245	0.889 ug/ml
15) N-TETRATRIACONTANE	19.369	314891	2.613 ug/ml
16) N-HEXATRIACONTANE	20.079	283180	2.359 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
 Data File : FF005576.D
 Signal(s) : FID2B.ch
 Acq On : 16 Sep 2019 17:01
 Operator : DD\AJ
 Sample : K4863-04 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 Client Sampled :
 CSA-4-6

Integration File: autoint1.e
 Quant Time: Sep 17 01:10:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

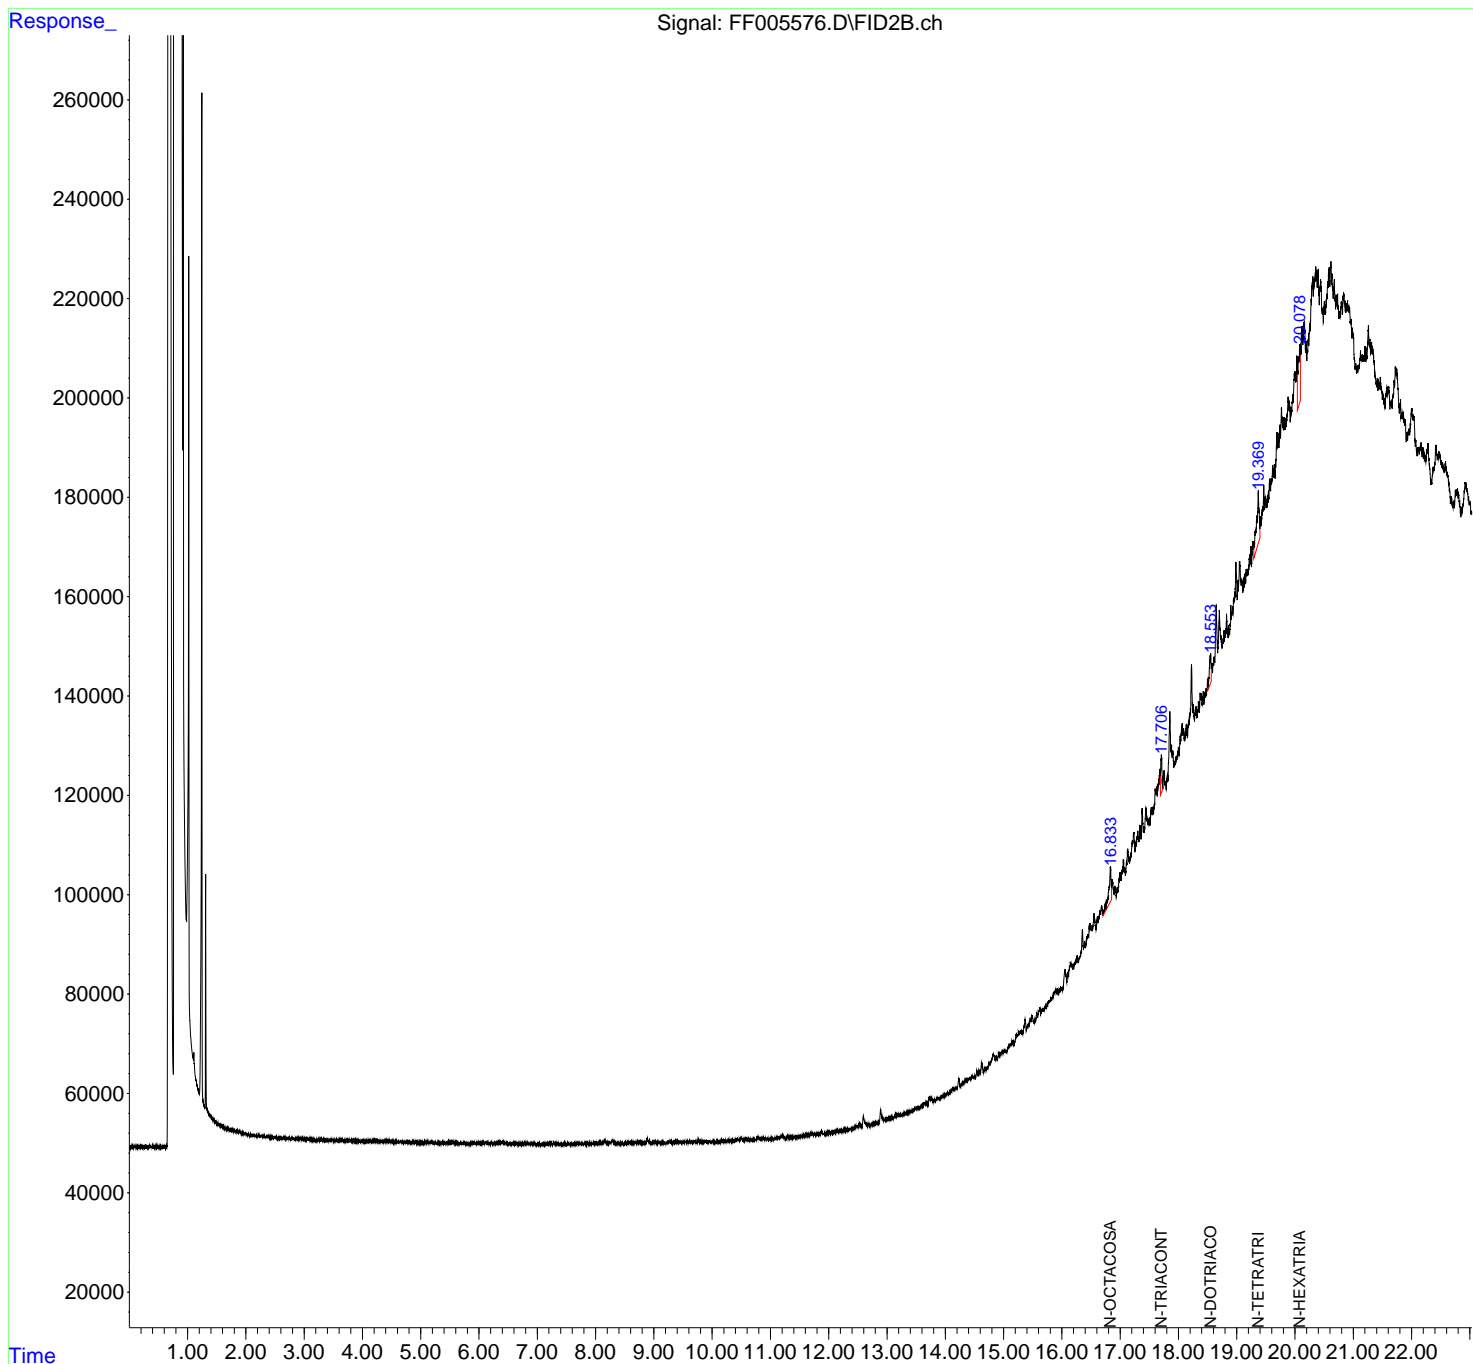


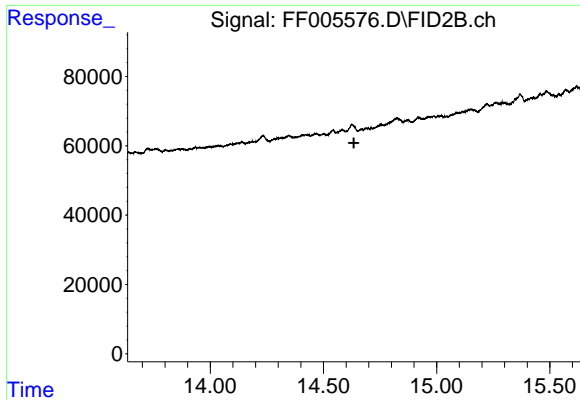

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
 Exp R.T.: 14.635 min
 Response: 0
 Conc: N.D.

Instrument :
 FID_F
 ClientSampleId :
 CSA-4-6

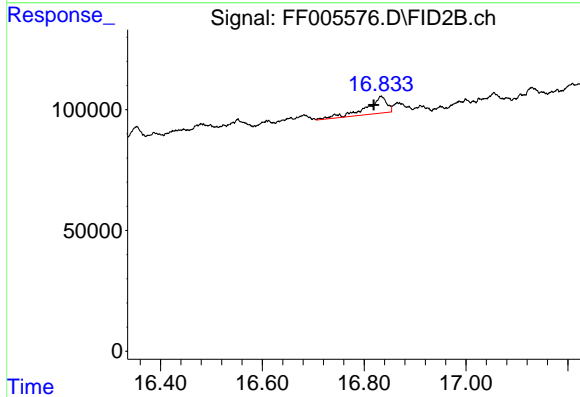


#12 N-OCTACOSANE

R.T.: 16.833 min
 Delta R.T.: 0.014 min
 Response: 195174
 Conc: 1.64 ug/ml

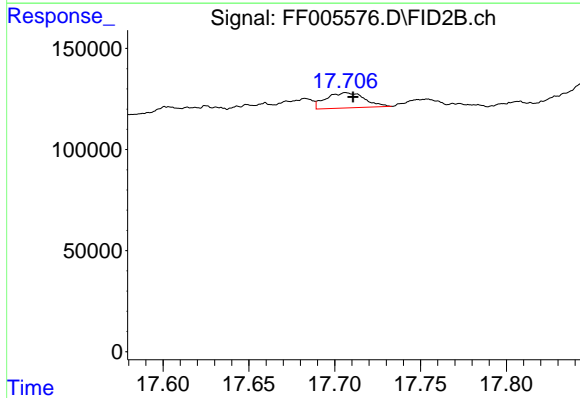


#13 N-TRIACONTANE

R.T.: 17.707 min
 Delta R.T.: -0.004 min
 Response: 118362
 Conc: 0.98 ug/ml

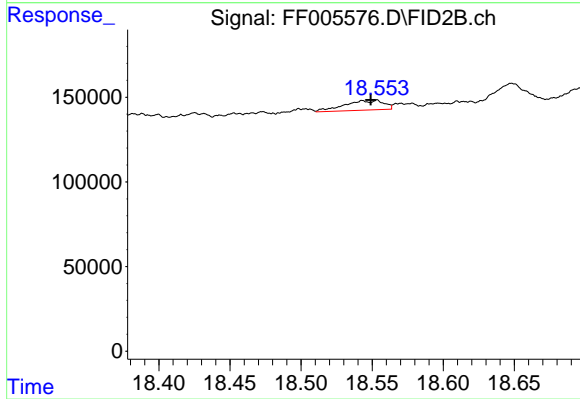

#14 N-DOTRIACONTANE


R.T.: 18.553 min
 Delta R.T.: 0.004 min
 Response: 110245
 Conc: 0.89 ug/ml

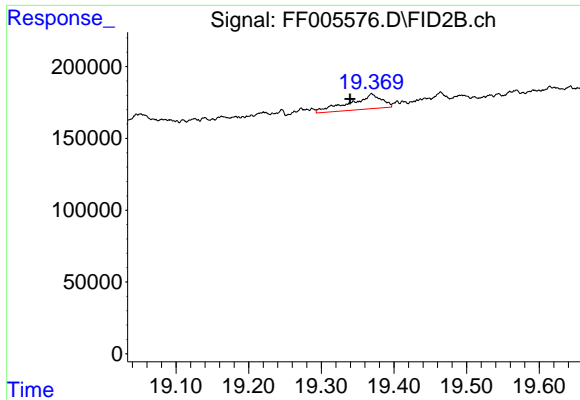

#15 N-TETRATRIACONTANE

R.T.: 19.369 min
Delta R.T.: 0.030 min
Response: 314891
Conc: 2.61 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-4-6

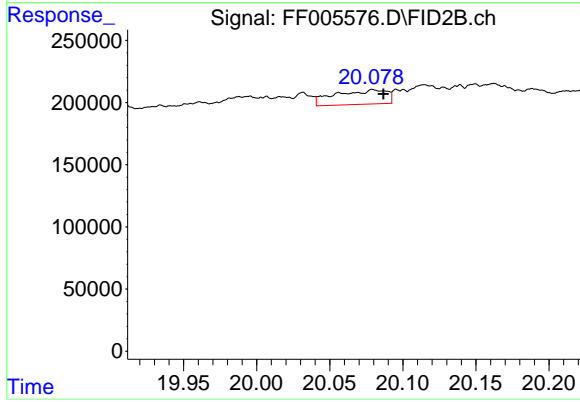

#16 N-HEXATRIACONTANE

R.T.: 20.079 min
Delta R.T.: -0.007 min
Response: 283180
Conc: 2.36 ug/ml