

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
Data File : FF005579.D
Signal(s) : FID2B.ch
Acq On : 16 Sep 2019 18:30
Operator : DD\AJ
Sample : K4877-06 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSA-2-3

Integration File: autoint1.e
Quant Time: Sep 17 01:11:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

12)	N-OCTACOSANE	16.834	82341	0.690 ug/ml
13)	N-TRIACONTANE	17.708	193305	1.598 ug/ml
14)	N-DOTRIACONTANE	18.549	193274	1.559 ug/ml
15)	N-TETRATRIACONTANE	19.339	100171	0.831 ug/ml
16)	N-HEXATRIACONTANE	20.135	798371	6.652 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
Data File : FF005579.D
Signal(s) : FID2B.ch
Acq On : 16 Sep 2019 18:30
Operator : DD\AJ
Sample : K4877-06 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSA-2-3

Integration File: autoint1.e
Quant Time: Sep 17 01:11:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

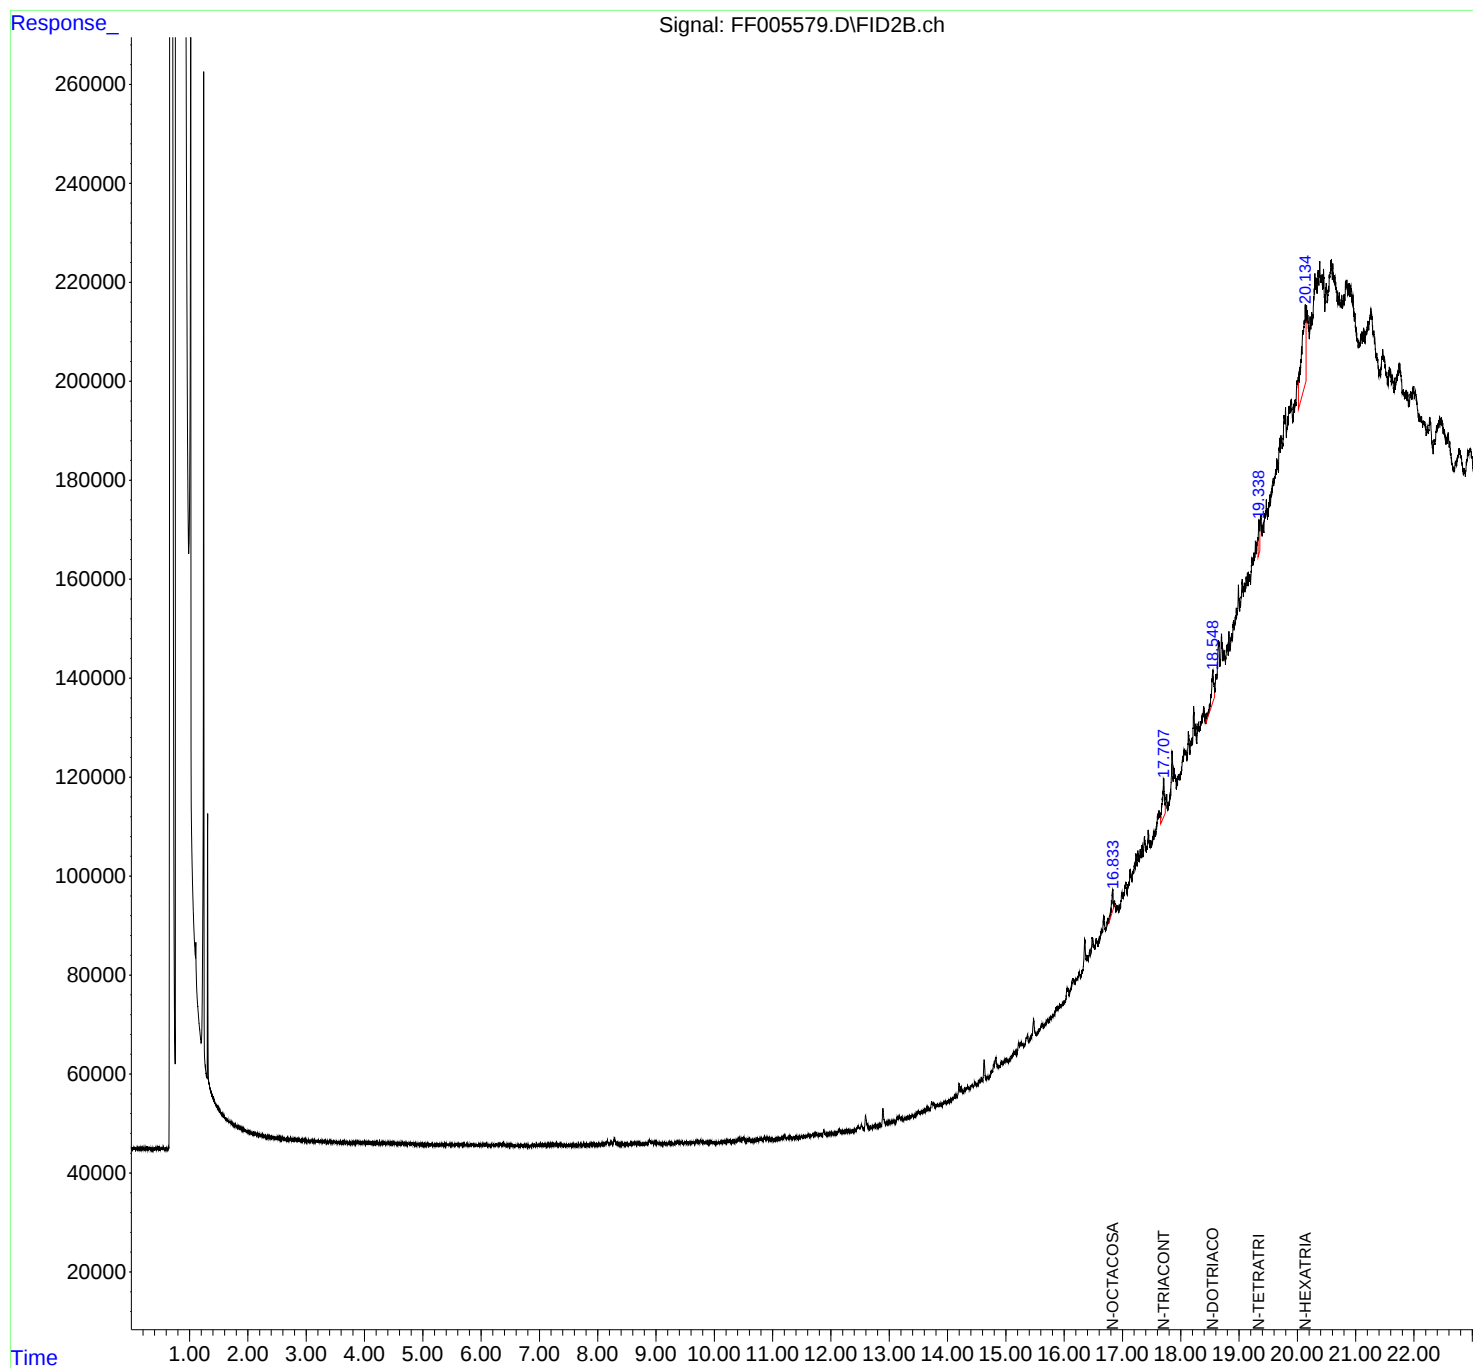


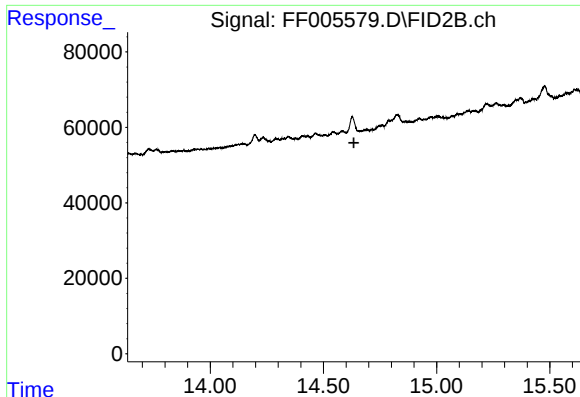

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.635 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
CSA-2-3

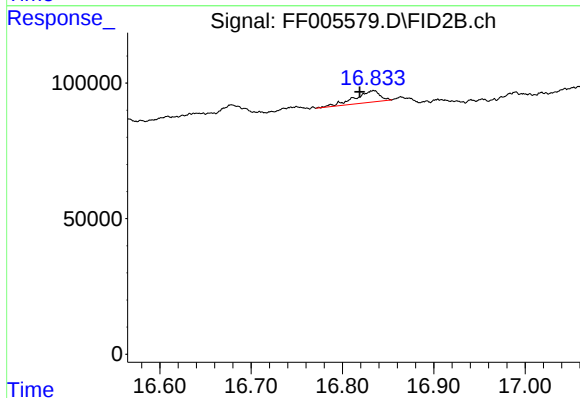


#12 N-OCTACOSANE

R.T.: 16.834 min
Delta R.T.: 0.015 min
Response: 82341
Conc: 0.69 ug/ml

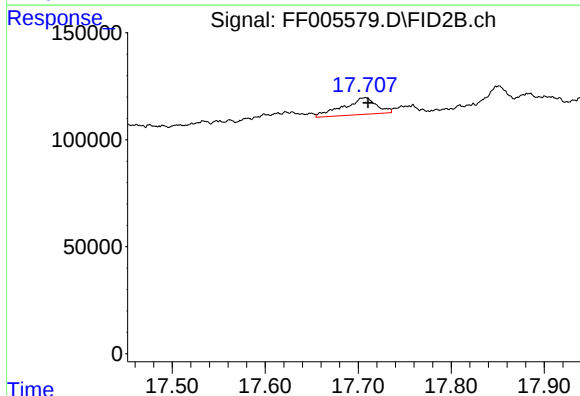


#13 N-TRIACONTANE

R.T.: 17.708 min
Delta R.T.: -0.003 min
Response: 193305
Conc: 1.60 ug/ml

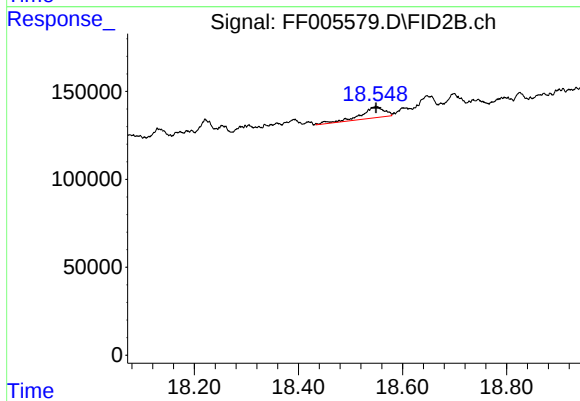

#14 N-DOTRIACONTANE


R.T.: 18.549 min
Delta R.T.: 0.000 min
Response: 193274
Conc: 1.56 ug/ml

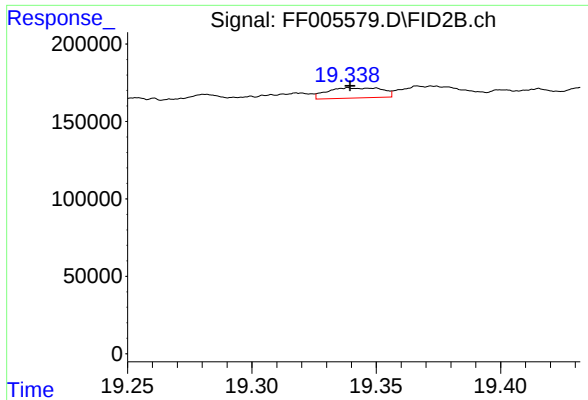

#15 N-TETRATRIACONTANE

R.T.: 19.339 min
Delta R.T.: 0.000 min
Response: 100171
Conc: 0.83 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-3

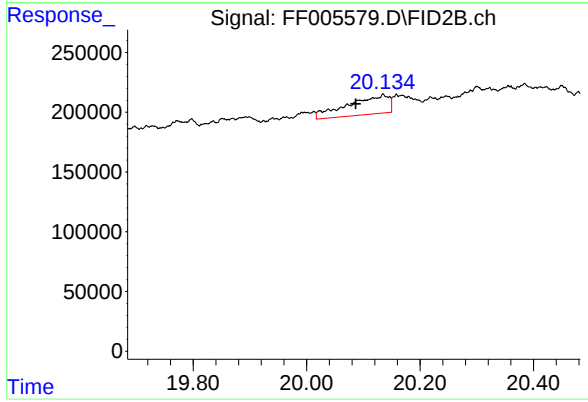

#16 N-HEXATRIACONTANE

R.T.: 20.135 min
Delta R.T.: 0.048 min
Response: 798371
Conc: 6.65 ug/ml