

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
Data File : FF005580.D
Signal(s) : FID2B.ch
Acq On : 16 Sep 2019 19:05
Operator : DD\AJ
Sample : K4877-09 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSA-2-4

Integration File: autoint1.e
Quant Time: Sep 17 01:11:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) N-HEXACOSANE	15.864	65237	0.545 ug/ml
12) N-OCTACOSANE	16.803	142996	1.198 ug/ml
13) N-TRIACONTANE	17.714	659214	5.450 ug/ml
14) N-DOTRIACONTANE	18.551	281395	2.270 ug/ml
15) N-TETRATRIACONTANE	19.344	47696	0.396 ug/ml
16) N-HEXATRIACONTANE	20.078	77849	0.649 ug/ml
17) N-OCTATRIACONTANE	20.854	128384	1.177 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
Data File : FF005580.D
Signal(s) : FID2B.ch
Acq On : 16 Sep 2019 19:05
Operator : DD\AJ
Sample : K4877-09 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSA-2-4

Integration File: autoint1.e
Quant Time: Sep 17 01:11:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

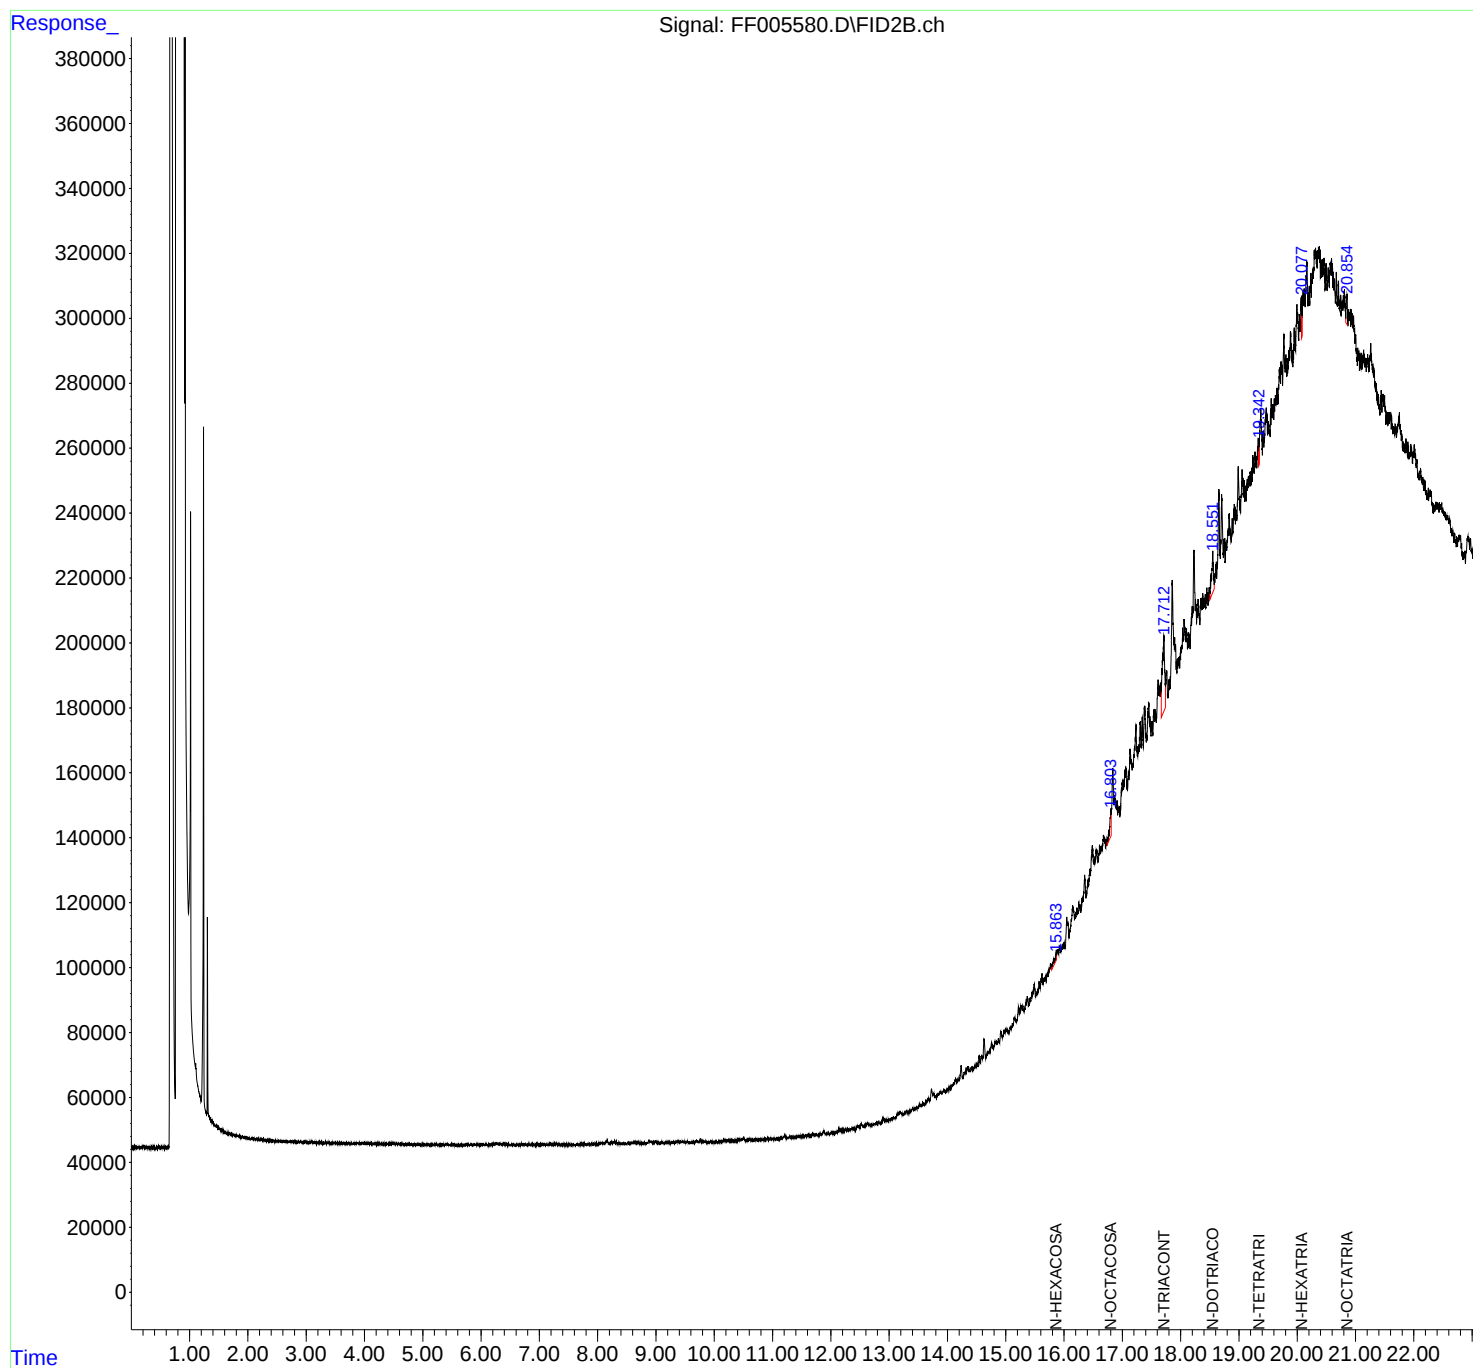


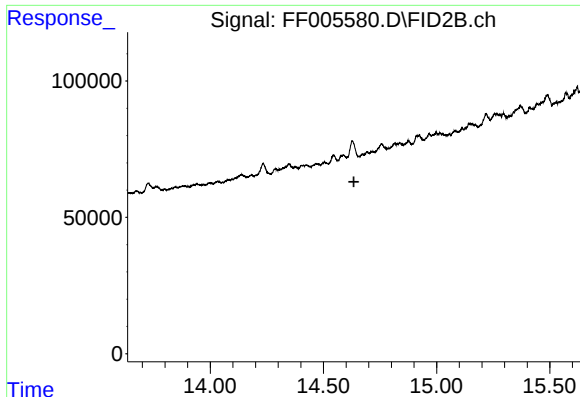

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.635 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
CSA-2-4

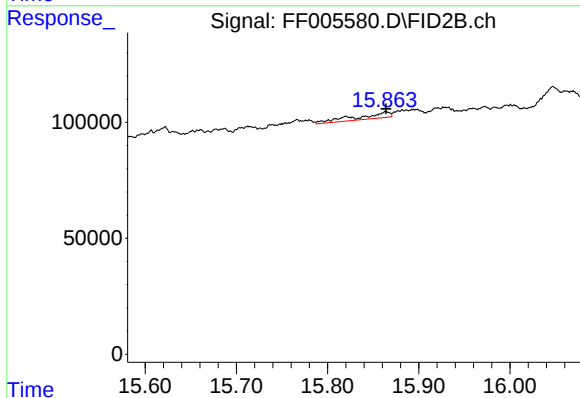


#11 N-HEXACOSANE

R.T.: 15.864 min
Delta R.T.: 0.000 min
Response: 65237
Conc: 0.54 ug/ml

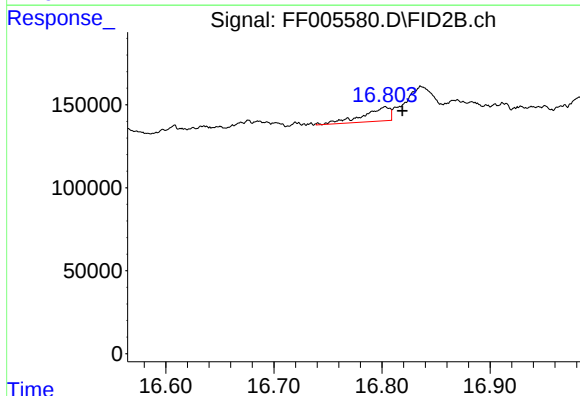


#12 N-OCTACOSANE

R.T.: 16.803 min
Delta R.T.: -0.016 min
Response: 142996
Conc: 1.20 ug/ml

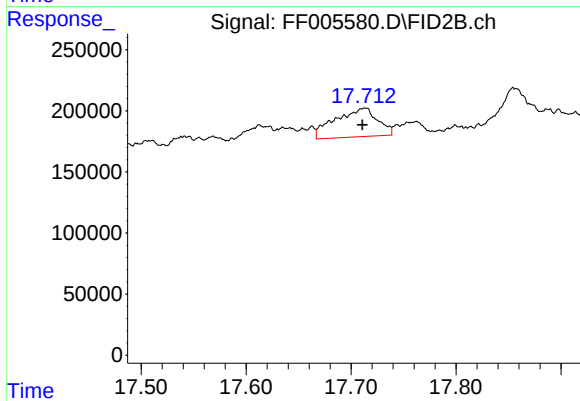

#13 N-TRIACONTANE


R.T.: 17.714 min
Delta R.T.: 0.003 min
Response: 659214
Conc: 5.45 ug/ml

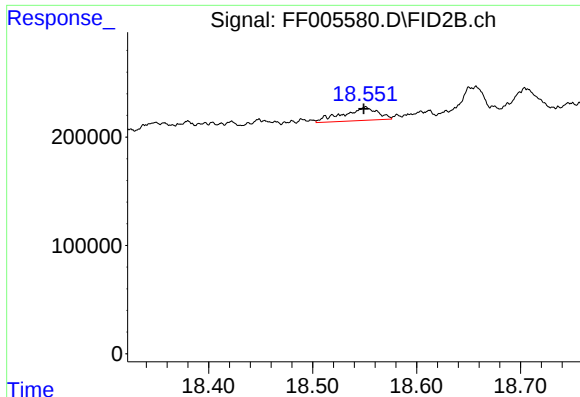

#14 N-DOTRIACONTANE


R.T.: 18.551 min
Delta R.T.: 0.002 min
Response: 281395
Conc: 2.27 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-4

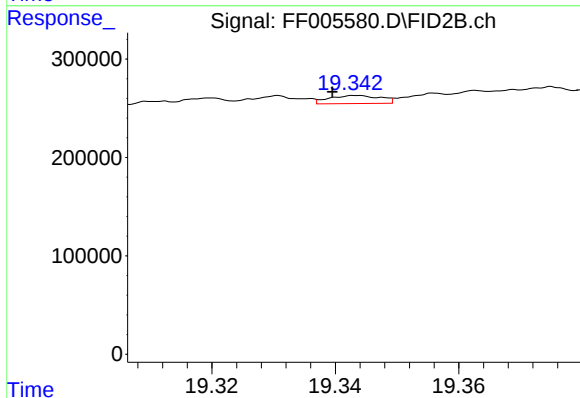


#15 N-TETRATRIACONTANE

R.T.: 19.344 min
Delta R.T.: 0.004 min
Response: 47696
Conc: 0.40 ug/ml

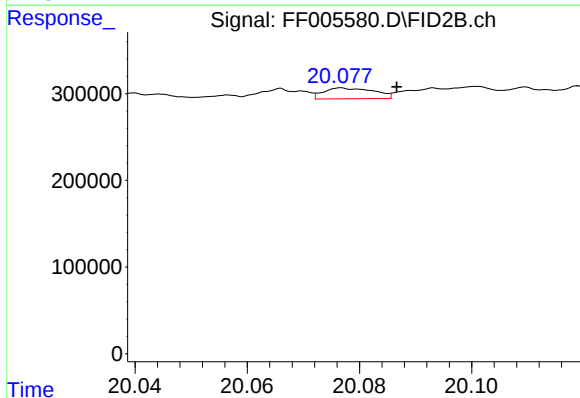

#16 N-HEXATRIACONTANE

R.T.: 20.078 min
Delta R.T.: -0.009 min
Response: 77849
Conc: 0.65 ug/ml

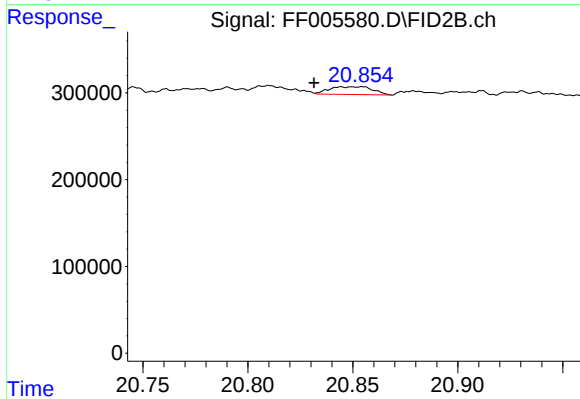

#17 N-OCTATRIACONTANE

R.T.: 20.854 min
Delta R.T.: 0.023 min
Response: 128384
Conc: 1.18 ug/ml