

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
 Data File : FF005581.D
 Signal(s) : FID2B.ch
 Acq On : 16 Sep 2019 19:34
 Operator : DD\AJ
 Sample : K4878-03 5X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CSA-2-6

Integration File: autoint1.e
 Quant Time: Sep 17 01:11:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
7) N-EICOSANE	12.589f	1441918	10.995 ug/ml
10) N-TETRACOSANE	14.820	749541	6.129 ug/ml
12) N-OCTACOSANE	16.839	522016	4.375 ug/ml
13) N-TRIACONTANE	17.712	358717	2.965 ug/ml
14) N-DOTRIACONTANE	18.547	352462	2.843 ug/ml
15) N-TETRATRIACONTANE	19.341	144101	1.196 ug/ml
16) N-HEXATRIACONTANE	20.094	484165	4.034 ug/ml
17) N-OCTATRIACONTANE	20.841	23878	0.219 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
Data File : FF005581.D
Signal(s) : FID2B.ch
Acq On : 16 Sep 2019 19:34
Operator : DD\AJ
Sample : K4878-03 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSA-2-6

Integration File: autoint1.e
Quant Time: Sep 17 01:11:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

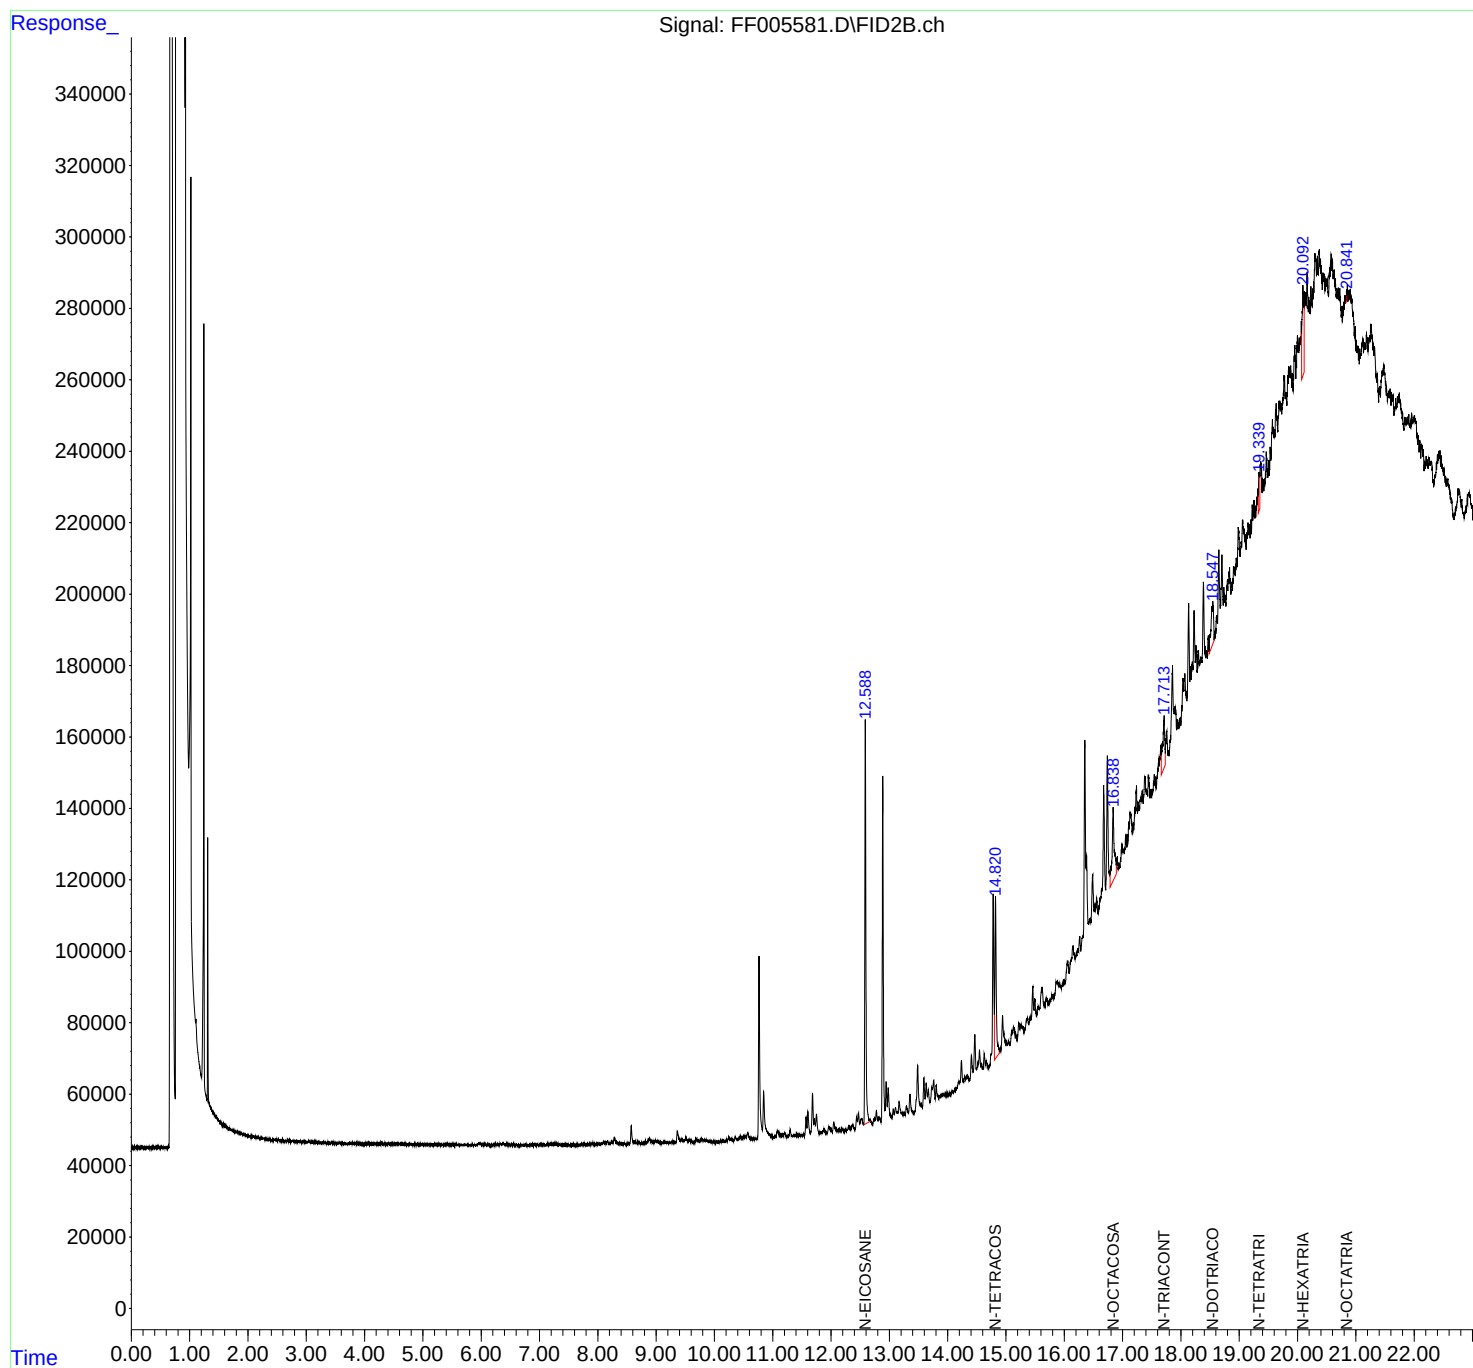


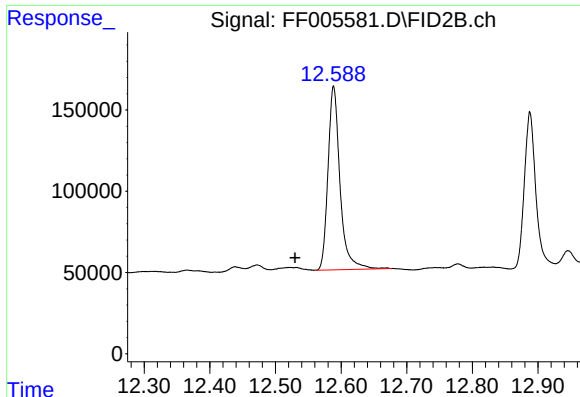

#7 N-EICOSANE


R.T.: 12.589 min
Delta R.T.: 0.059 min
Response: 1441918
Conc: 10.99 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-6

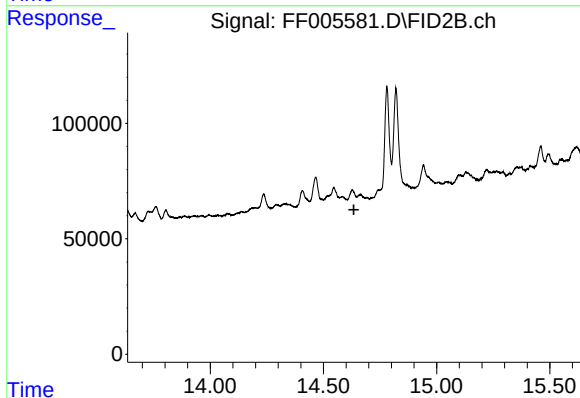


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.635 min
Response: 0
Conc: N.D.

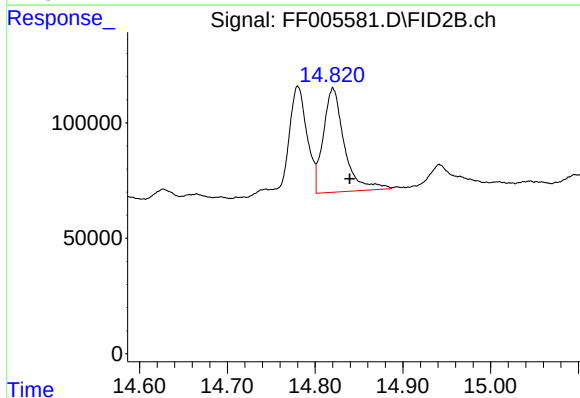


#10 N-TETRACOSANE

R.T.: 14.820 min
Delta R.T.: -0.019 min
Response: 749541
Conc: 6.13 ug/ml

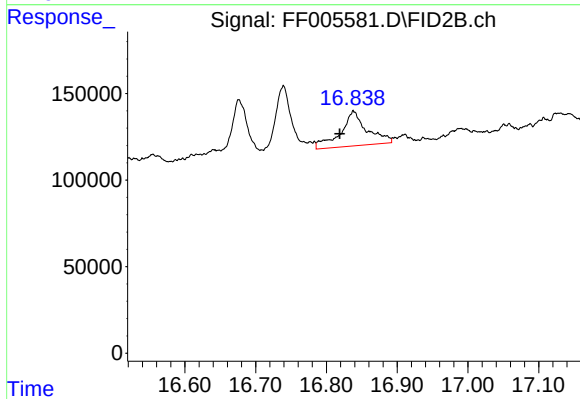

#12 N-OCTACOSANE


R.T.: 16.839 min
Delta R.T.: 0.020 min
Response: 522016
Conc: 4.37 ug/ml

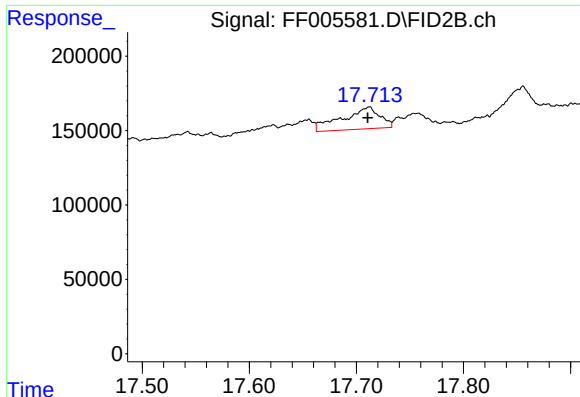

#13 N-TRIACONTANE


R.T.: 17.712 min
Delta R.T.: 0.001 min
Response: 358717
Conc: 2.97 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-6

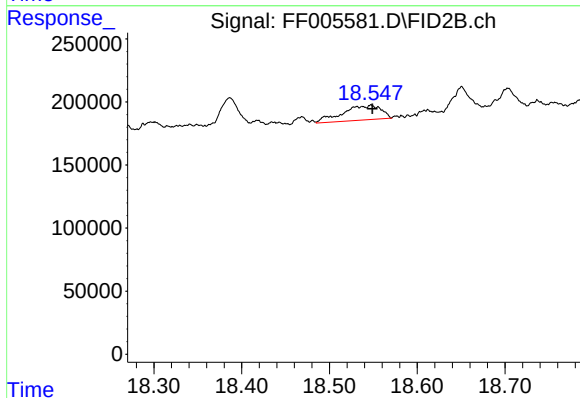


#14 N-DOTRIACONTANE

R.T.: 18.547 min
Delta R.T.: -0.002 min
Response: 352462
Conc: 2.84 ug/ml

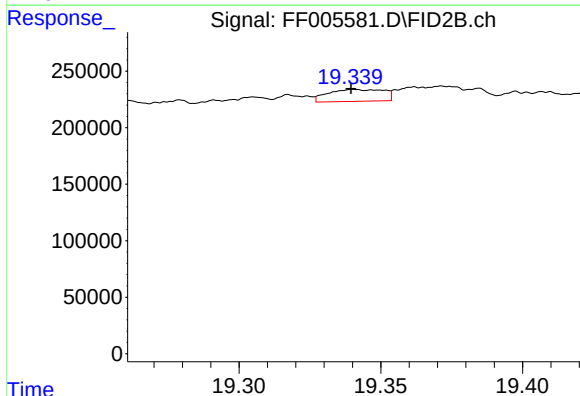


#15 N-TETRATRIACONTANE

R.T.: 19.341 min
Delta R.T.: 0.000 min
Response: 144101
Conc: 1.20 ug/ml

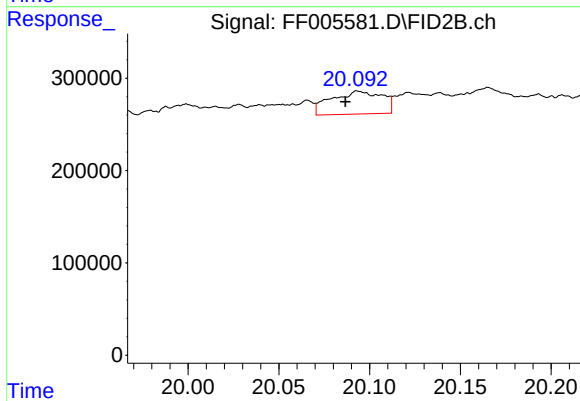

#16 N-HEXATRIACONTANE

R.T.: 20.094 min
Delta R.T.: 0.007 min
Response: 484165
Conc: 4.03 ug/ml

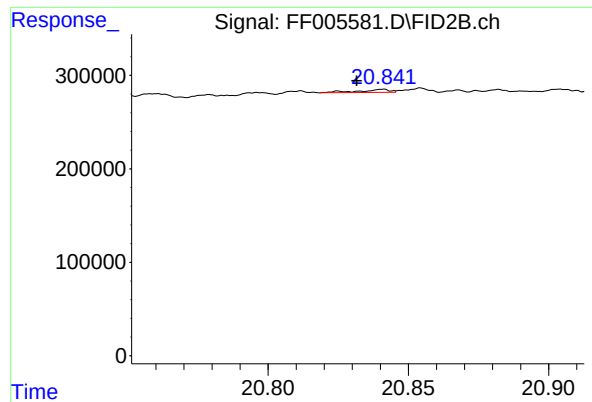

#17 N-OCTATRIACONTANE

R.T.: 20.841 min
Delta R.T.: 0.009 min
Response: 23878
Conc: 0.22 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-6