

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
 Data File : FF005582.D
 Signal(s) : FID2B.ch
 Acq On : 16 Sep 2019 20:04
 Operator : DD\AJ
 Sample : K4878-06 5X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CSA-2-7

Integration File: autoint1.e
 Quant Time: Sep 17 01:11:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
7)	N-EICOSANE	12.472f	144730	1.104 ug/ml
8)	N-DOCOSANE	13.759	392372	3.116 ug/ml
10)	N-TETRACOSANE	14.821	2044355	16.716 ug/ml
11)	N-HEXACOSANE	15.855	232676	1.944 ug/ml
12)	N-OCTACOSANE	16.840	654172	5.482 ug/ml
13)	N-TRIACONTANE	17.710	328264	2.714 ug/ml
14)	N-DOTRIACONTANE	18.524	499068	4.026 ug/ml
15)	N-TETRATRIACONTANE	19.340	171088	1.420 ug/ml
16)	N-HEXATRIACONTANE	20.096	1244728	10.371 ug/ml
17)	N-OCTATRIACONTANE	20.846	63461	0.582 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
Data File : FF005582.D
Signal(s) : FID2B.ch
Acq On : 16 Sep 2019 20:04
Operator : DD\AJ
Sample : K4878-06 5X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSA-2-7

Integration File: autoint1.e
Quant Time: Sep 17 01:11:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

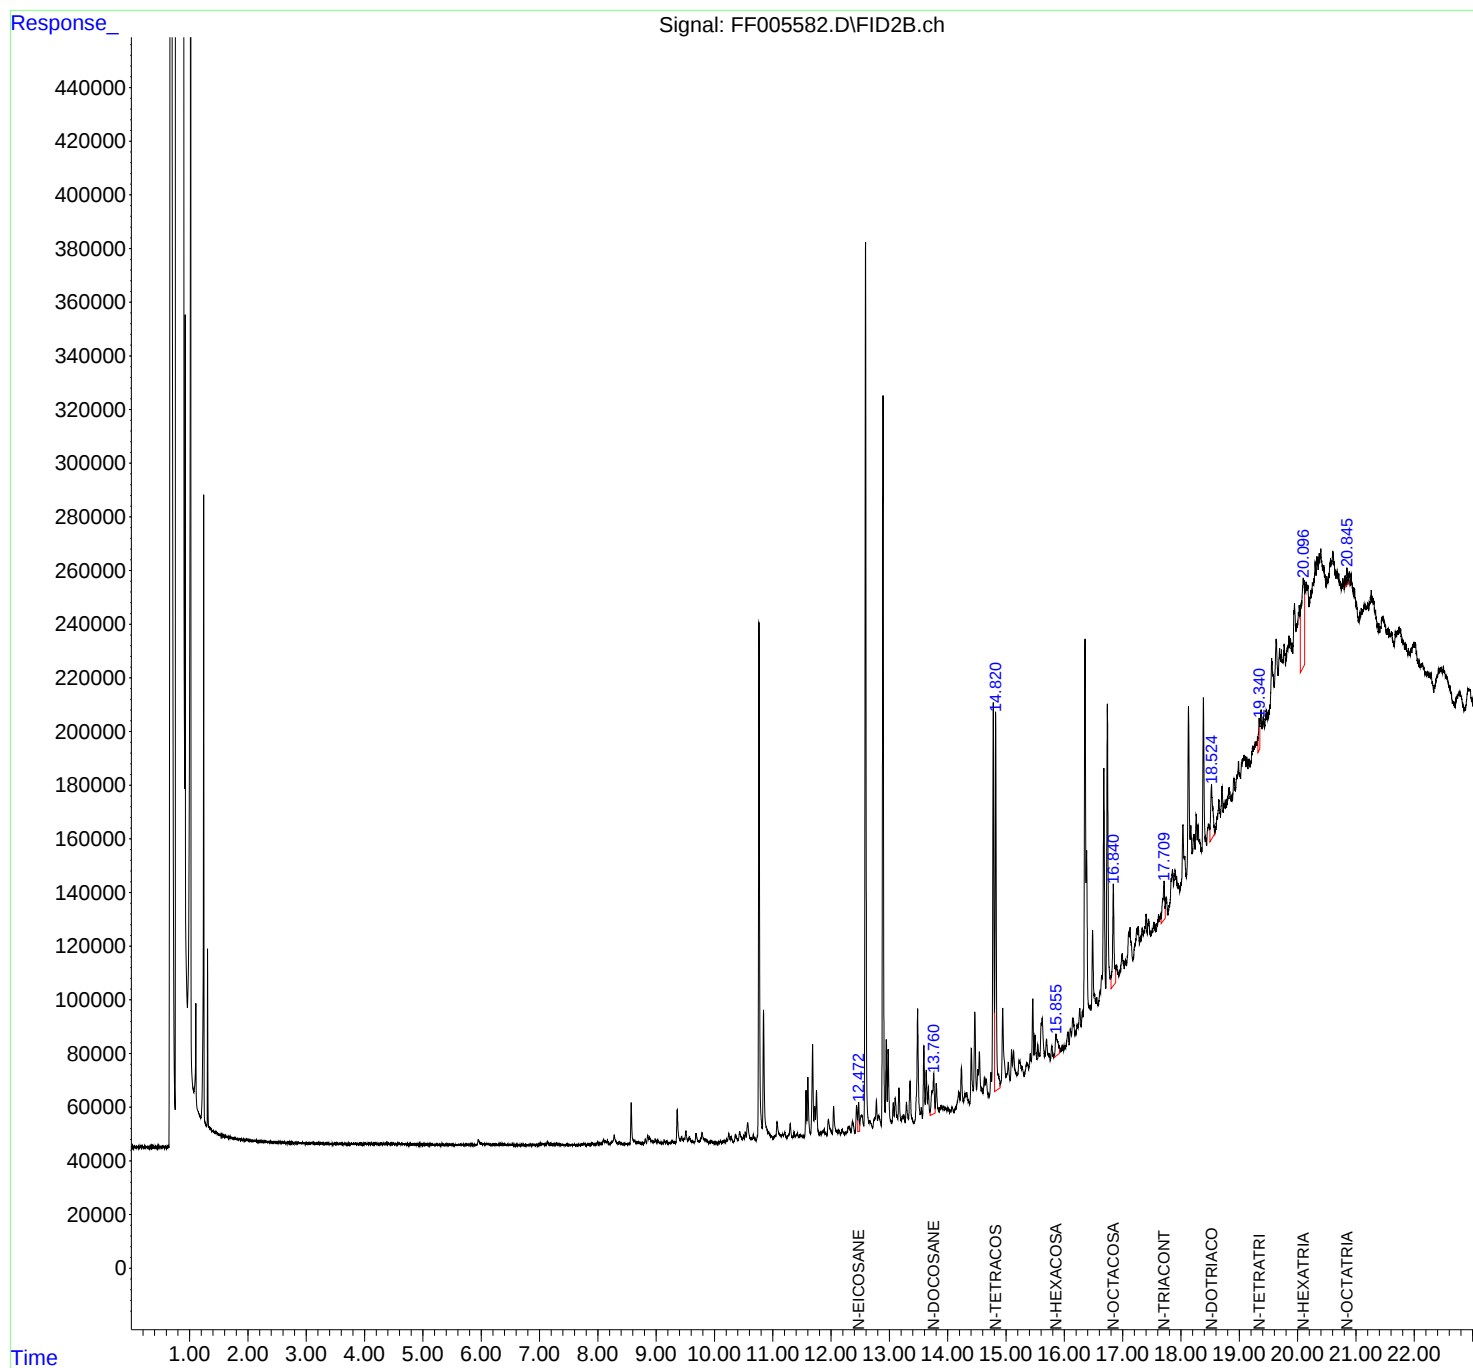


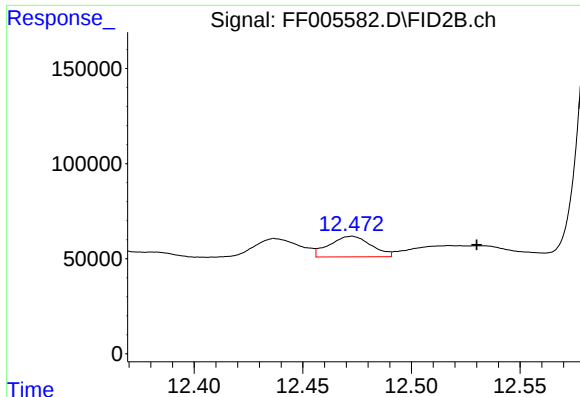

#7 N-EICOSANE


R.T.: 12.472 min
Delta R.T.: -0.058 min
Response: 144730
Conc: 1.10 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-7

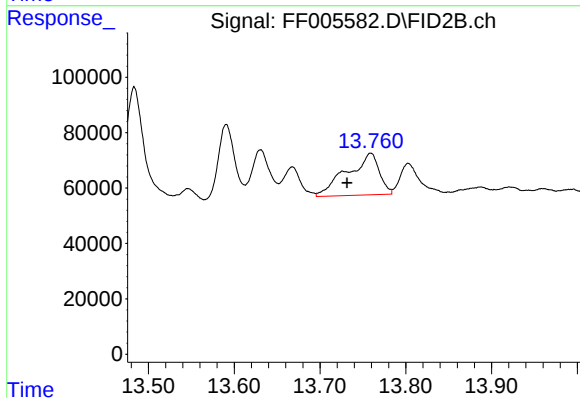


#8 N-DOCOSANE

R.T.: 13.759 min
Delta R.T.: 0.027 min
Response: 392372
Conc: 3.12 ug/ml

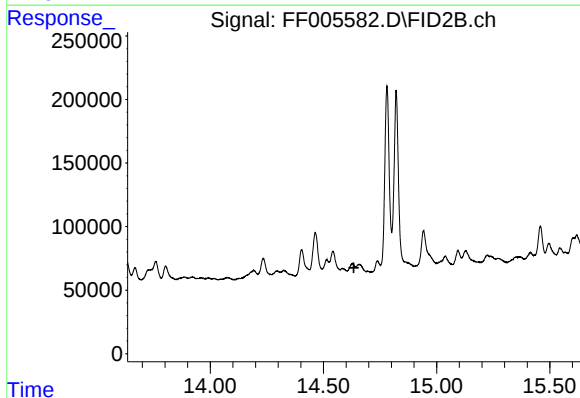


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.635 min
Response: 0
Conc: N.D.

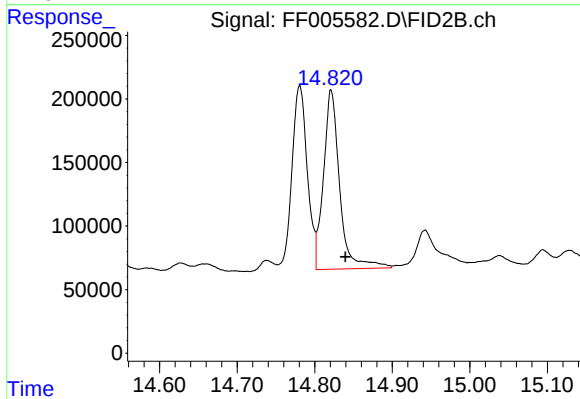

#10 N-TETRACOSANE


R.T.: 14.821 min
Delta R.T.: -0.018 min
Response: 2044355
Conc: 16.72 ug/ml

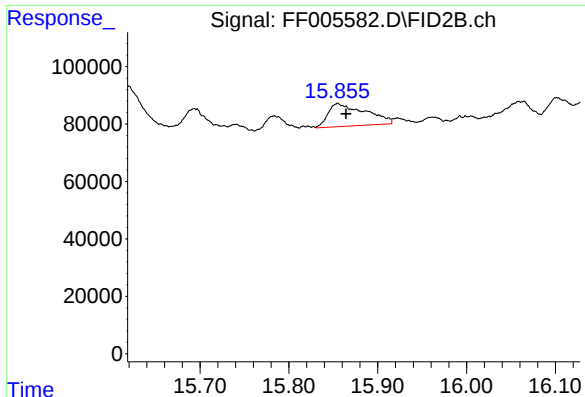

#11 N-HEXACOSANE


R.T.: 15.855 min
Delta R.T.: -0.009 min
Response: 232676
Conc: 1.94 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-7

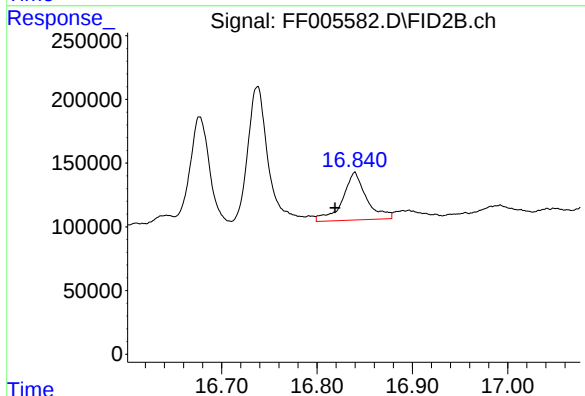


#12 N-OCTACOSANE

R.T.: 16.840 min
Delta R.T.: 0.021 min
Response: 654172
Conc: 5.48 ug/ml

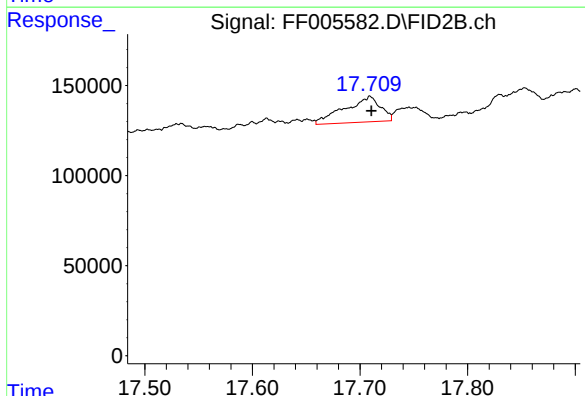


#13 N-TRIACONTANE

R.T.: 17.710 min
Delta R.T.: -0.001 min
Response: 328264
Conc: 2.71 ug/ml

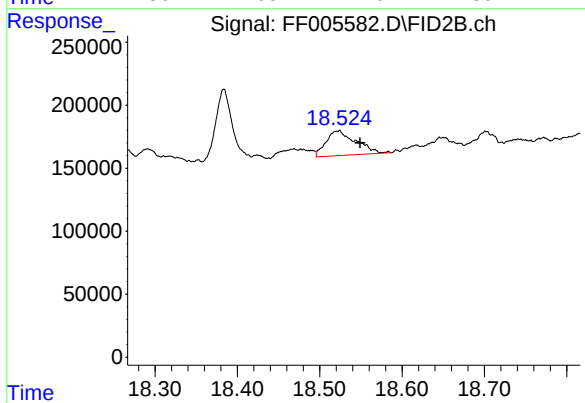

#14 N-DOTRIACONTANE


R.T.: 18.524 min
Delta R.T.: -0.025 min
Response: 499068
Conc: 4.03 ug/ml

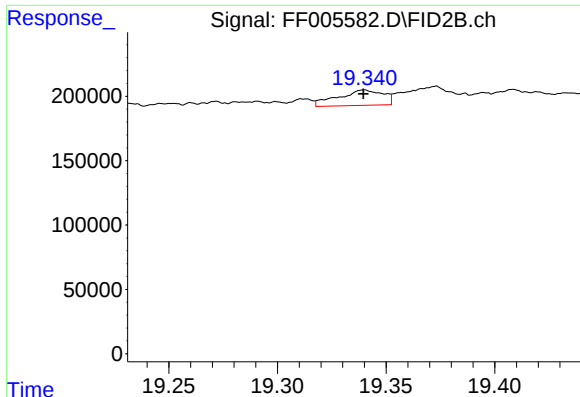

#15 N-TETRATRIACONTANE


R.T.: 19.340 min
Delta R.T.: 0.000 min
Response: 171088
Conc: 1.42 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-7

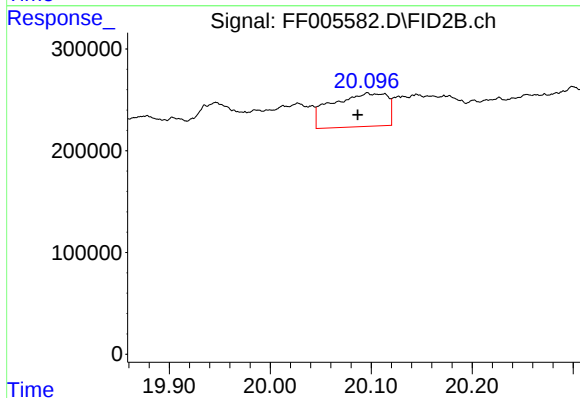

#16 N-HEXATRIACONTANE

R.T.: 20.096 min
Delta R.T.: 0.010 min
Response: 1244728
Conc: 10.37 ug/ml

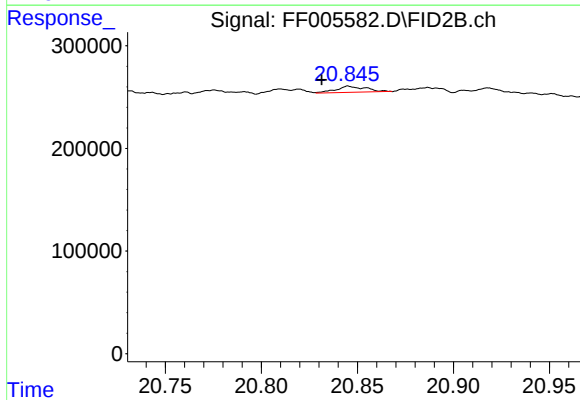

#17 N-OCTATRIACONTANE

R.T.: 20.846 min
Delta R.T.: 0.014 min
Response: 63461
Conc: 0.58 ug/ml