

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
 Data File : FF005583.D
 Signal(s) : FID2B.ch
 Acq On : 16 Sep 2019 20:34
 Operator : DD\AJ
 Sample : K4878-09 5X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CSA-2-8

Integration File: autoint1.e
 Quant Time: Sep 17 01:12:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.516	140197	1.069 ug/ml
8) N-DOCOSANE	13.760	562063	4.464 ug/ml
10) N-TETRACOSANE	14.824	2742458	22.425 ug/ml
11) N-HEXACOSANE	15.854	271504	2.268 ug/ml
12) N-OCTACOSANE	16.840	808622	6.777 ug/ml
13) N-TRIACONTANE	17.708	239951	1.984 ug/ml
14) N-DOTRIACONTANE	18.522	639531	5.159 ug/ml
15) N-TETRATRIACONTANE	19.369	366745	3.043 ug/ml
16) N-HEXATRIACONTANE	20.087	660693	5.505 ug/ml
18) N-TETRACONTANE	21.737	105402	0.829 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091619\
 Data File : FF005583.D
 Signal(s) : FID2B.ch
 Acq On : 16 Sep 2019 20:34
 Operator : DD\AJ
 Sample : K4878-09 5X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampled :
 CSA-2-8

Integration File: autoint1.e
 Quant Time: Sep 17 01:12:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

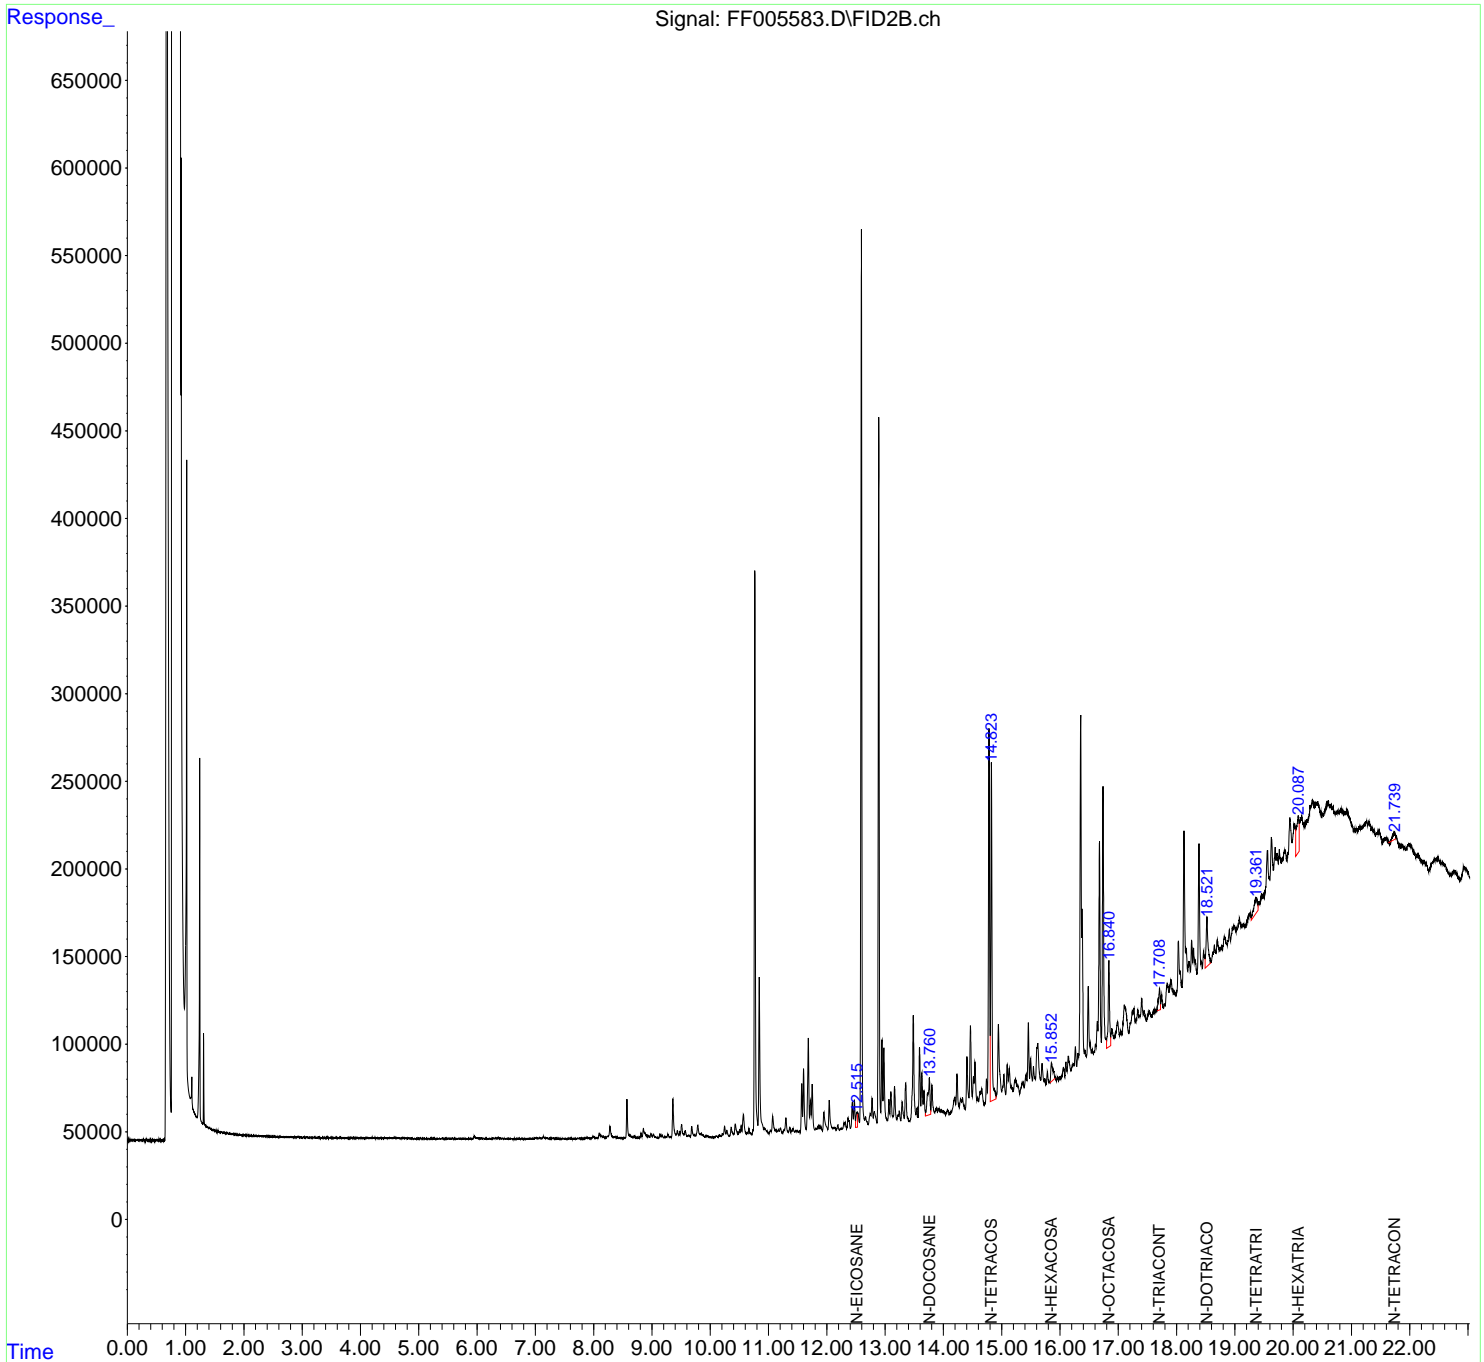

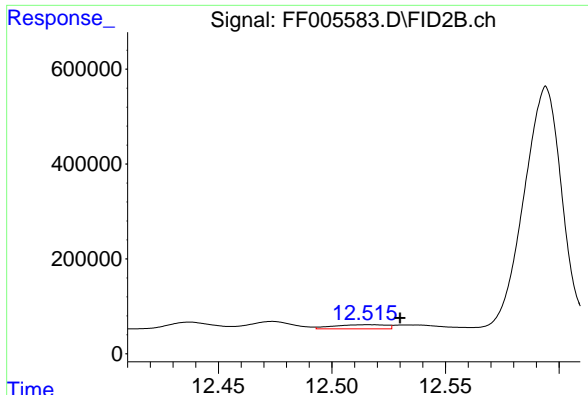


#7 N-EICOSANE
 R.T.: 12.516 min
 Delta R.T.: -0.014 min
 Response: 140197
 Conc: 1.07 ug/ml


Instrument :
 FID_F
 ClientSampleId :
 CSA-2-8

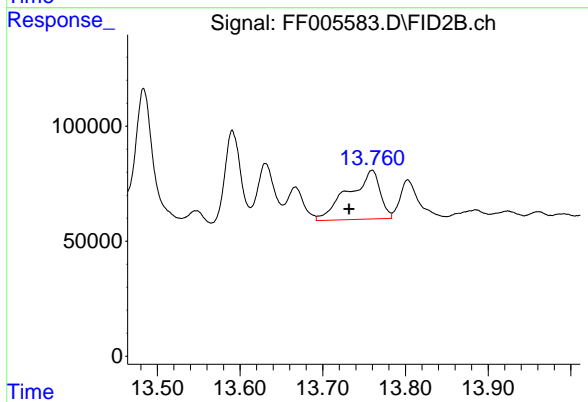


#8 N-DOCOSANE
 R.T.: 13.760 min
 Delta R.T.: 0.028 min
 Response: 562063
 Conc: 4.46 ug/ml

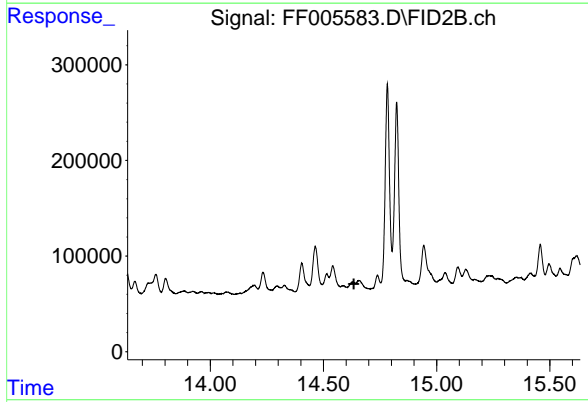

#9 TETRACOSANE-d50 (SURROGATE)
 R.T.: 0.000 min
 Exp R.T. : 14.635 min
 Response: 0
 Conc: N.D.

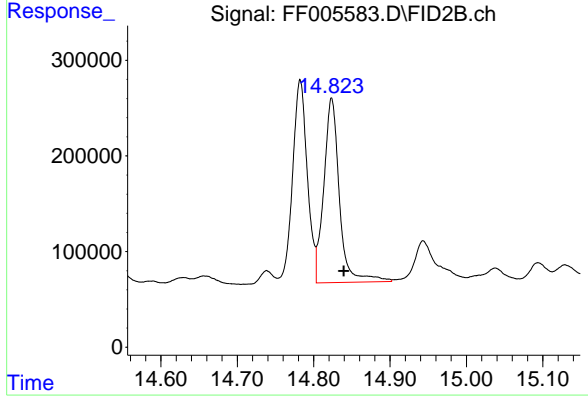


#10 N-TETRACOSANE
 R.T.: 14.824 min
 Delta R.T.: -0.016 min
 Response: 2742458
 Conc: 22.42 ug/ml

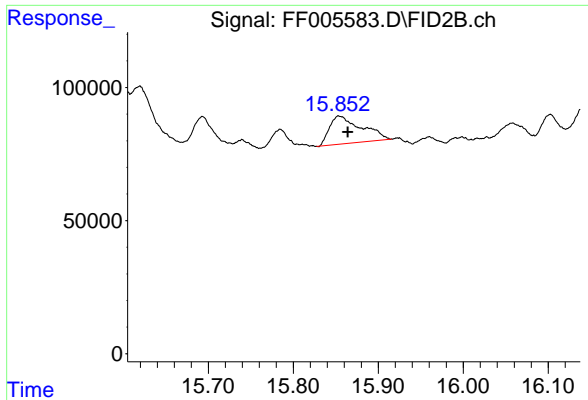

#11 N-HEXACOSANE


R.T.: 15.854 min
Delta R.T.: -0.011 min
Response: 271504
Conc: 2.27 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-8

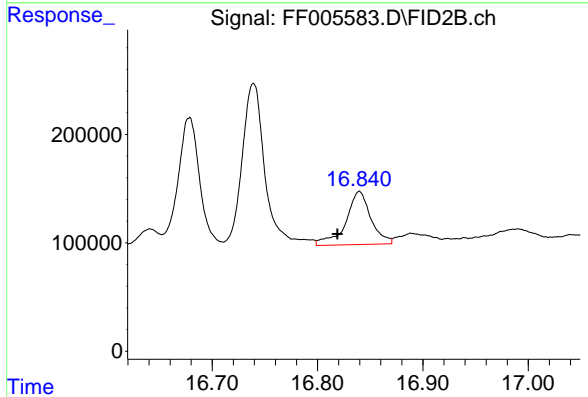


#12 N-OCTACOSANE

R.T.: 16.840 min
Delta R.T.: 0.021 min
Response: 808622
Conc: 6.78 ug/ml

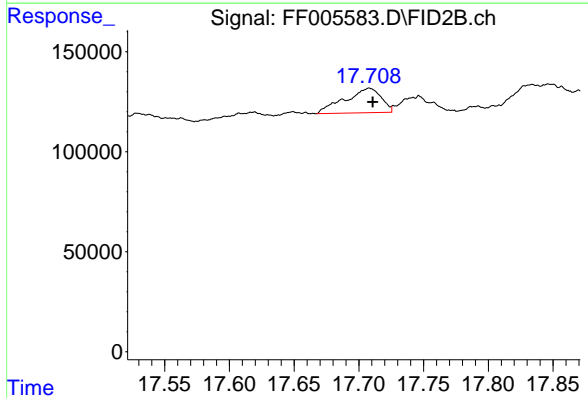


#13 N-TRIACONTANE

R.T.: 17.708 min
Delta R.T.: -0.002 min
Response: 239951
Conc: 1.98 ug/ml

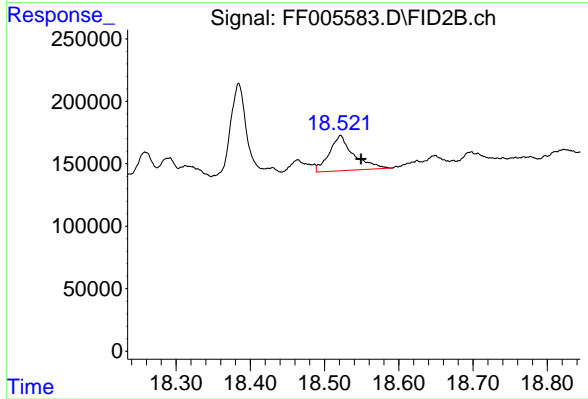

#14 N-DOTRIACONTANE

R.T.: 18.522 min
Delta R.T.: -0.027 min
Response: 639531
Conc: 5.16 ug/ml

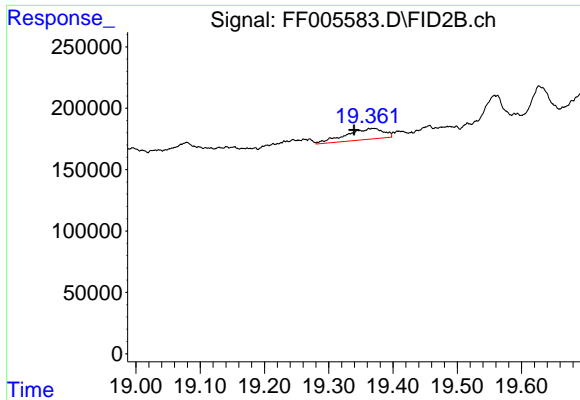

#15 N-TETRATRIACONTANE


R.T.: 19.369 min

Delta R.T.: 0.030 min

Response: 366745

Conc: 3.04 ug/ml

Instrument :
FID_F
ClientSampled :
CSA-2-8

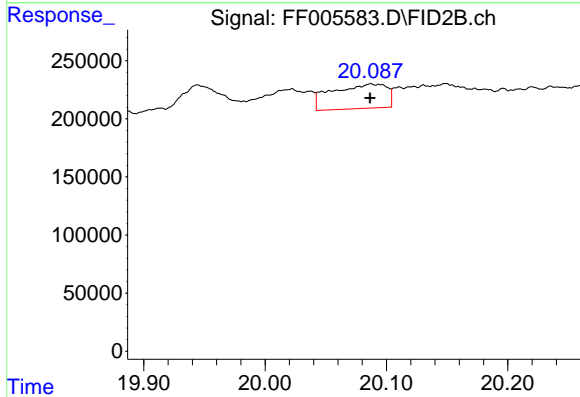


#16 N-HEXATRIACONTANE

R.T.: 20.087 min

Delta R.T.: 0.000 min

Response: 660693

Conc: 5.50 ug/ml

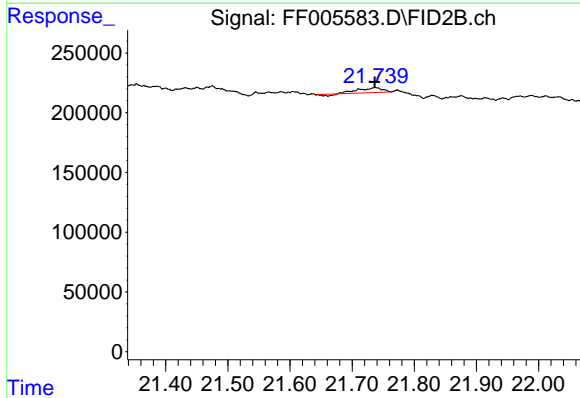

#18 N-TETRACONTANE

R.T.: 21.737 min

Delta R.T.: 0.000 min

Response: 105402

Conc: 0.83 ug/ml