

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
 Data File : FF005589.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2019 10:33
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Sep 18 00:51:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.583f	545704	5.100 ug/ml
Target Compounds			
3) N-DODECANE	6.361	3659543	25.529 ug/ml
11) N-HEXACOSANE	15.856	125427	1.048 ug/ml
12) N-OCTACOSANE	16.815	4247451	35.596 ug/ml
13) N-TRIACONTANE	17.708	450155	3.721 ug/ml
14) N-DOTRIACONTANE	18.549	504024	4.066 ug/ml
15) N-TETRATRIACONTANE	19.342	362720	3.010 ug/ml
16) N-HEXATRIACONTANE	20.091	186400	1.553 ug/ml
17) N-OCTATRIACONTANE	20.839	206907	1.896 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
Data File : FF005589.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2019 10:33
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 18 00:51:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

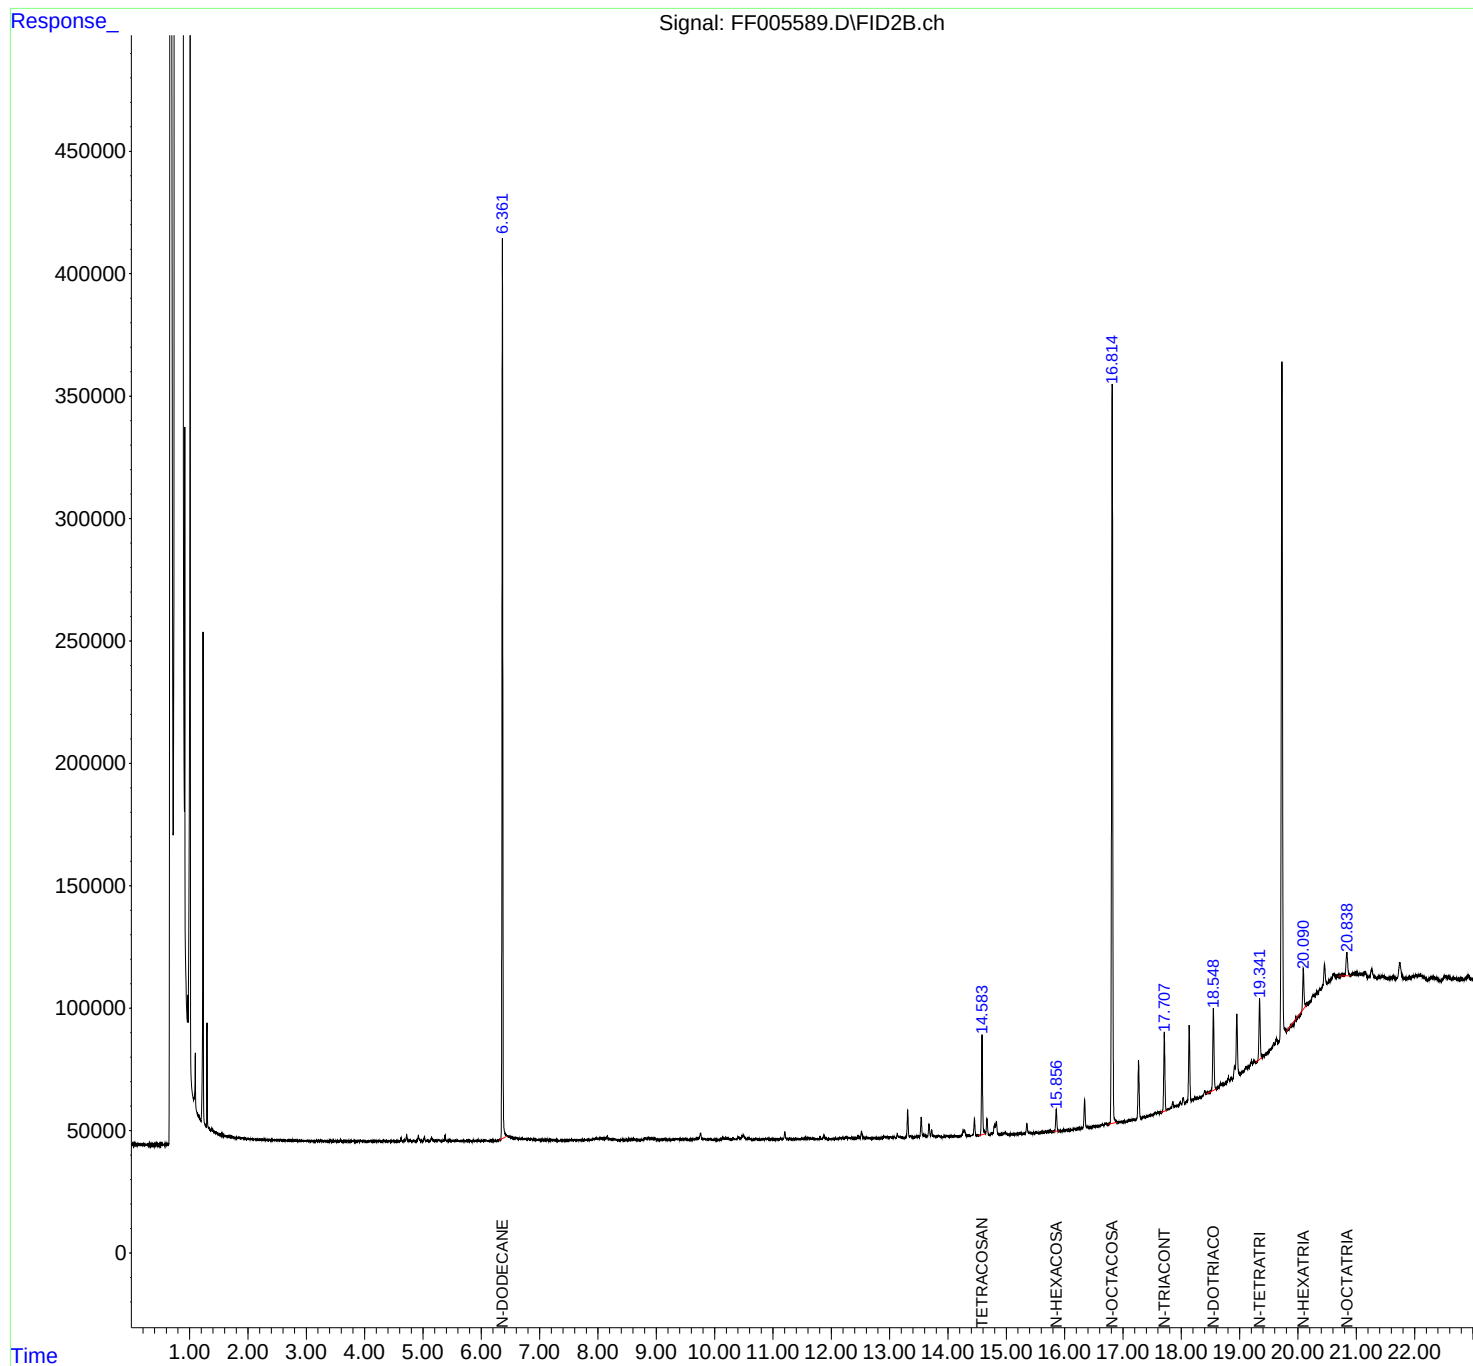


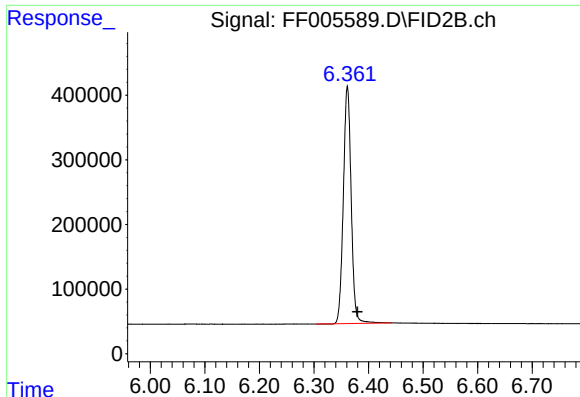

#3 N-DODECANE


R.T.: 6.361 min
Delta R.T.: -0.018 min
Response: 3659543
Conc: 25.53 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

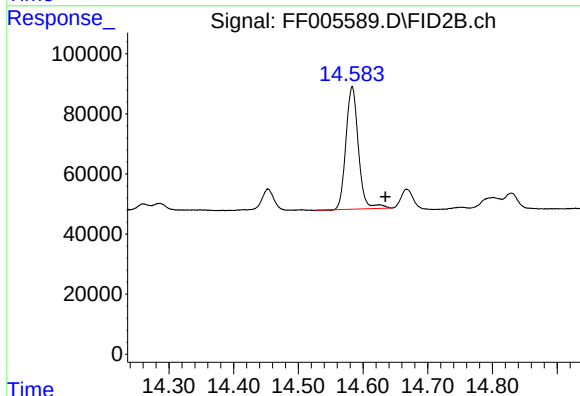


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.583 min
Delta R.T.: -0.051 min
Response: 545704
Conc: 5.10 ug/ml

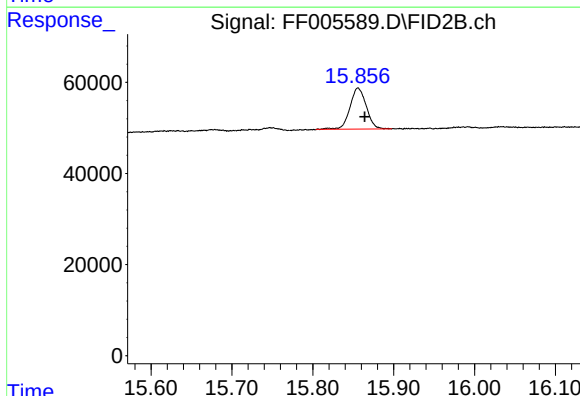


#11 N-HEXACOSANE

R.T.: 15.856 min
Delta R.T.: -0.008 min
Response: 125427
Conc: 1.05 ug/ml

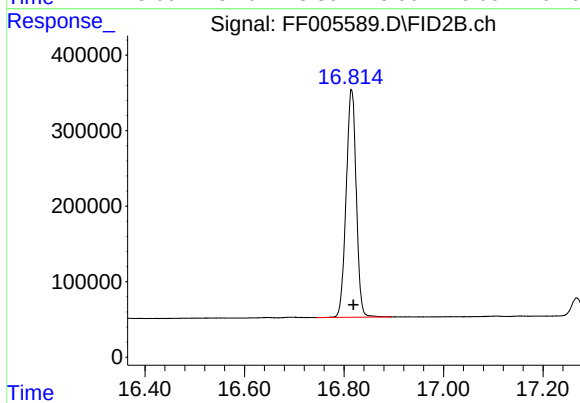

#12 N-OCTACOSANE


R.T.: 16.815 min
Delta R.T.: -0.004 min
Response: 4247451
Conc: 35.60 ug/ml

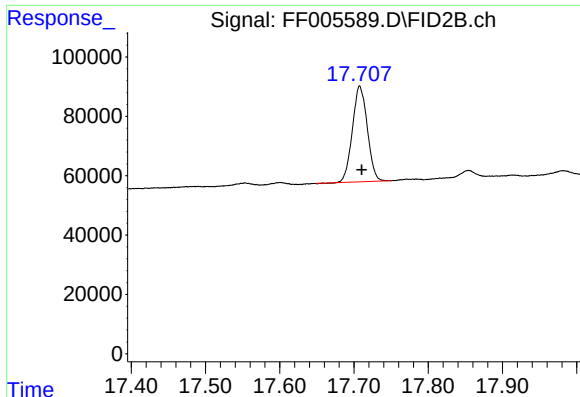

#13 N-TRIACONTANE


R.T.: 17.708 min
Delta R.T.: -0.003 min
Response: 450155
Conc: 3.72 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

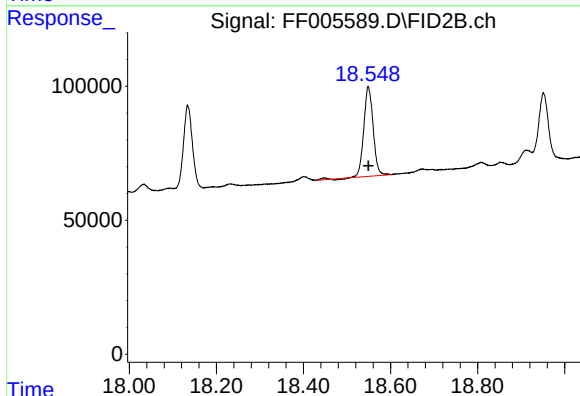


#14 N-DOTRIACONTANE

R.T.: 18.549 min
Delta R.T.: 0.000 min
Response: 504024
Conc: 4.07 ug/ml

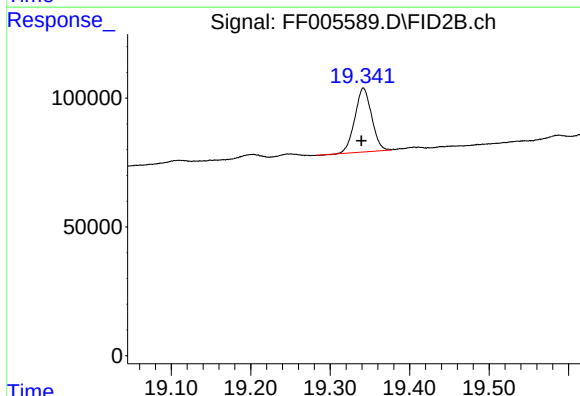


#15 N-TETRATRIACONTANE

R.T.: 19.342 min
Delta R.T.: 0.002 min
Response: 362720
Conc: 3.01 ug/ml

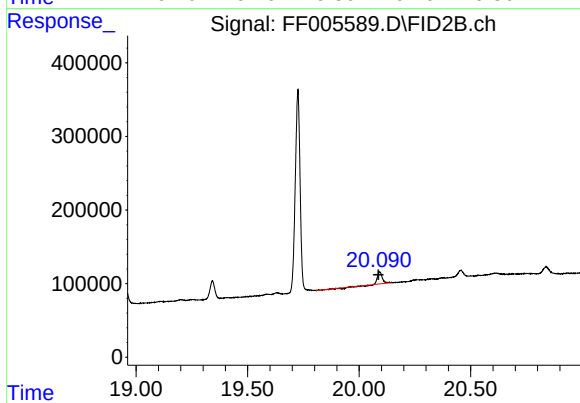

#16 N-HEXATRIACONTANE

R.T.: 20.091 min
Delta R.T.: 0.005 min
Response: 186400
Conc: 1.55 ug/ml

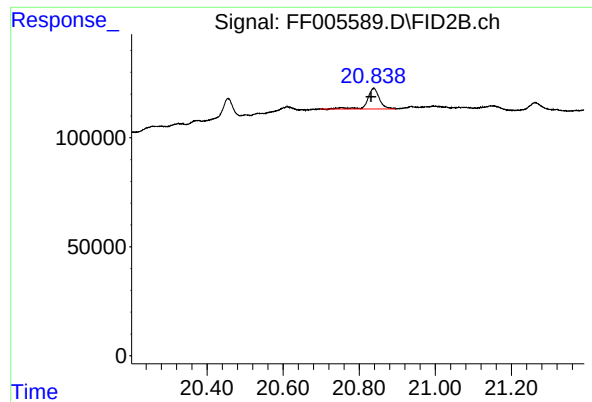

#17 N-OCTATRIACONTANE

R.T.: 20.839 min
Delta R.T.: 0.007 min
Response: 206907
Conc: 1.90 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER