

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
 Data File : FF005593.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2019 14:58
 Operator : DD\AJ
 Sample : K4863-13 2X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CSA-2-5

Integration File: autoint1.e
 Quant Time: Sep 18 00:52:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.628	135415	1.265 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.890	154008	1.287 ug/ml
12) N-OCTACOSANE	16.841	1171088	9.814 ug/ml
13) N-TRIACONTANE	17.713	2167272	17.916 ug/ml
14) N-DOTRIACONTANE	18.563	1044260	8.424 ug/ml
15) N-TETRATRIACONTANE	19.310	365254	3.031 ug/ml
16) N-HEXATRIACONTANE	20.107	1638859	13.654 ug/ml
17) N-OCTATRIACONTANE	20.854	633153	5.803 ug/ml
18) N-TETRACONTANE	21.746	569351	4.478 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
Data File : FF005593.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2019 14:58
Operator : DD\AJ
Sample : K4863-13 2X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSA-2-5

Integration File: autoint1.e
Quant Time: Sep 18 00:52:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

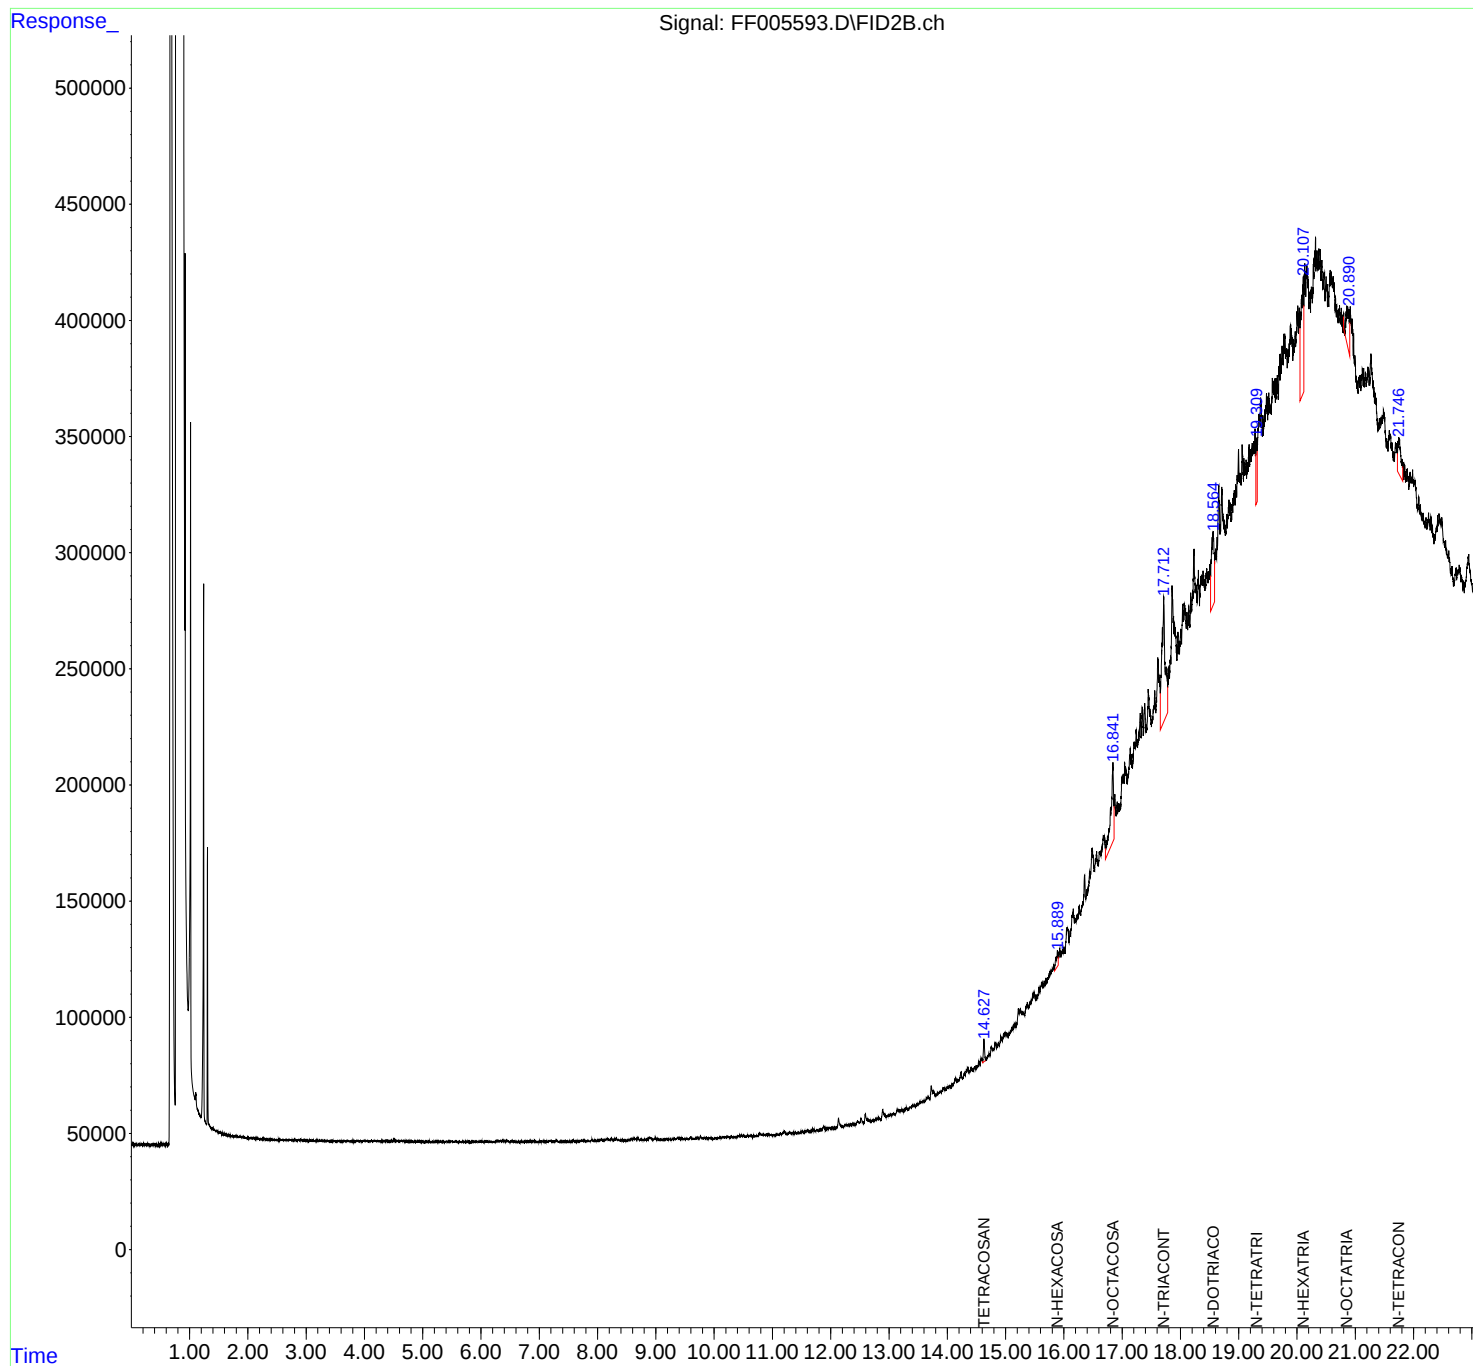


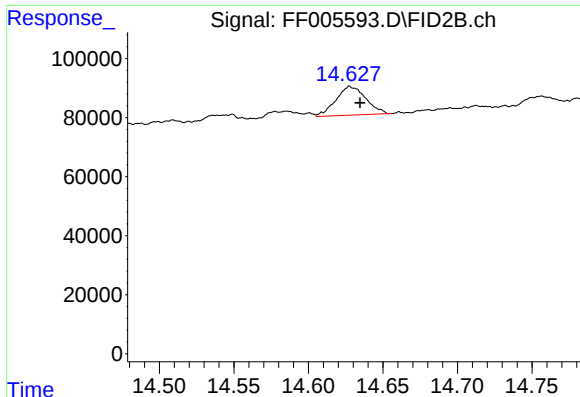

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.628 min
Delta R.T.: -0.007 min
Response: 135415
Conc: 1.27 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-5

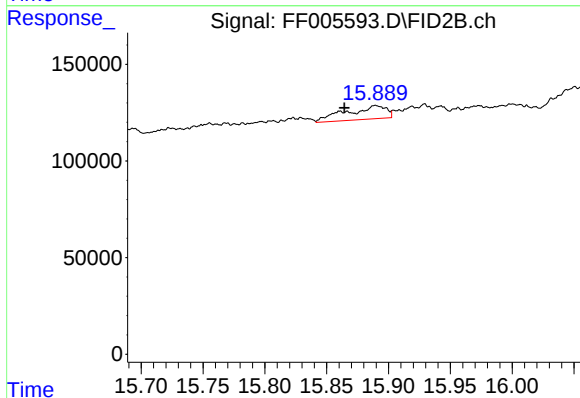


#11 N-HEXACOSANE

R.T.: 15.890 min
Delta R.T.: 0.025 min
Response: 154008
Conc: 1.29 ug/ml

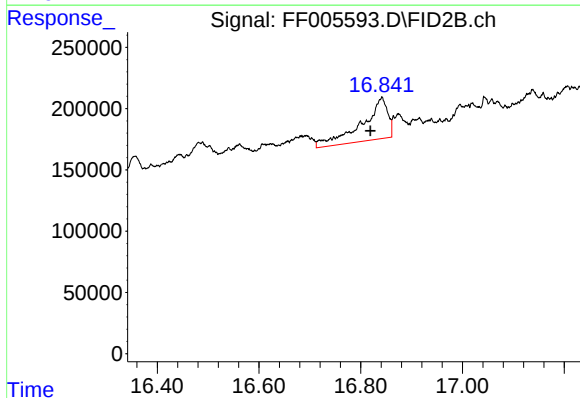


#12 N-OCTACOSANE

R.T.: 16.841 min
Delta R.T.: 0.022 min
Response: 1171088
Conc: 9.81 ug/ml

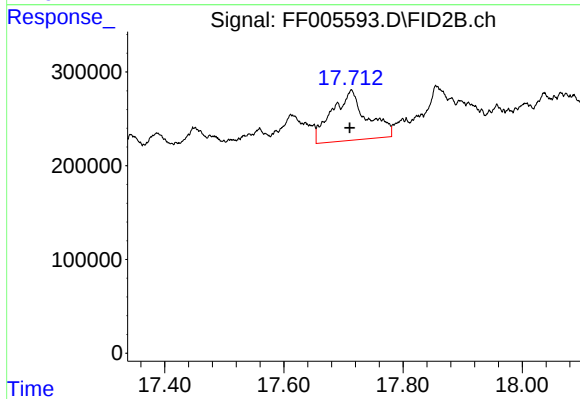

#13 N-TRIACONTANE


R.T.: 17.713 min
Delta R.T.: 0.003 min
Response: 2167272
Conc: 17.92 ug/ml

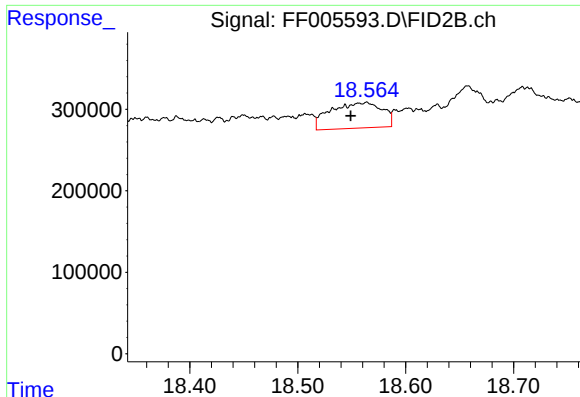

#14 N-DOTRIACONTANE


R.T.: 18.563 min
Delta R.T.: 0.014 min
Response: 1044260
Conc: 8.42 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-5

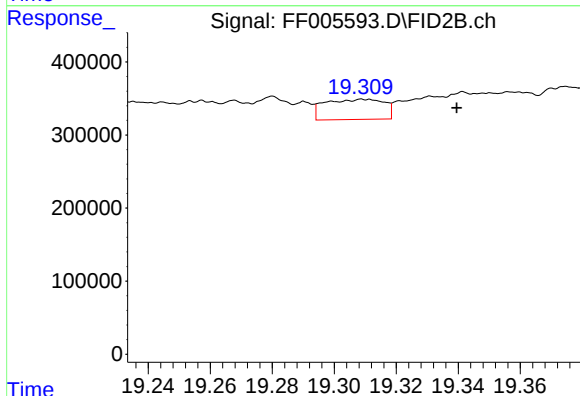


#15 N-TETRATRIACONTANE

R.T.: 19.310 min
Delta R.T.: -0.030 min
Response: 365254
Conc: 3.03 ug/ml

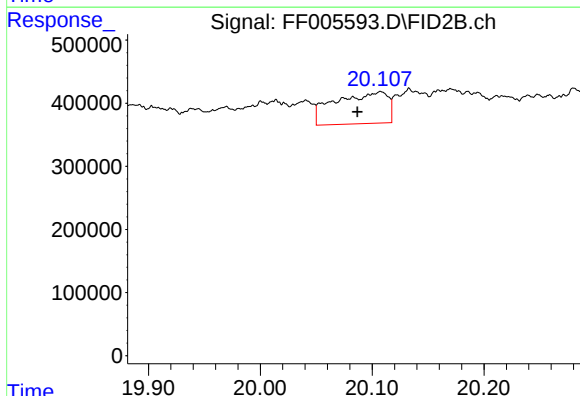


#16 N-HEXATRIACONTANE

R.T.: 20.107 min
Delta R.T.: 0.021 min
Response: 1638859
Conc: 13.65 ug/ml

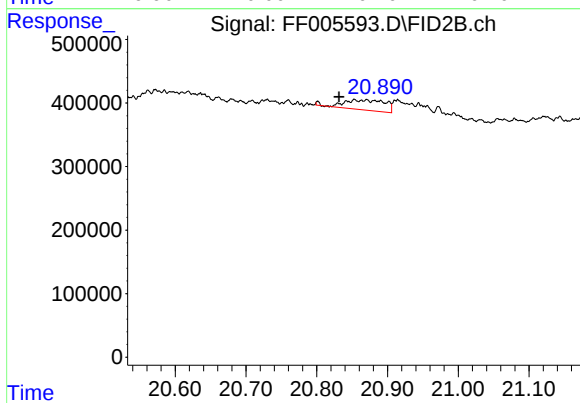

#17 N-OCTATRIACONTANE

R.T.: 20.854 min
Delta R.T.: 0.022 min
Response: 633153
Conc: 5.80 ug/ml

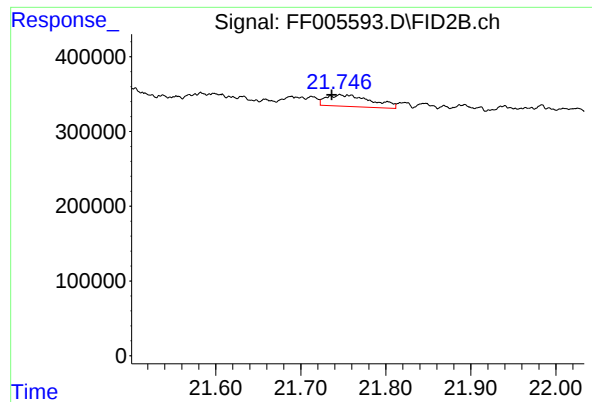

#18 N-TETRACONTANE

R.T.: 21.746 min
Delta R.T.: 0.010 min
Response: 569351
Conc: 4.48 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-5