

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
 Data File : FF005594.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2019 15:27
 Operator : DD\AJ
 Sample : K4877-06 2X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CSA-2-3

Integration File: autoint1.e
 Quant Time: Sep 18 00:53:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	148516	1.388 ug/ml
Target Compounds			
7) N-EICOSANE	12.594f	121847	0.929 ug/ml
10) N-TETRACOSANE	14.827	119463	0.977 ug/ml
11) N-HEXACOSANE	15.883	77288	0.646 ug/ml
12) N-OCTACOSANE	16.839	607412	5.090 ug/ml
13) N-TRIACONTANE	17.712	1265224	10.459 ug/ml
14) N-DOTRIACONTANE	18.554	771381	6.223 ug/ml
15) N-TETRATRIACONTANE	19.339	1335532	11.083 ug/ml
16) N-HEXATRIACONTANE	20.096	1913576	15.943 ug/ml
17) N-OCTATRIACONTANE	20.838	1024153	9.387 ug/ml
18) N-TETRACONTANE	21.750	517900	4.074 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
Data File : FF005594.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2019 15:27
Operator : DD\AJ
Sample : K4877-06 2X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
CSA-2-3

Integration File: autoint1.e
Quant Time: Sep 18 00:53:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

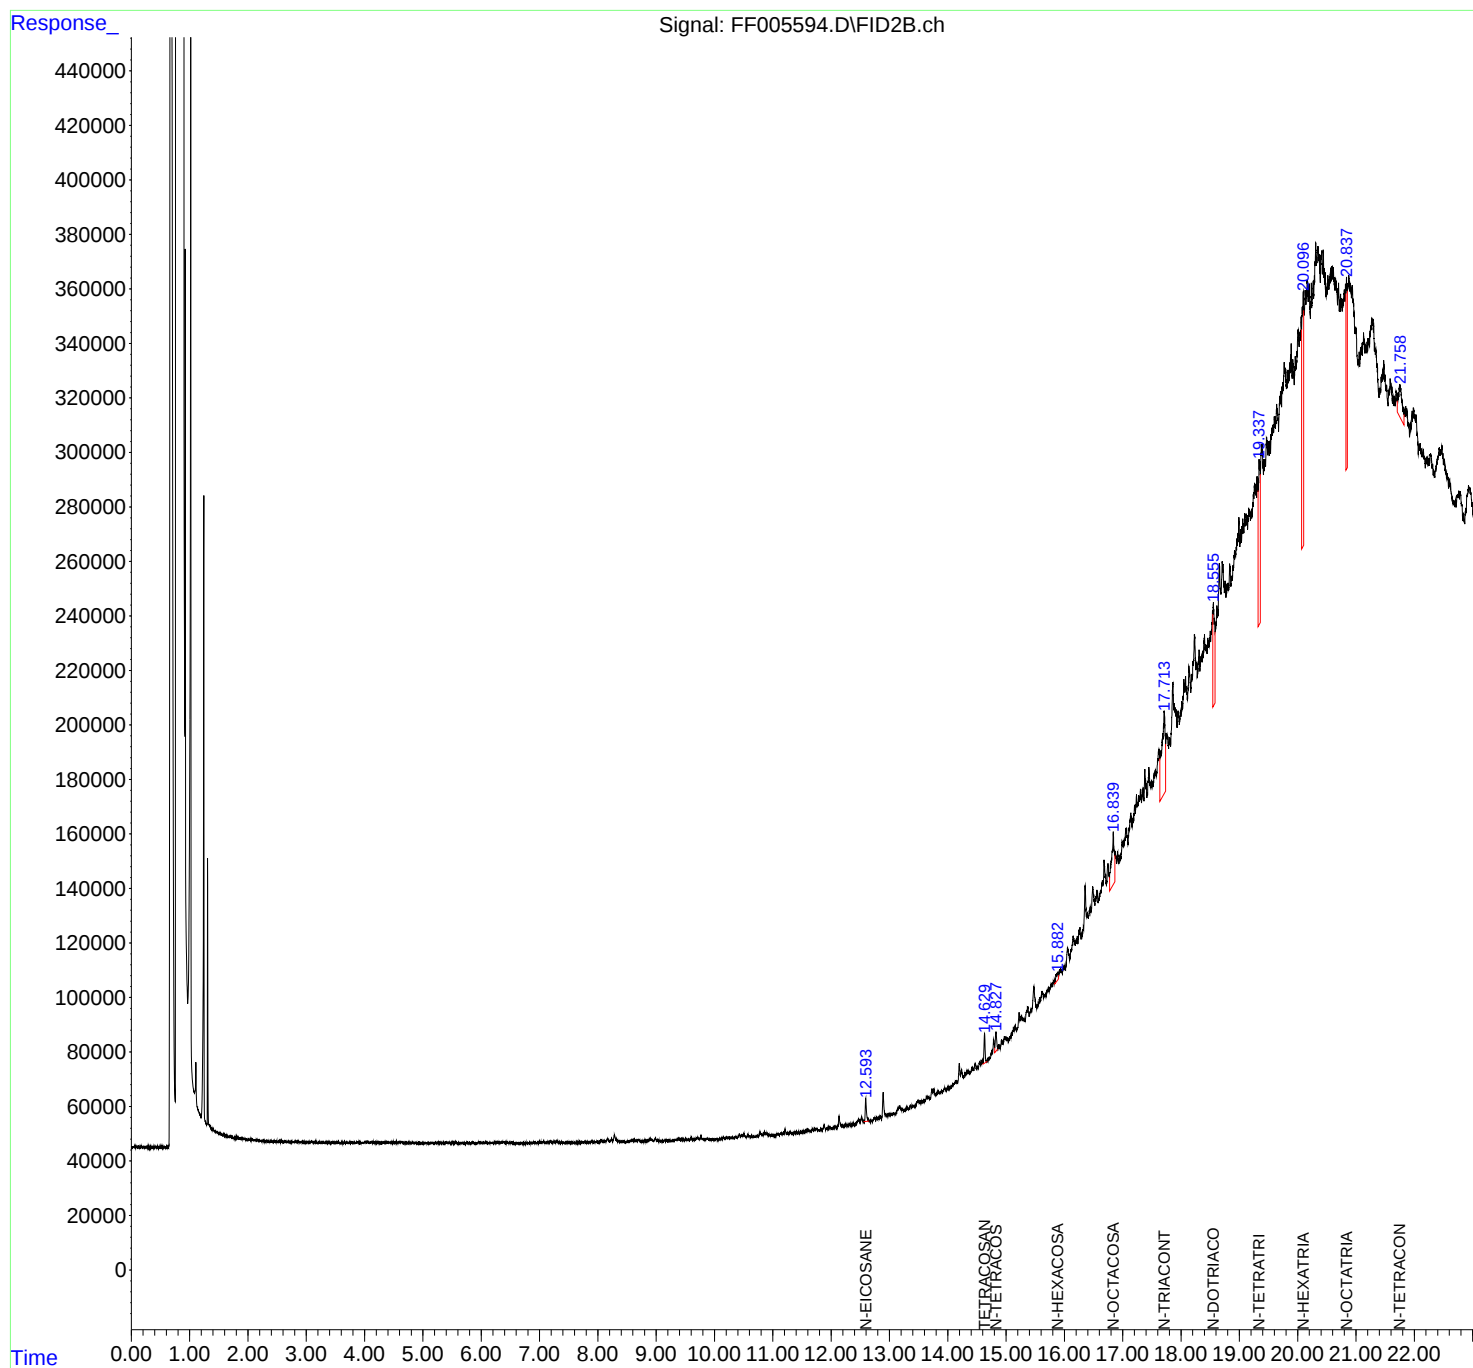


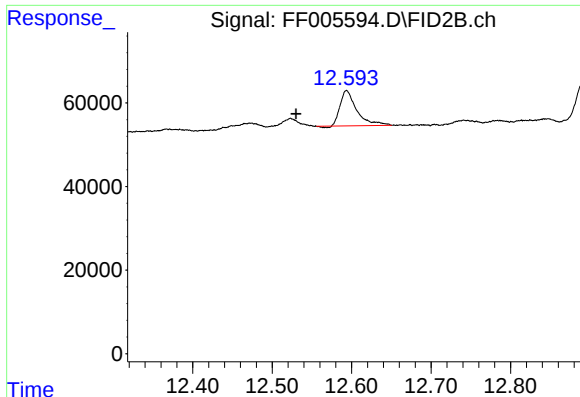

#7 N-EICOSANE


R.T.: 12.594 min
Delta R.T.: 0.064 min
Response: 121847
Conc: 0.93 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-3

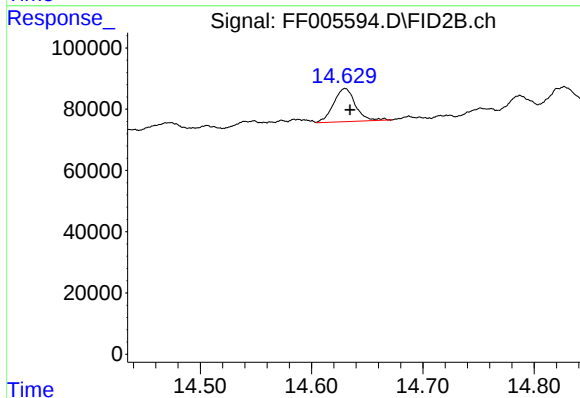


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.630 min
Delta R.T.: -0.004 min
Response: 148516
Conc: 1.39 ug/ml

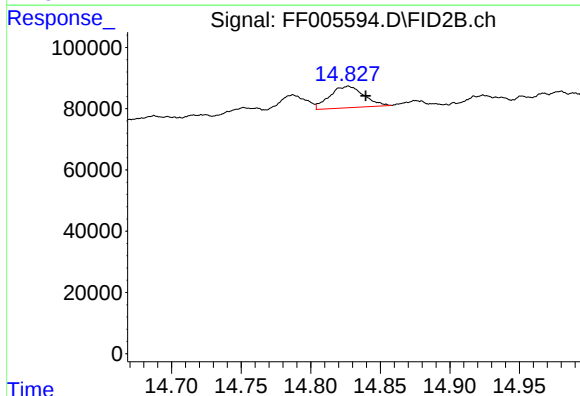


#10 N-TETRACOSANE

R.T.: 14.827 min
Delta R.T.: -0.012 min
Response: 119463
Conc: 0.98 ug/ml

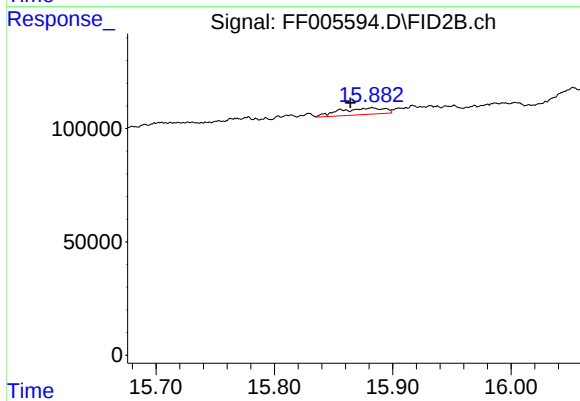

#11 N-HEXACOSANE


R.T.: 15.883 min
Delta R.T.: 0.018 min
Response: 77288
Conc: 0.65 ug/ml

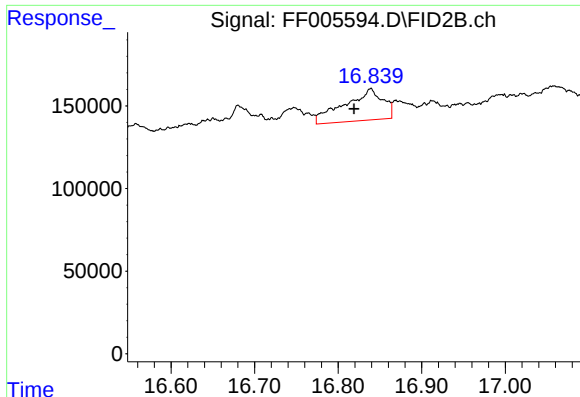

#12 N-OCTACOSANE


R.T.: 16.839 min
Delta R.T.: 0.020 min
Response: 607412
Conc: 5.09 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-3

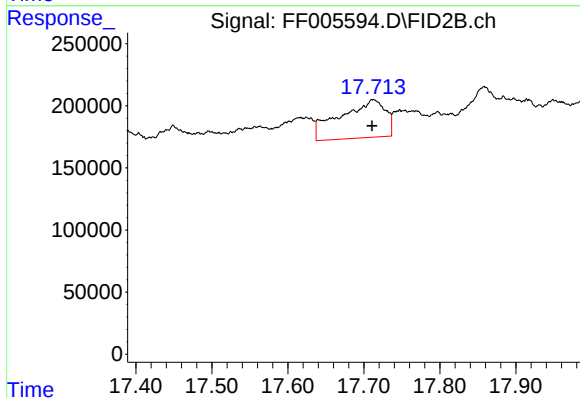


#13 N-TRIACONTANE

R.T.: 17.712 min
Delta R.T.: 0.001 min
Response: 1265224
Conc: 10.46 ug/ml

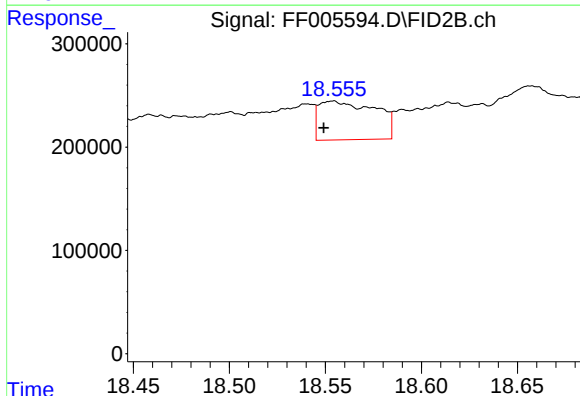


#14 N-DOTRIACONTANE

R.T.: 18.554 min
Delta R.T.: 0.005 min
Response: 771381
Conc: 6.22 ug/ml

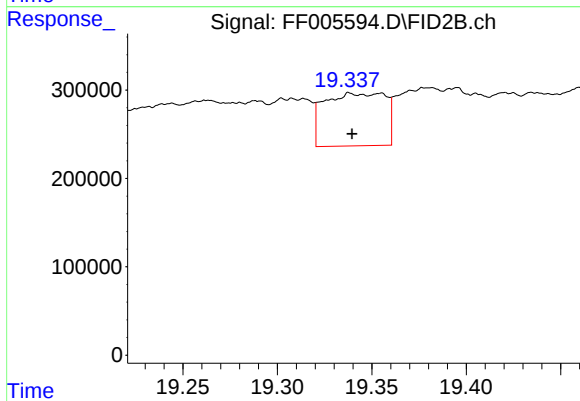

#15 N-TETRATRIACONTANE


R.T.: 19.339 min
Delta R.T.: 0.000 min
Response: 1335532
Conc: 11.08 ug/ml

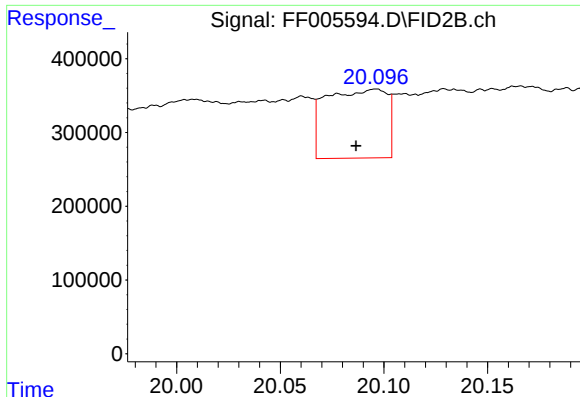

#16 N-HEXATRIACONTANE


R.T.: 20.096 min
Delta R.T.: 0.009 min
Response: 1913576
Conc: 15.94 ug/ml

Instrument :
FID_F
ClientSampleId :
CSA-2-3

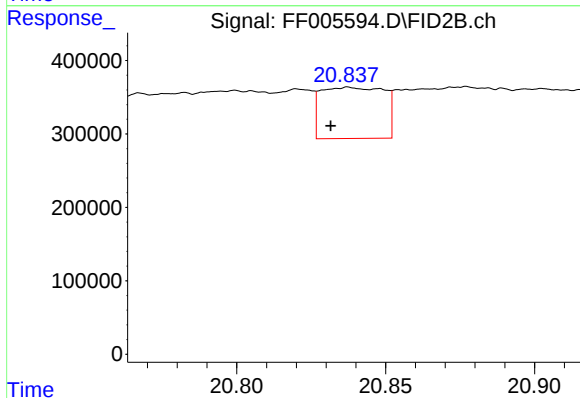

#17 N-OCTATRIACONTANE

R.T.: 20.838 min
Delta R.T.: 0.006 min
Response: 1024153
Conc: 9.39 ug/ml

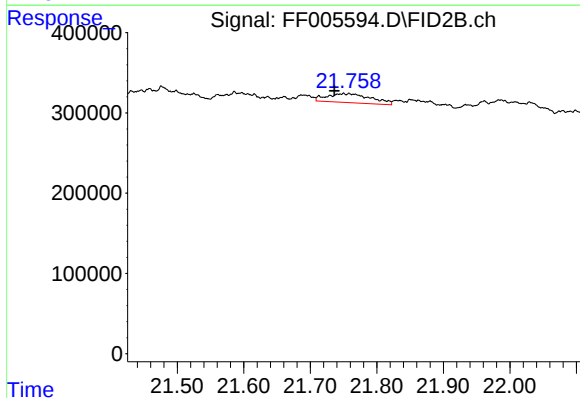

#18 N-TETRACONTANE

R.T.: 21.750 min
Delta R.T.: 0.014 min
Response: 517900
Conc: 4.07 ug/ml