

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
Data File : FF005595.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2019 15:57
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Sep 18 00:53:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13)	N-TRIACONTANE	17.711	91349	0.755 ug/ml
15)	N-TETRATRIACONTANE	19.340	333487	2.767 ug/ml
16)	N-HEXATRIACONTANE	20.096	706756	5.888 ug/ml
17)	N-OCTATRIACONTANE	20.882f	4372177	40.074 ug/ml
18)	N-TETRACONTANE	21.742	433335	3.408 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
Data File : FF005595.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2019 15:57
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Sep 18 00:53:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

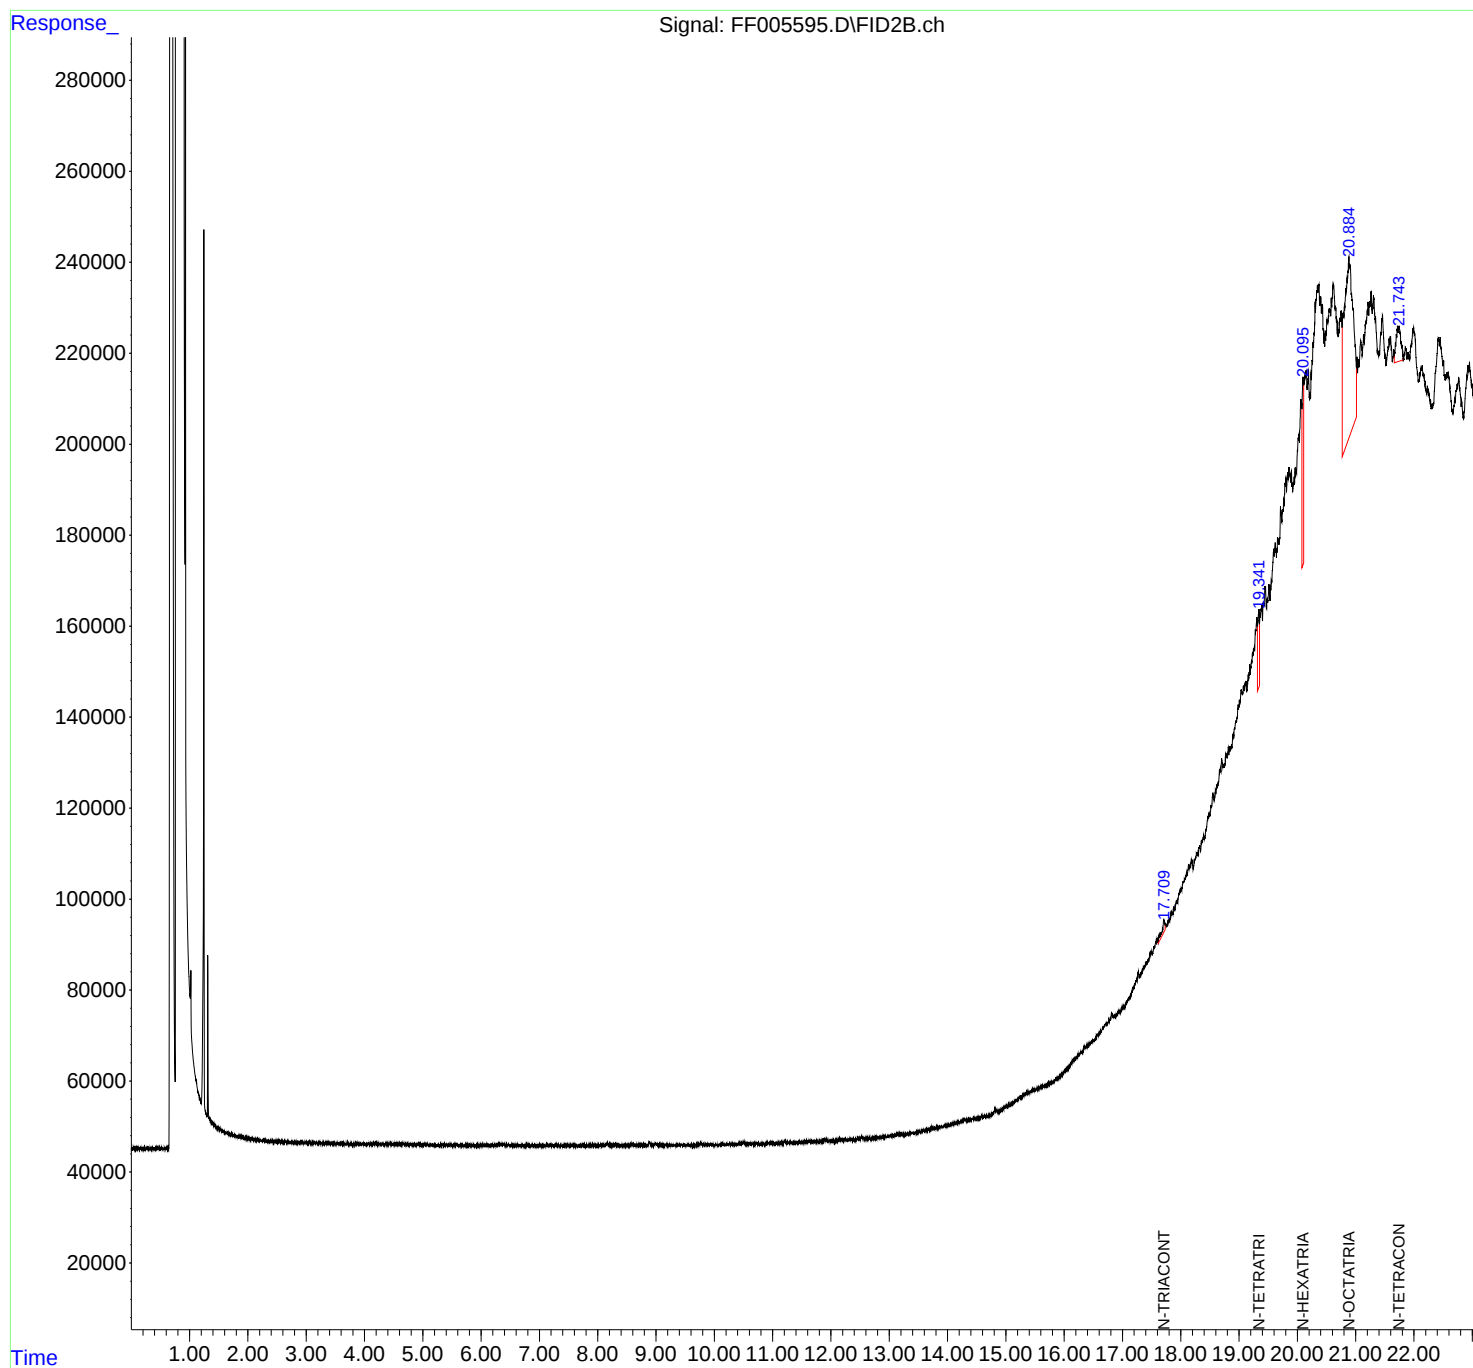


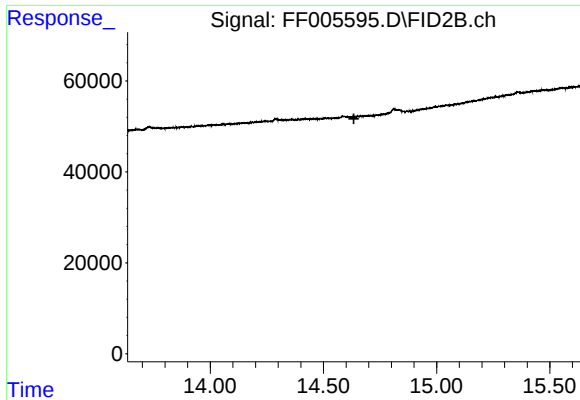

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.635 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
MECL2

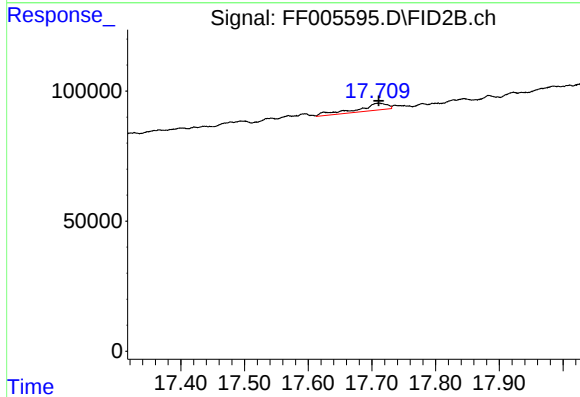


#13 N-TRIACONTANE

R.T.: 17.711 min
Delta R.T.: 0.000 min
Response: 91349
Conc: 0.76 ug/ml

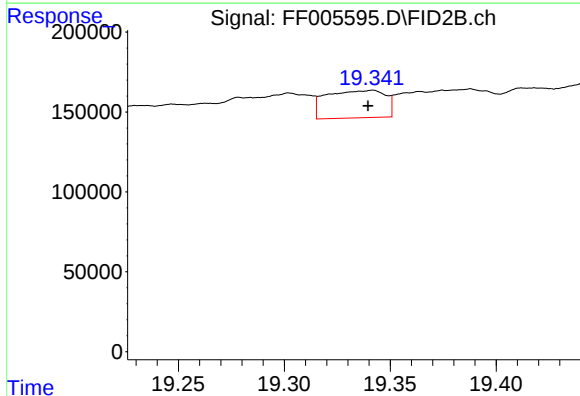


#15 N-TETRATRIACONTANE

R.T.: 19.340 min
Delta R.T.: 0.000 min
Response: 333487
Conc: 2.77 ug/ml

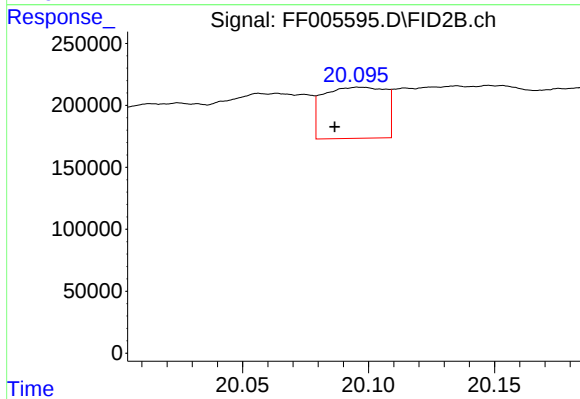

#16 N-HEXATRIACONTANE


R.T.: 20.096 min
Delta R.T.: 0.010 min
Response: 706756
Conc: 5.89 ug/ml

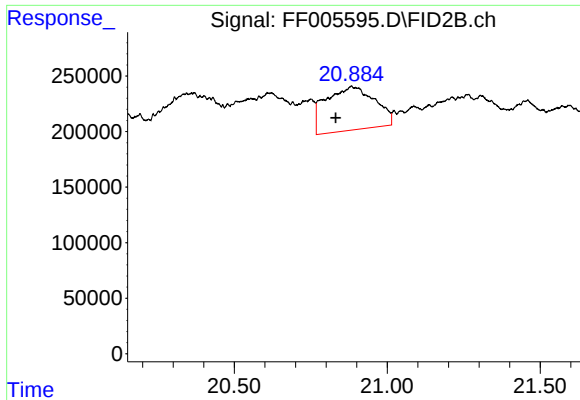

#17 N-OCTATRIACONTANE

R.T.: 20.882 min
Delta R.T.: 0.051 min
Response: 4372177
Conc: 40.07 ug/ml

Instrument :
FID_F
ClientSampleId :
MECL2

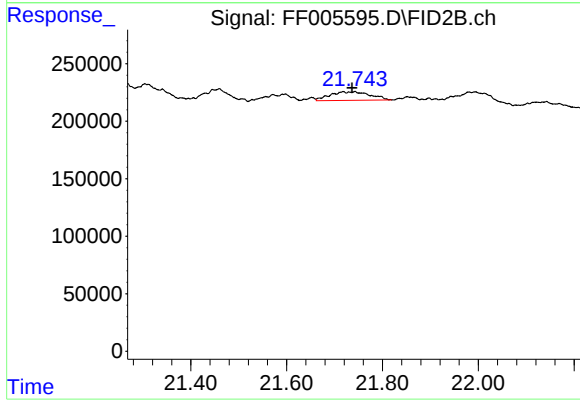

#18 N-TETRACONTANE

R.T.: 21.742 min
Delta R.T.: 0.006 min
Response: 433335
Conc: 3.41 ug/ml