

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
 Data File : FF005596.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2019 16:29
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 18 00:53:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	1954574	18.266 ug/ml
Target Compounds			
15) N-TETRATRIACONTANE	19.345	168993	1.402 ug/ml
16) N-HEXATRIACONTANE	20.121	285369	2.378 ug/ml
17) N-OCTATRIACONTANE	20.843	117689	1.079 ug/ml
18) N-TETRACONTANE	21.767	189297	1.489 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
Data File : FF005596.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2019 16:29
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Sep 18 00:53:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

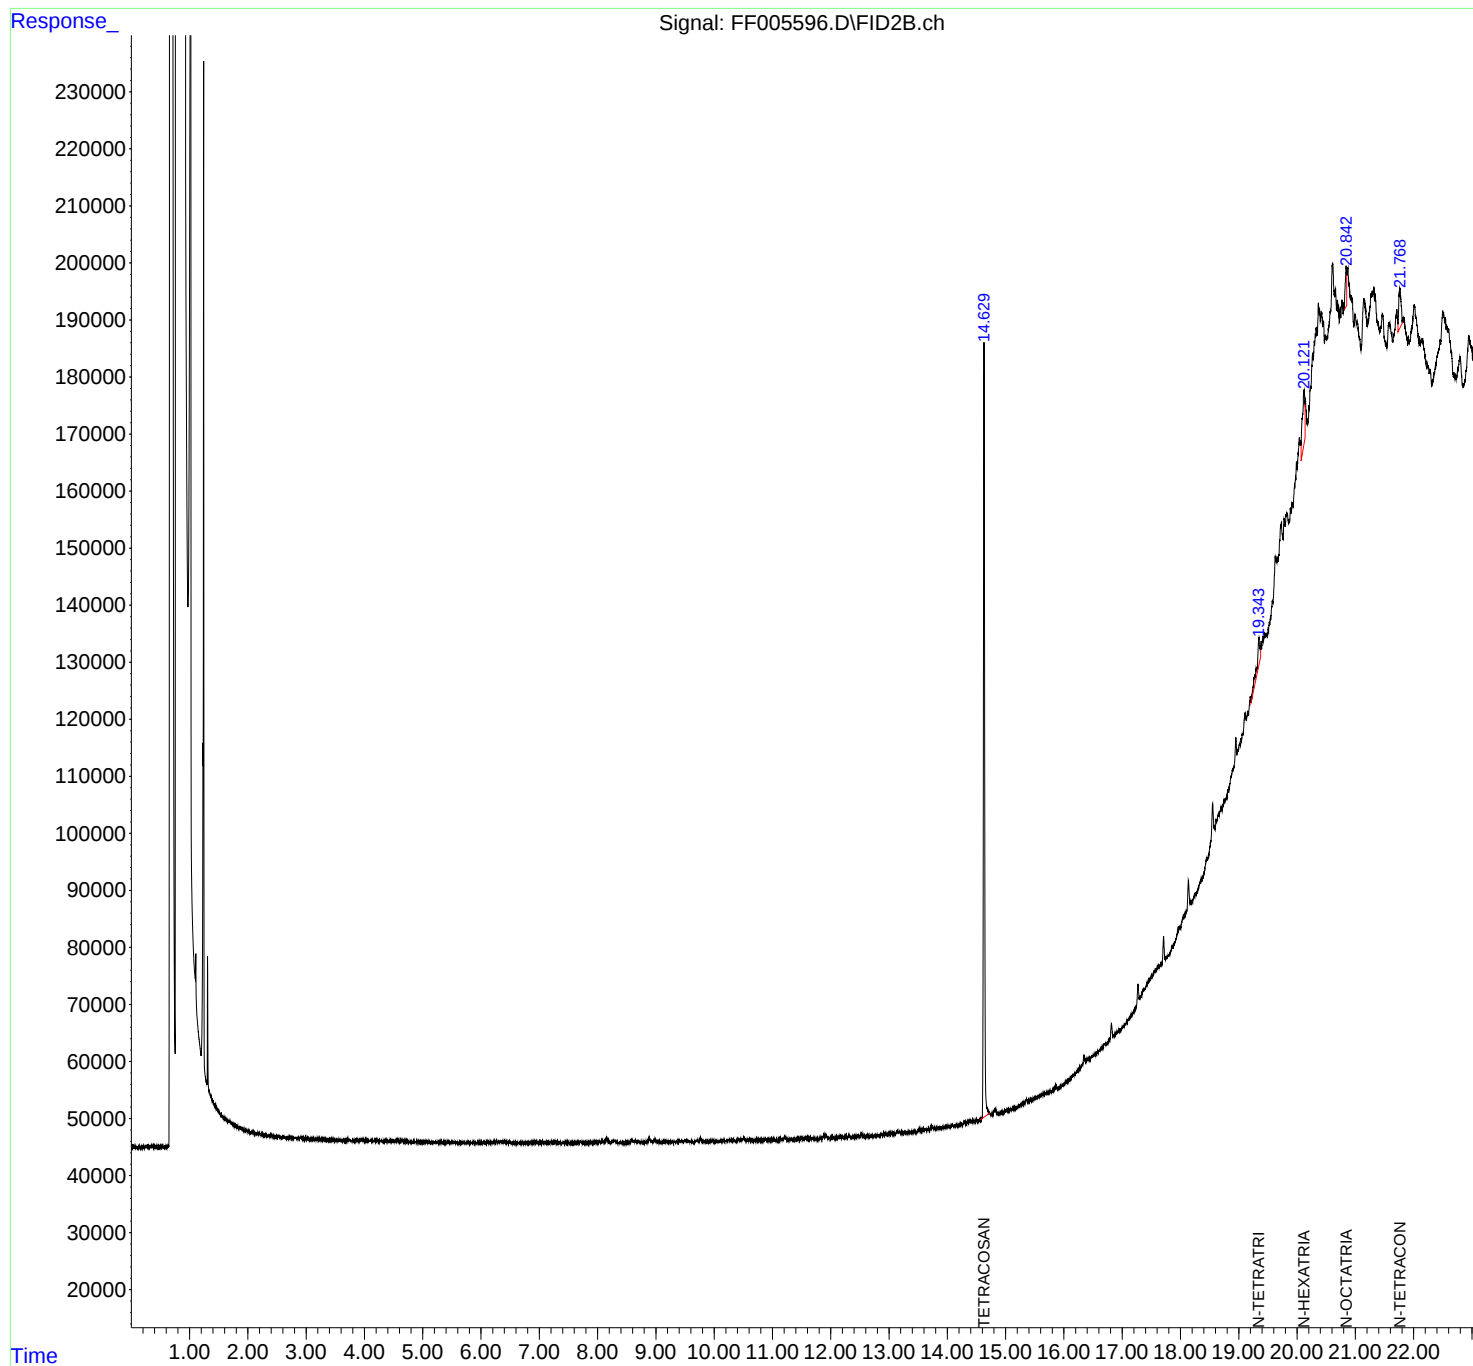


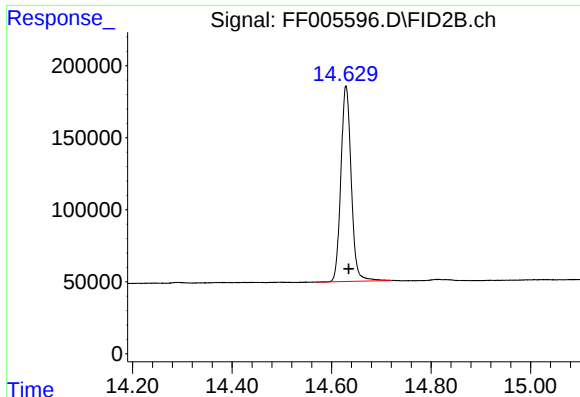

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.629 min
Delta R.T.: -0.006 min
Response: 1954574
Conc: 18.27 ug/ml

Instrument :
FID_F
ClientSampleId :

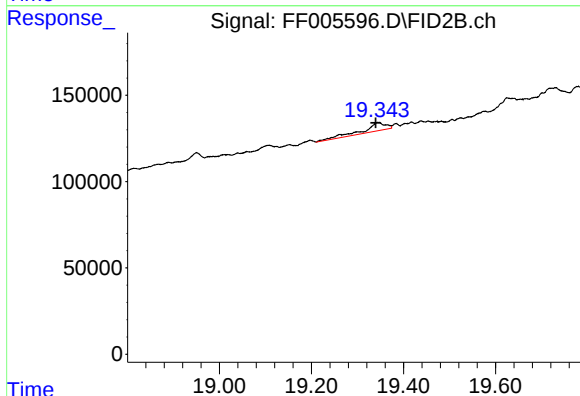


#15 N-TETRATRIACONTANE

R.T.: 19.345 min
Delta R.T.: 0.006 min
Response: 168993
Conc: 1.40 ug/ml

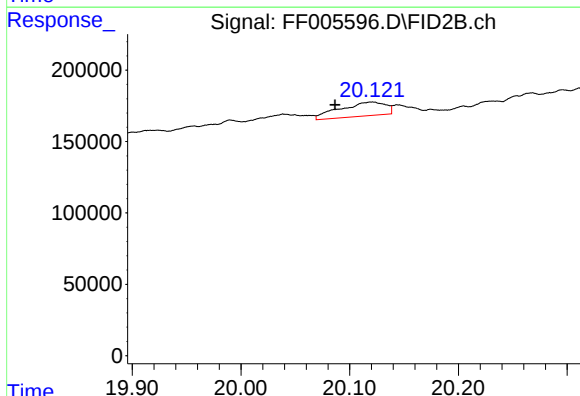


#16 N-HEXATRIACONTANE

R.T.: 20.121 min
Delta R.T.: 0.034 min
Response: 285369
Conc: 2.38 ug/ml

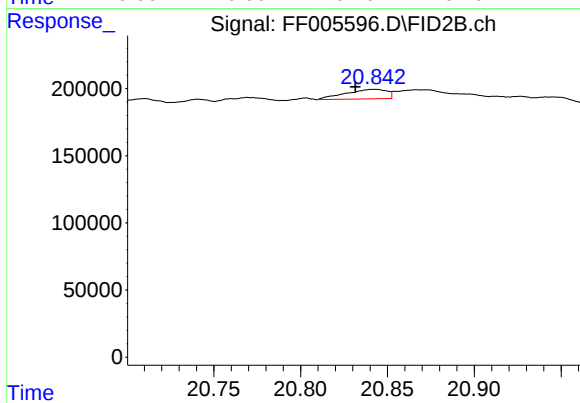

#17 N-OCTATRIACONTANE

R.T.: 20.843 min
Delta R.T.: 0.011 min
Response: 117689
Conc: 1.08 ug/ml

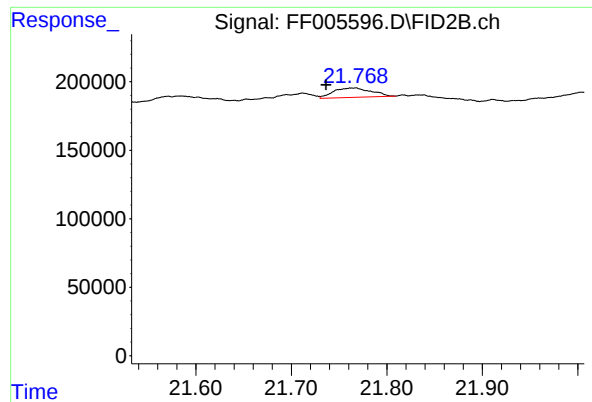

#18 N-TETRACONTANE

R.T.: 21.767 min
Delta R.T.: 0.031 min
Response: 189297
Conc: 1.49 ug/ml

Instrument :
FID_F
ClientSampleId :