

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
 Data File : FF005602.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2019 19:56
 Operator : DD\AJ
 Sample : K4924-02
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-48-COMP

Integration File: autoint1.e
 Quant Time: Sep 18 00:55:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.625	1510241	14.113 ug/ml
Target Compounds			
4) N-TETRADECANE	8.226f	336532	2.387 ug/ml
8) N-DOCOSANE	13.721	83696	0.665 ug/ml
10) N-TETRACOSANE	14.828	142238	1.163 ug/ml
11) N-HEXACOSANE	15.855	114769	0.959 ug/ml
12) N-OCTACOSANE	16.810	290235	2.432 ug/ml
13) N-TRIACONTANE	17.704	373927	3.091 ug/ml
14) N-DOTRIACONTANE	18.539	345769	2.789 ug/ml
15) N-TETRATRIACONTANE	19.400f	92718	0.769 ug/ml
16) N-HEXATRIACONTANE	20.084	74555	0.621 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
Data File : FF005602.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2019 19:56
Operator : DD\AJ
Sample : K4924-02
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-48-COMP

Integration File: autoint1.e
Quant Time: Sep 18 00:55:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

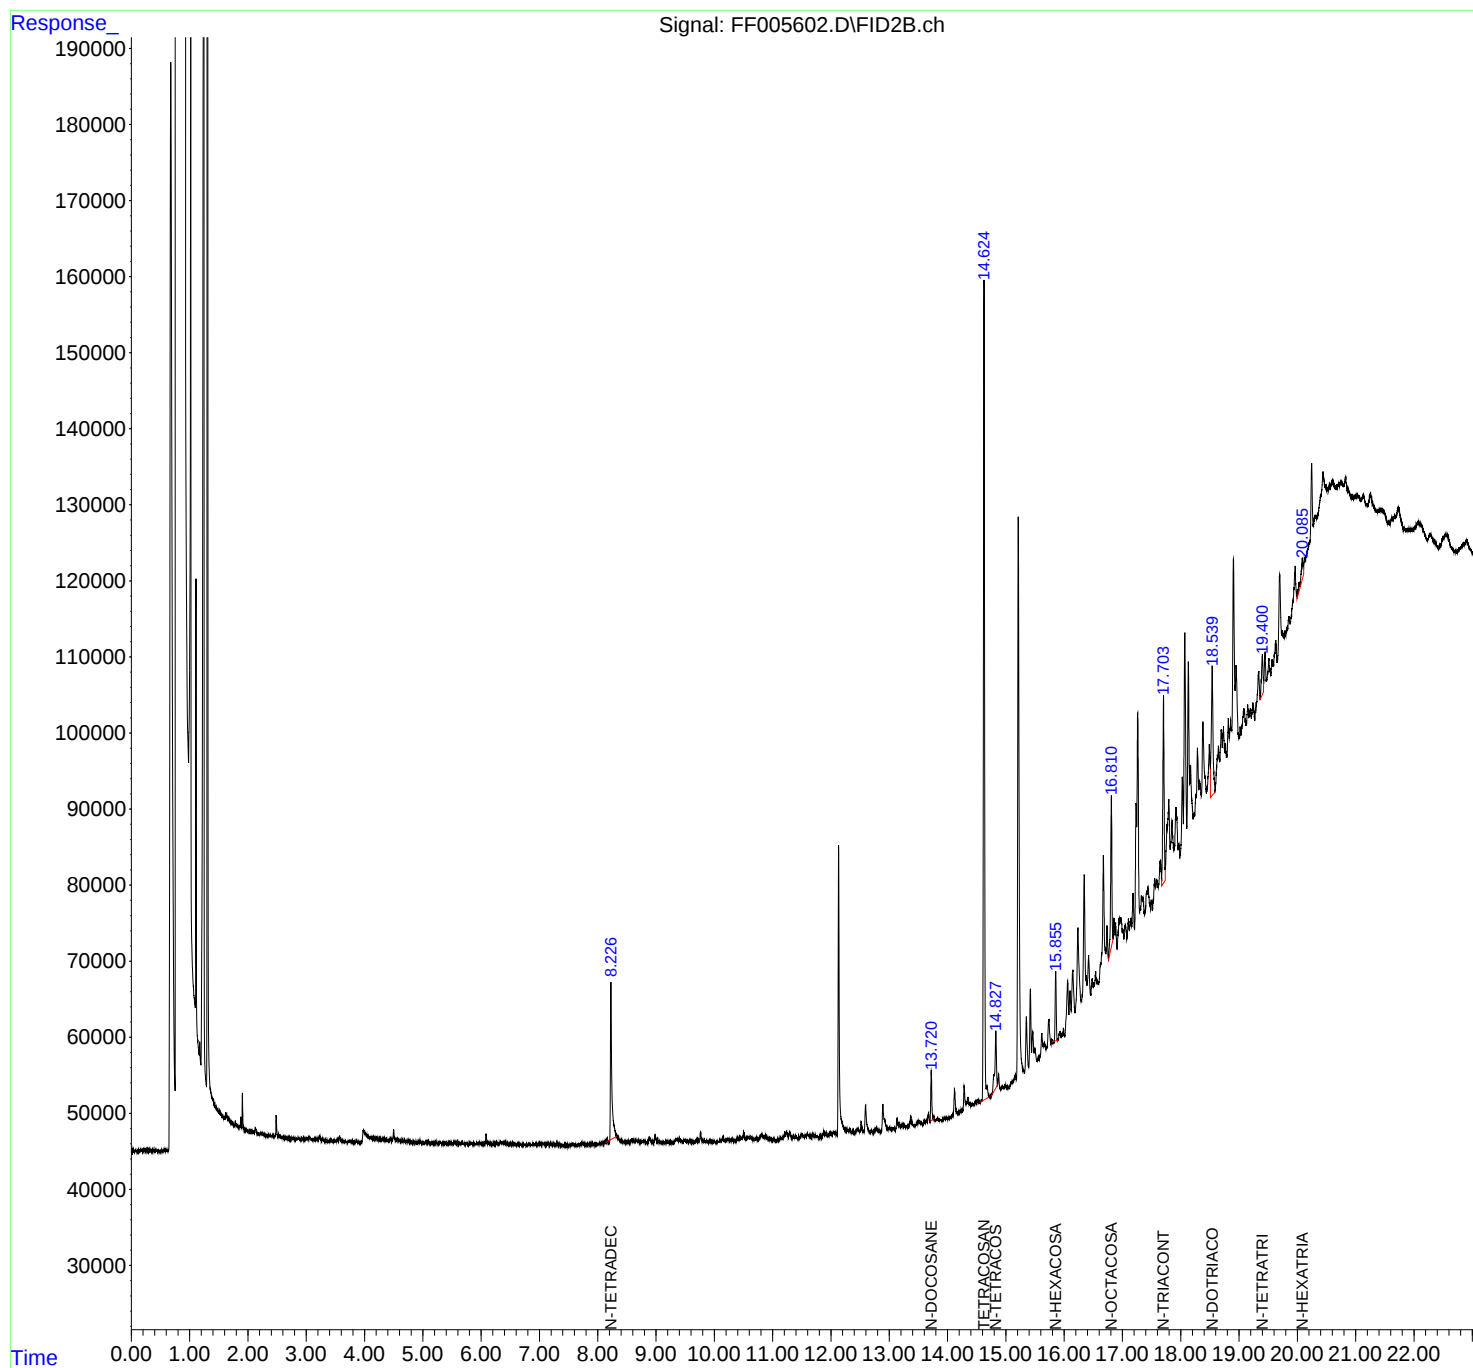


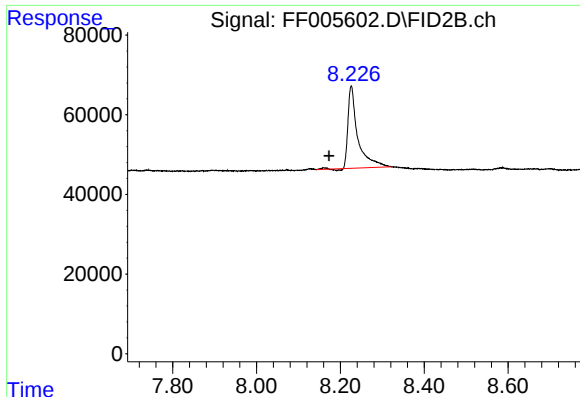

#4 N-TETRADECANE


R.T.: 8.226 min
Delta R.T.: 0.053 min
Response: 336532
Conc: 2.39 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-48-COMP

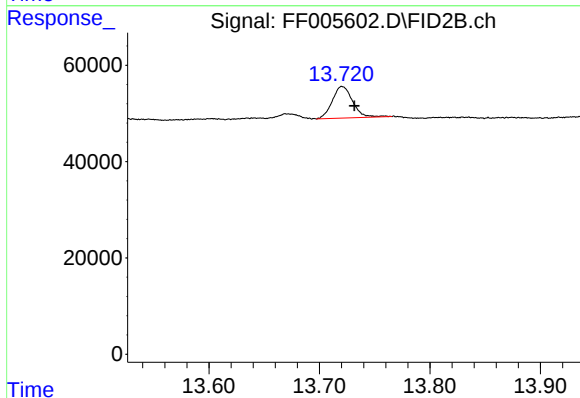


#8 N-DOCOSANE

R.T.: 13.721 min
Delta R.T.: -0.011 min
Response: 83696
Conc: 0.66 ug/ml

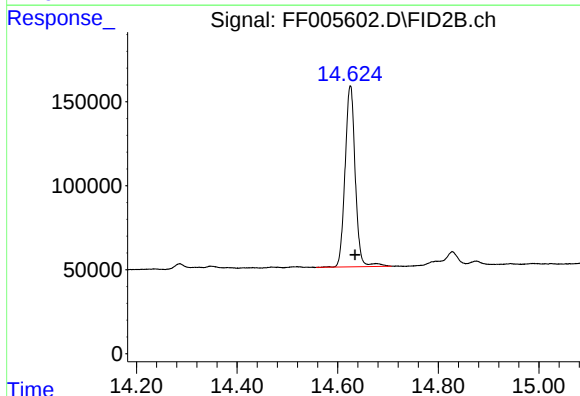


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.625 min
Delta R.T.: -0.009 min
Response: 1510241
Conc: 14.11 ug/ml

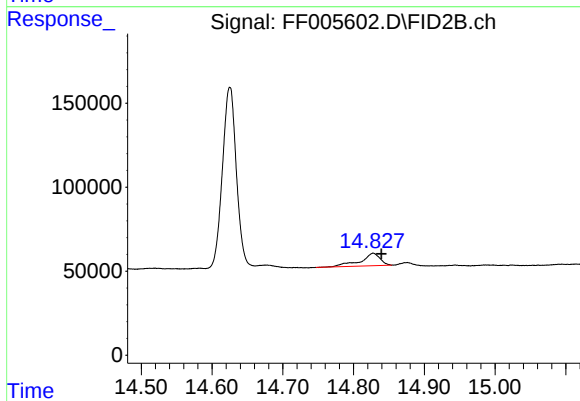

#10 N-TETRACOSANE


R.T.: 14.828 min
Delta R.T.: -0.012 min
Response: 142238
Conc: 1.16 ug/ml

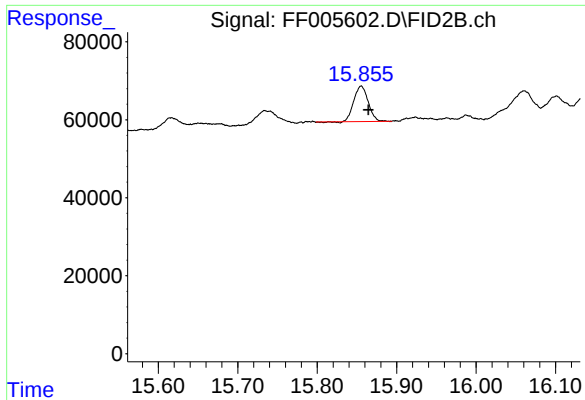

#11 N-HEXACOSANE


R.T.: 15.855 min
Delta R.T.: -0.009 min
Response: 114769
Conc: 0.96 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-48-COMP

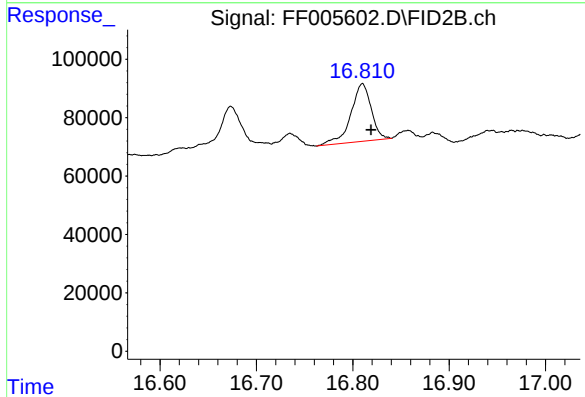


#12 N-OCTACOSANE

R.T.: 16.810 min
Delta R.T.: -0.009 min
Response: 290235
Conc: 2.43 ug/ml

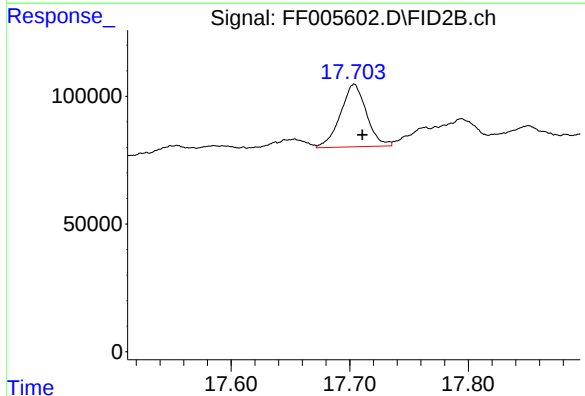


#13 N-TRIACONTANE

R.T.: 17.704 min
Delta R.T.: -0.007 min
Response: 373927
Conc: 3.09 ug/ml

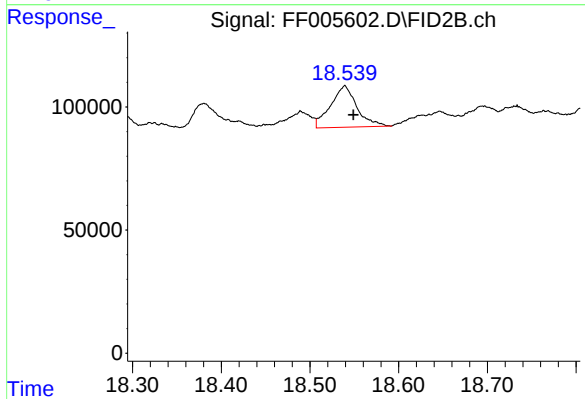

#14 N-DOTRIACONTANE


R.T.: 18.539 min
Delta R.T.: -0.010 min
Response: 345769
Conc: 2.79 ug/ml

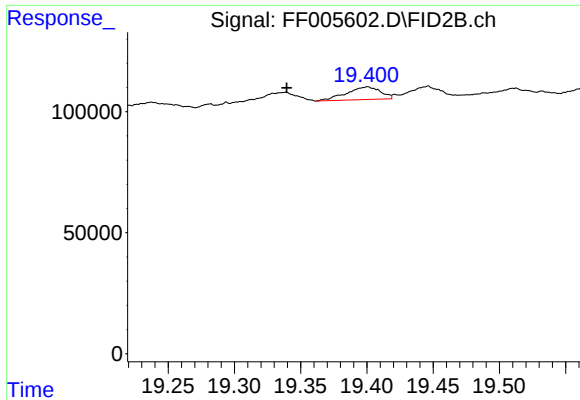

#15 N-TETRATRIACONTANE

R.T.: 19.400 min
Delta R.T.: 0.061 min
Response: 92718
Conc: 0.77 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-48-COMP

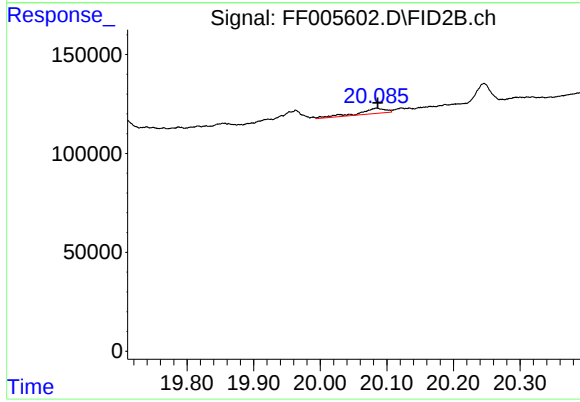

#16 N-HEXATRIACONTANE

R.T.: 20.084 min
Delta R.T.: -0.002 min
Response: 74555
Conc: 0.62 ug/ml