

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
 Data File : FF005607.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2019 22:53
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Sep 18 00:57:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.625	1996231	18.655 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.541	29890	0.241 ug/ml
15) N-TETRATRIACONTANE	19.332	103458	0.859 ug/ml
16) N-HEXATRIACONTANE	20.079	225456	1.878 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
Data File : FF005607.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2019 22:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 18 00:57:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

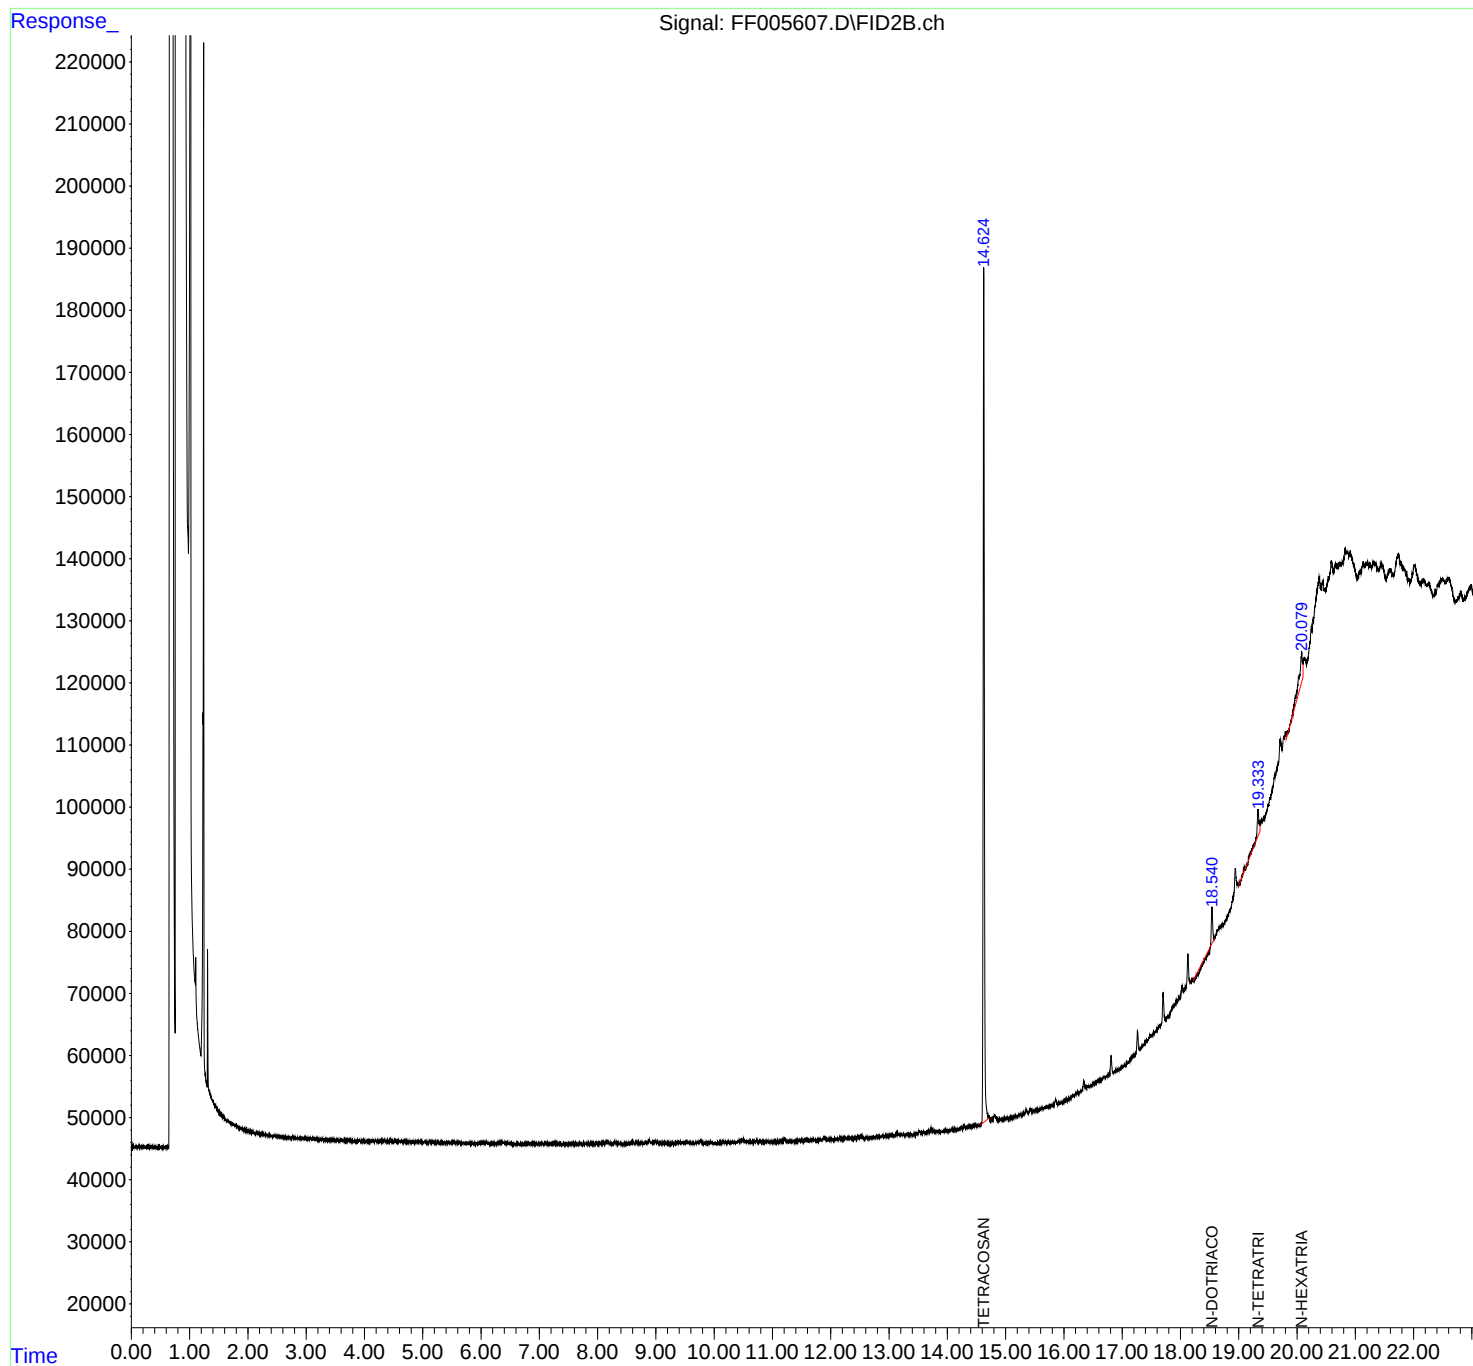


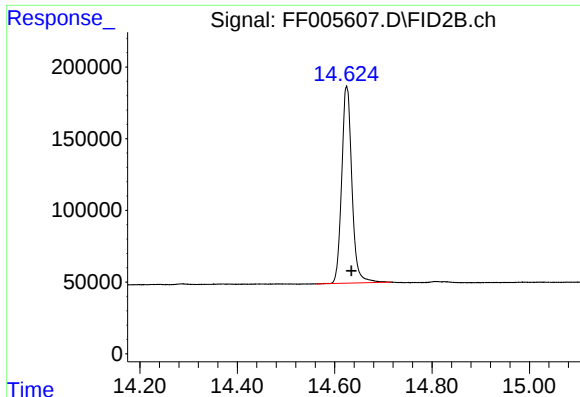

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.625 min
Delta R.T.: -0.010 min
Response: 1996231
Conc: 18.65 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

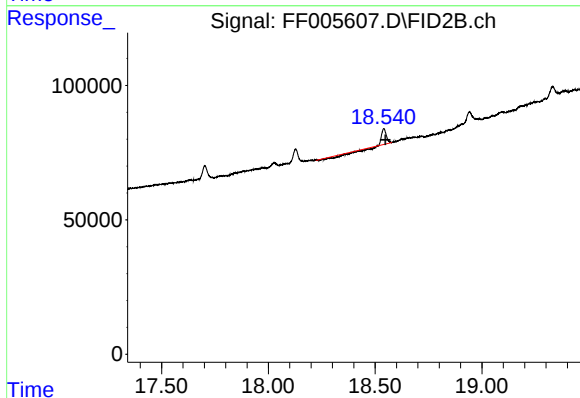


#14 N-DOTRIACONTANE

R.T.: 18.541 min
Delta R.T.: -0.008 min
Response: 29890
Conc: 0.24 ug/ml

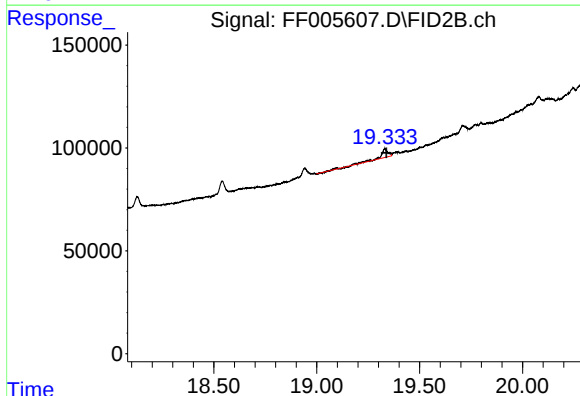

#15 N-TETRATRIACONTANE

R.T.: 19.332 min
Delta R.T.: -0.007 min
Response: 103458
Conc: 0.86 ug/ml

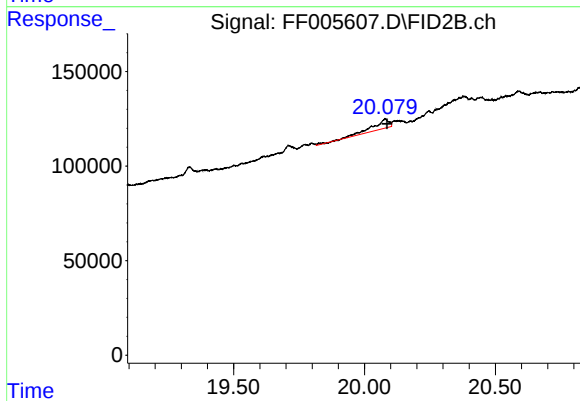

#16 N-HEXATRIACONTANE

R.T.: 20.079 min
Delta R.T.: -0.008 min
Response: 225456
Conc: 1.88 ug/ml