

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
 Data File : FF005599.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2019 18:27
 Operator : DD\AJ
 Sample : PB123163BS
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB123163BS

Integration File: autoint1.e
 Quant Time: Sep 18 00:54:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	2177434	20.348 ug/ml
Target Compounds			
2) N-DECANE	4.350	2815953	19.696 ug/ml
3) N-DODECANE	6.370	2780013	19.393 ug/ml
4) N-TETRADECANE	8.163	2653832	18.822 ug/ml
5) N-HEXADECANE	9.765	2739693	19.588 ug/ml
6) N-OCTADECANE	11.208	2712781	20.163 ug/ml
7) N-EICOSANE	12.521	2673494	20.386 ug/ml
8) N-DOCOSANE	13.724	2637965	20.952 ug/ml
10) N-TETRACOSANE	14.832	2696172	22.046 ug/ml
11) N-HEXACOSANE	15.858	2729844	22.805 ug/ml
12) N-OCTACOSANE	16.813	2810364	23.552 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091719\
Data File : FF005599.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2019 18:27
Operator : DD\AJ
Sample : PB123163BS
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
PB123163BS

Integration File: autoint1.e
Quant Time: Sep 18 00:54:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

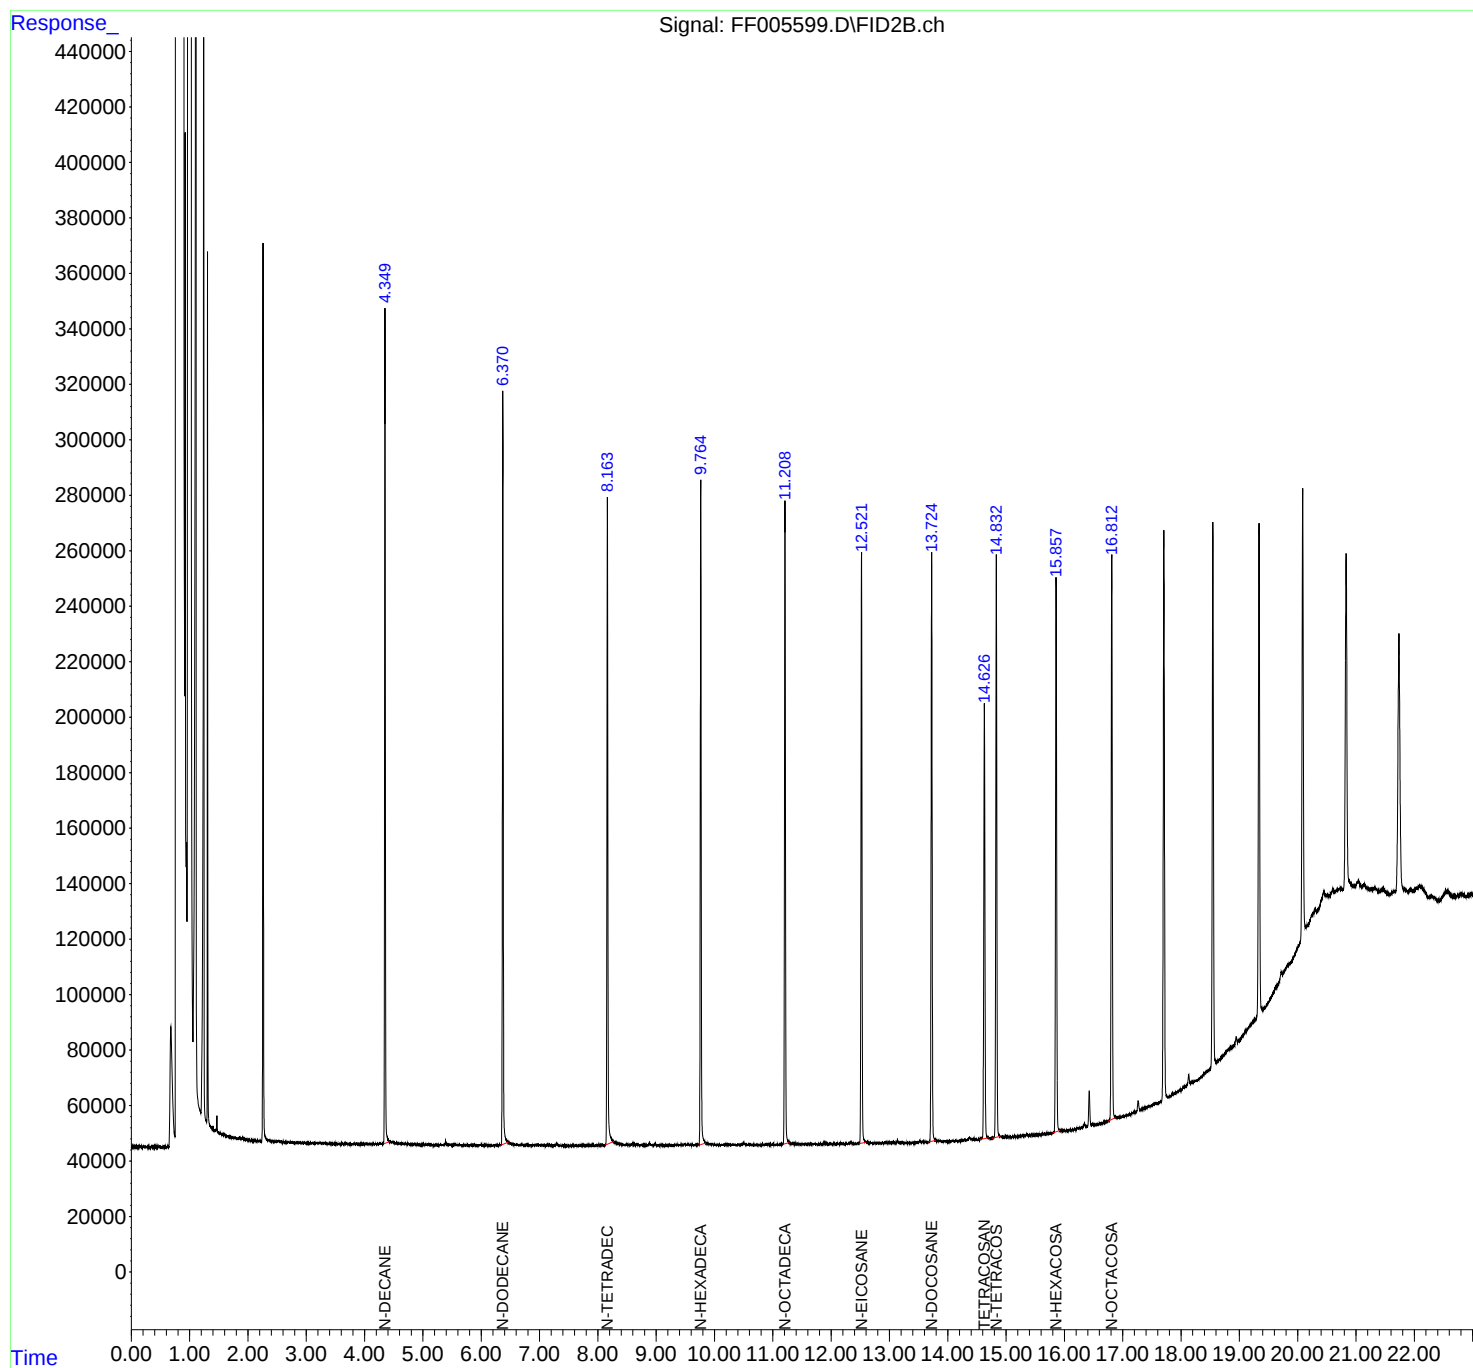


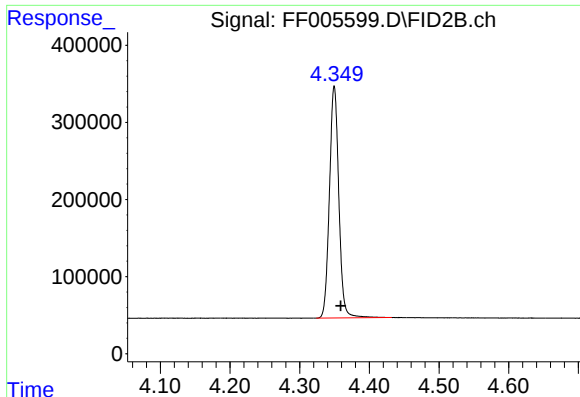

#2 N-DECANE


R.T.: 4.350 min
Delta R.T.: -0.009 min
Response: 2815953
Conc: 19.70 ug/ml

Instrument :
FID_F
ClientSampleId :
PB123163BS

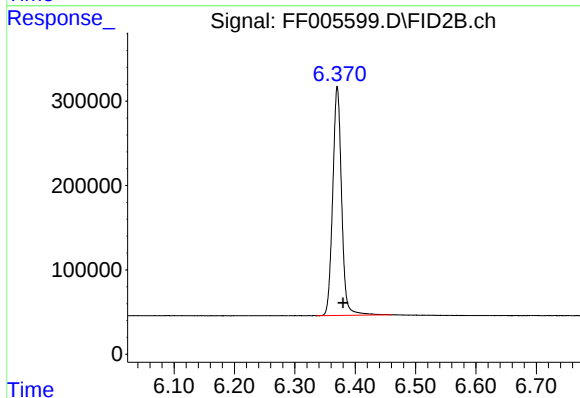


#3 N-DODECANE

R.T.: 6.370 min
Delta R.T.: -0.009 min
Response: 2780013
Conc: 19.39 ug/ml

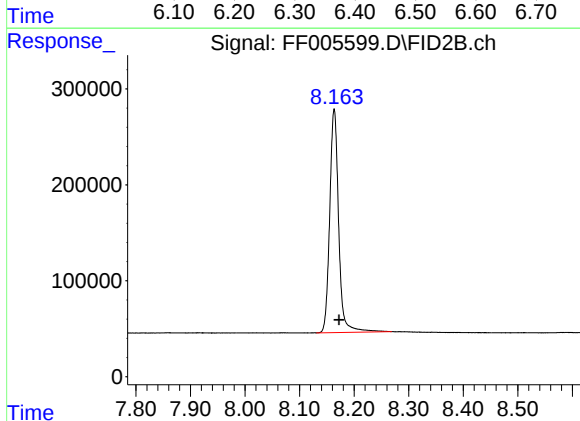


#4 N-TETRADECANE

R.T.: 8.163 min
Delta R.T.: -0.009 min
Response: 2653832
Conc: 18.82 ug/ml

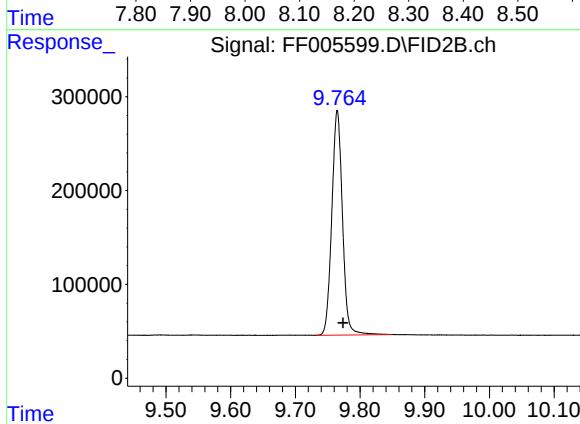

#5 N-HEXADECANE


R.T.: 9.765 min
Delta R.T.: -0.009 min
Response: 2739693
Conc: 19.59 ug/ml

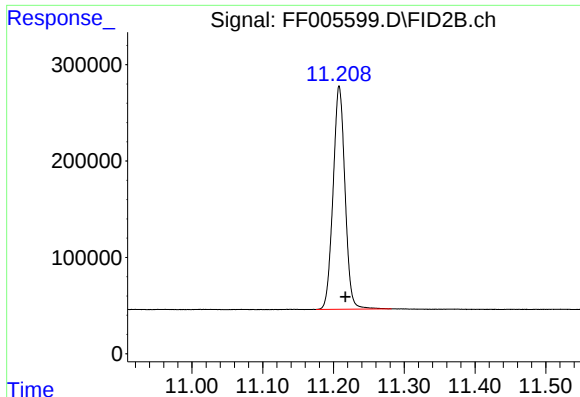

#6 N-OCTADECANE


R.T.: 11.208 min
Delta R.T.: -0.009 min
Response: 2712781
Conc: 20.16 ug/ml

Instrument :
FID_F
ClientSampleId :
PB123163BS

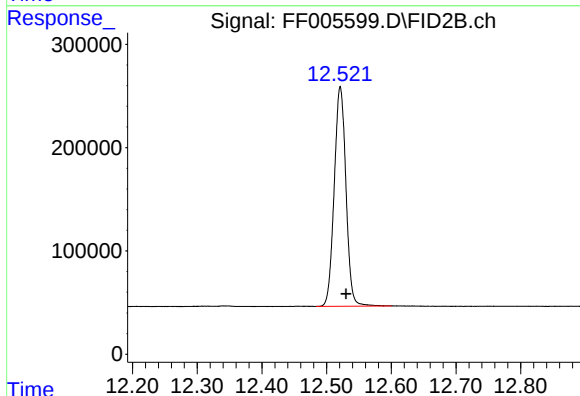


#7 N-EICOSANE

R.T.: 12.521 min
Delta R.T.: -0.009 min
Response: 2673494
Conc: 20.39 ug/ml

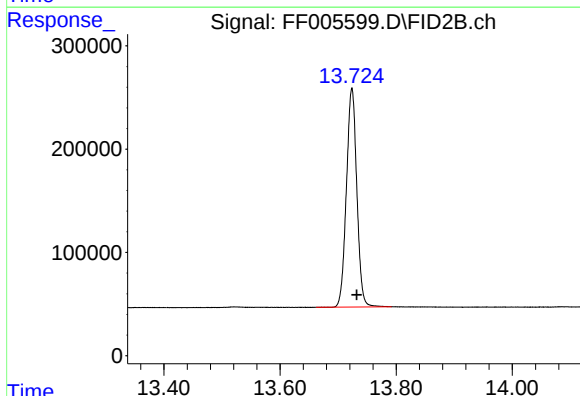


#8 N-DOCOSANE

R.T.: 13.724 min
Delta R.T.: -0.008 min
Response: 2637965
Conc: 20.95 ug/ml

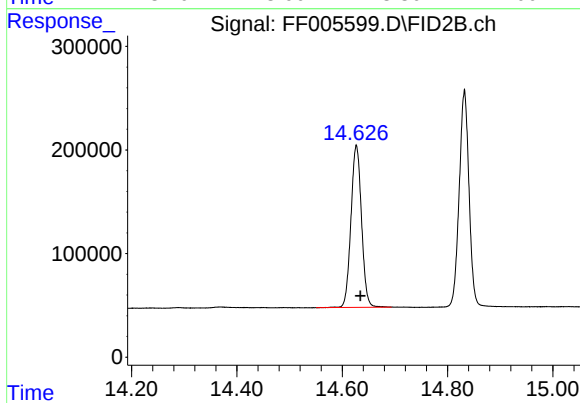

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.627 min
Delta R.T.: -0.008 min
Response: 2177434
Conc: 20.35 ug/ml

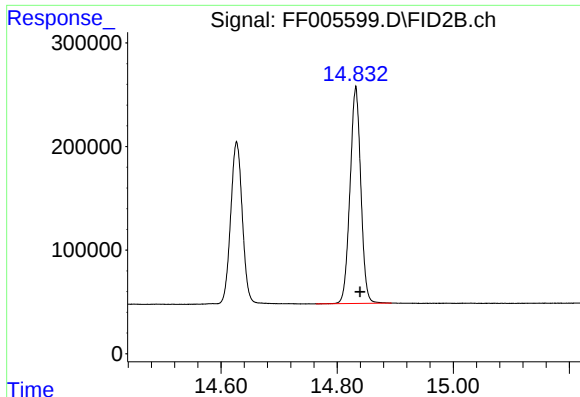

#10 N-TETRACOSANE


R.T.: 14.832 min
Delta R.T.: -0.007 min
Response: 2696172
Conc: 22.05 ug/ml

Instrument :
FID_F
ClientSampleId :
PB123163BS

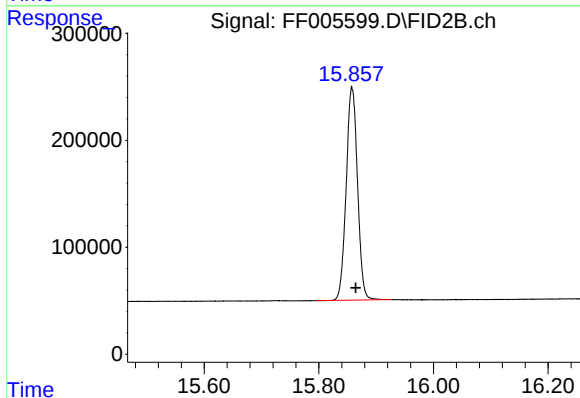

#11 N-HEXACOSANE

R.T.: 15.858 min
Delta R.T.: -0.006 min
Response: 2729844
Conc: 22.80 ug/ml

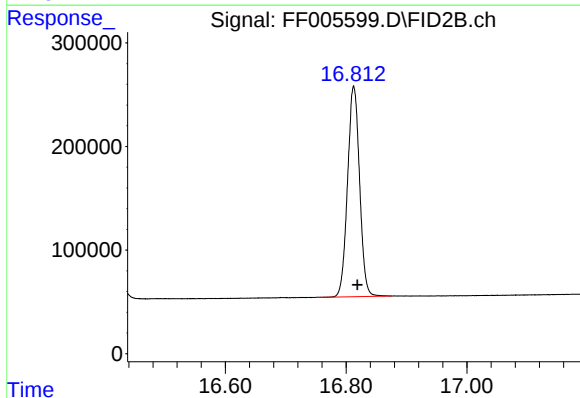

#12 N-OCTACOSANE

R.T.: 16.813 min
Delta R.T.: -0.006 min
Response: 2810364
Conc: 23.55 ug/ml