

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091720\
 Data File : FF007596.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2020 17:47
 Operator : DD\AJ
 Sample : L4062-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 18 01:59:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	1806240	12.281 ug/ml
Target Compounds			
4) N-TETRADECANE	8.336f	401048	2.437 ug/ml
7) N-EICOSANE	12.584f	82033	0.488 ug/ml
10) N-TETRACOSANE	14.927	415496	2.548 ug/ml
11) N-HEXACOSANE	15.966	97252	0.615 ug/ml
12) N-OCTACOSANE	16.931	646876	4.215 ug/ml
13) N-TRIACONTANE	17.809	556294	3.764 ug/ml
14) N-DOTRIACONTANE	18.638	504342	3.635 ug/ml
15) N-TETRATRIACONTANE	19.430	218614	1.732 ug/ml
16) N-HEXATRIACONTANE	20.168	345518	2.891 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091720\
Data File : FF007596.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2020 17:47
Operator : DD\AJ
Sample : L4062-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 18 01:59:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

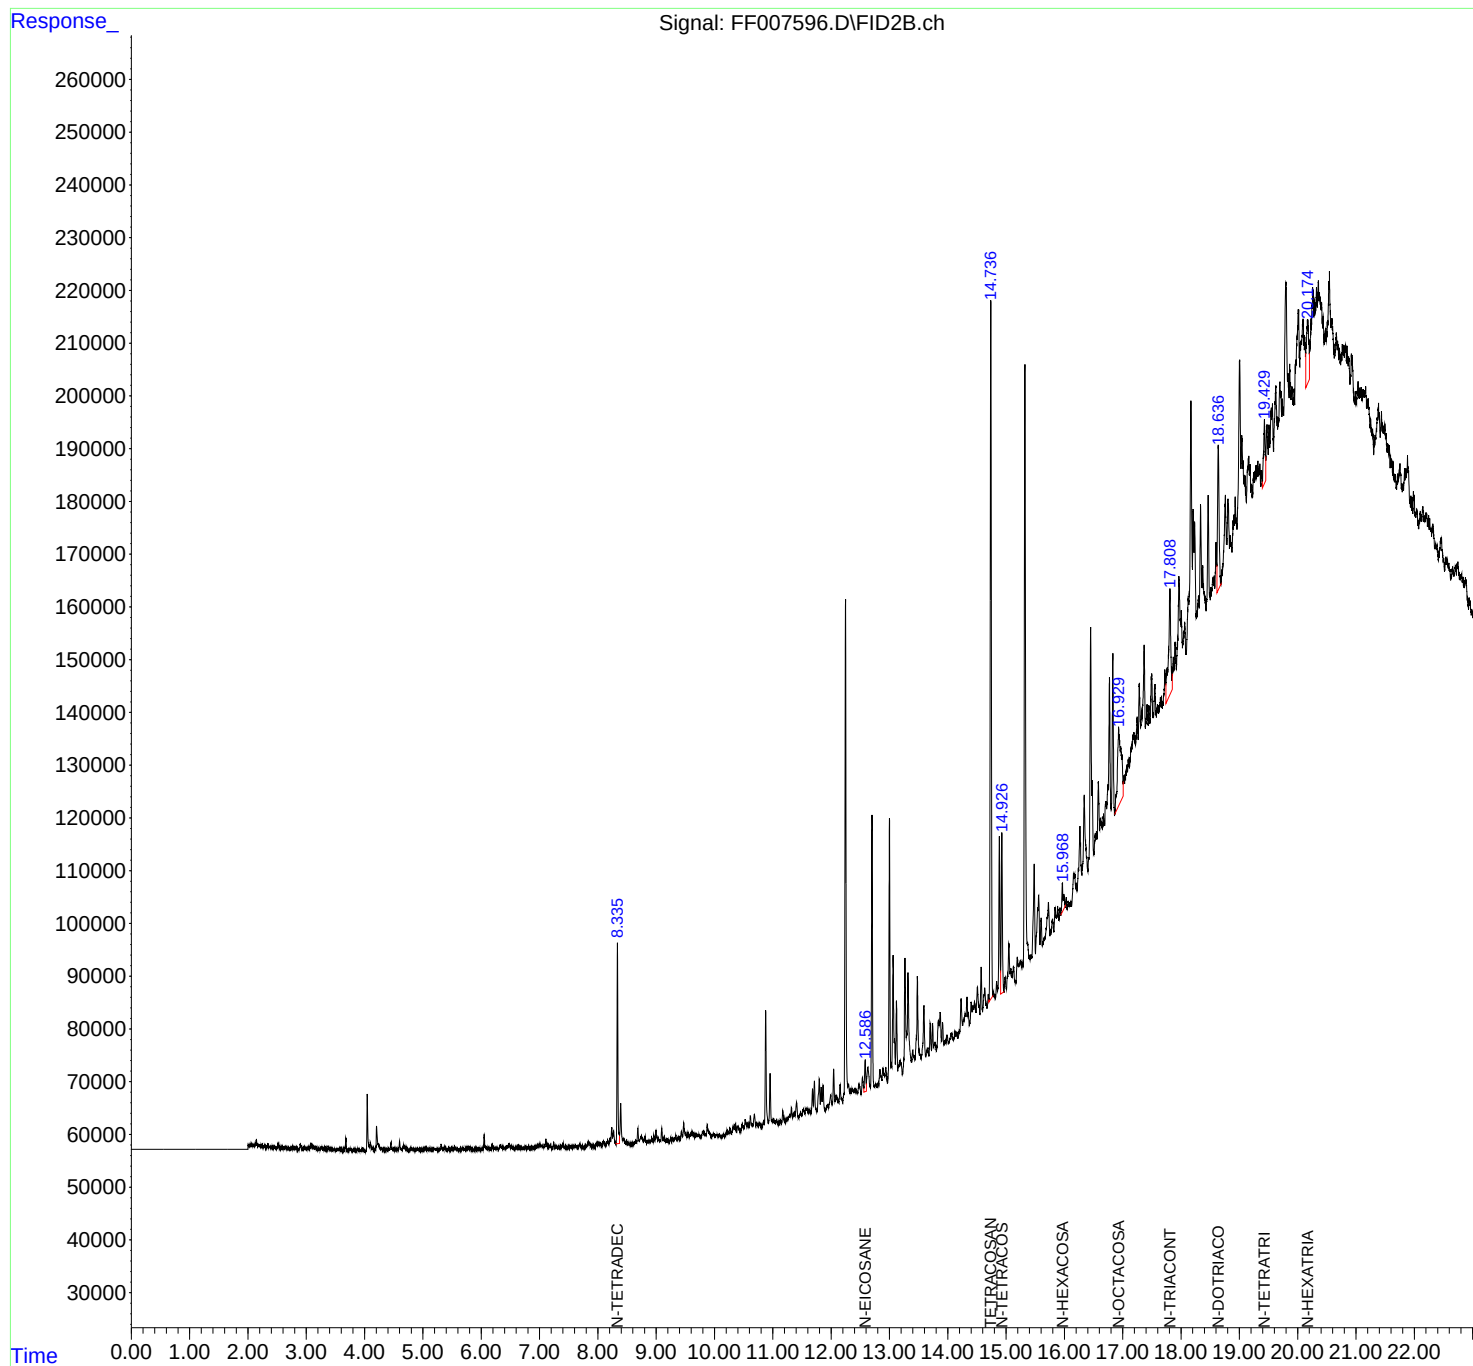


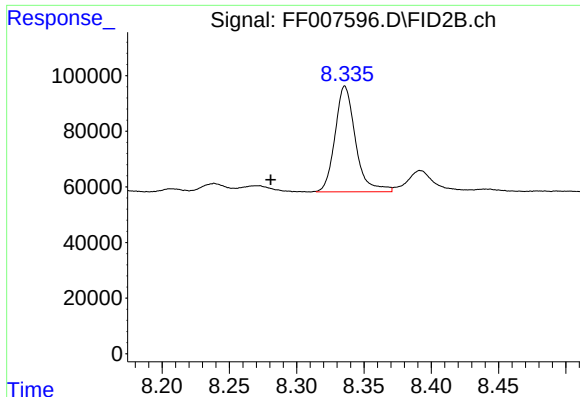

#4 N-TETRADECANE


R.T.: 8.336 min
Delta R.T.: 0.055 min
Response: 401048
Conc: 2.44 ug/ml

Instrument :
FID_F
ClientSampleId :

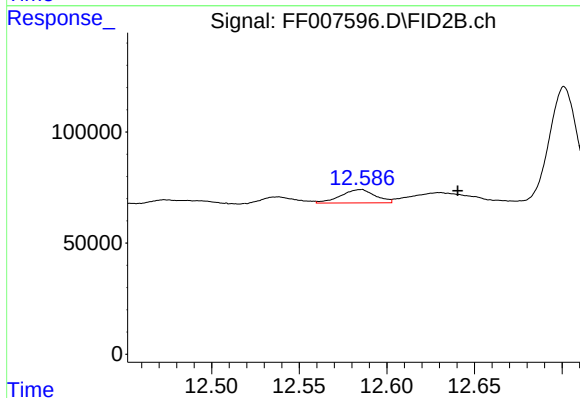


#7 N-EICOSANE

R.T.: 12.584 min
Delta R.T.: -0.056 min
Response: 82033
Conc: 0.49 ug/ml

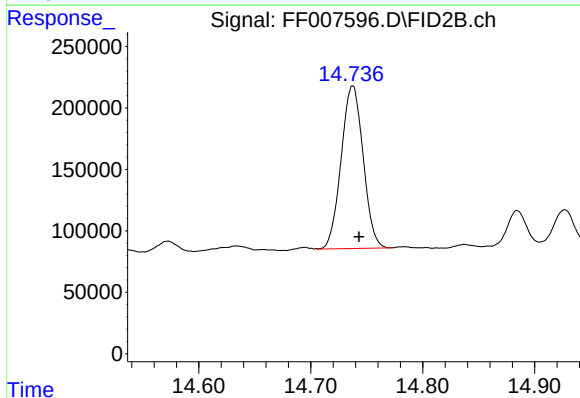


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.737 min
Delta R.T.: -0.006 min
Response: 1806240
Conc: 12.28 ug/ml

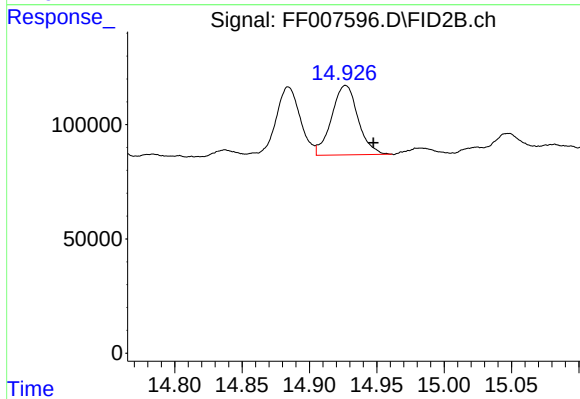

#10 N-TETRACOSANE


R.T.: 14.927 min
Delta R.T.: -0.021 min
Response: 415496
Conc: 2.55 ug/ml

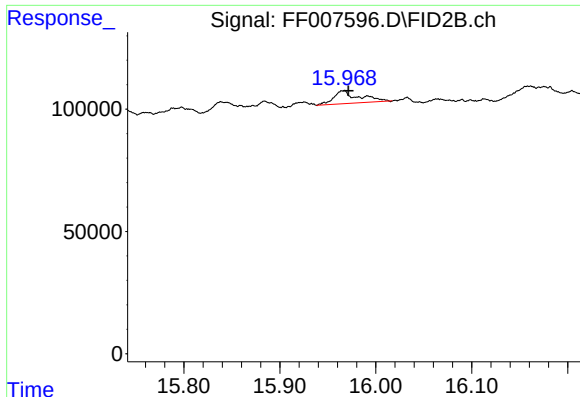

#11 N-HEXACOSANE


R.T.: 15.966 min
Delta R.T.: -0.006 min
Response: 97252
Conc: 0.62 ug/ml

Instrument :
FID_F
ClientSampleId :

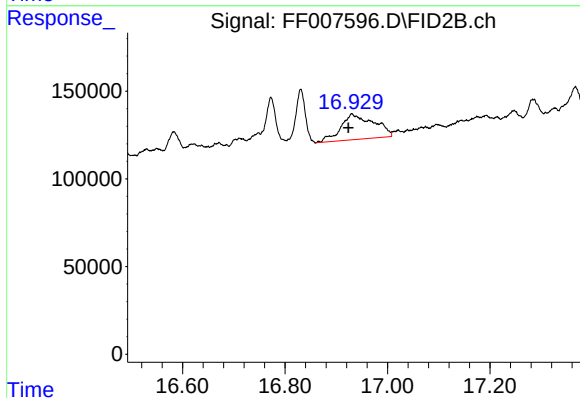


#12 N-OCTACOSANE

R.T.: 16.931 min
Delta R.T.: 0.007 min
Response: 646876
Conc: 4.22 ug/ml

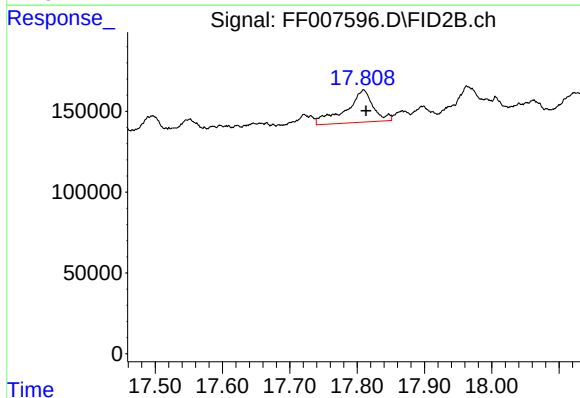


#13 N-TRIACONTANE

R.T.: 17.809 min
Delta R.T.: -0.004 min
Response: 556294
Conc: 3.76 ug/ml

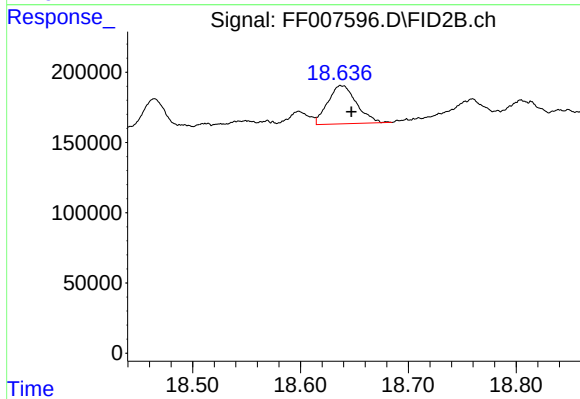

#14 N-DOTRIACONTANE


R.T.: 18.638 min
Delta R.T.: -0.009 min
Response: 504342
Conc: 3.63 ug/ml

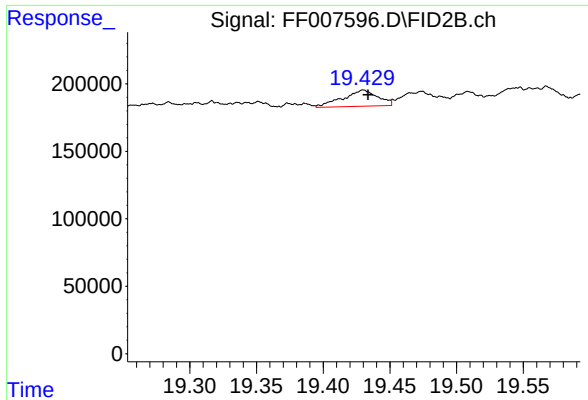

#15 N-TETRATRIACONTANE

R.T.: 19.430 min
Delta R.T.: -0.003 min
Response: 218614
Conc: 1.73 ug/ml

Instrument :
FID_F
ClientSampleId :

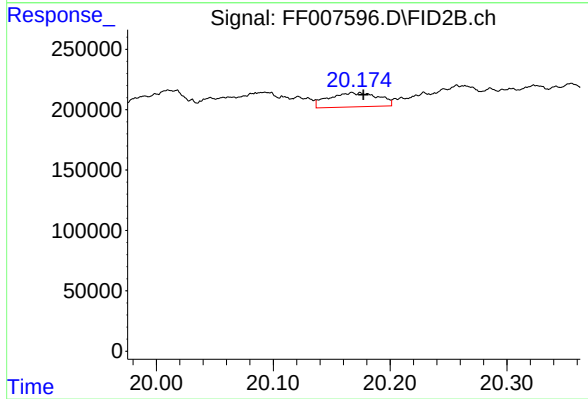

#16 N-HEXATRIACONTANE

R.T.: 20.168 min
Delta R.T.: -0.009 min
Response: 345518
Conc: 2.89 ug/ml