

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091720\
 Data File : FF007597.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2020 18:18
 Operator : DD\AJ
 Sample : L4062-02
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 18 01:59:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	2257387	15.349 ug/ml
Target Compounds			
4) N-TETRADECANE	8.336f	503211	3.058 ug/ml
7) N-EICOSANE	12.586f	89154	0.530 ug/ml
8) N-DOCOSANE	13.870	121214	0.736 ug/ml
10) N-TETRACOSANE	14.927	810713	4.971 ug/ml
11) N-HEXACOSANE	15.964	120454	0.762 ug/ml
12) N-OCTACOSANE	16.932	378375	2.466 ug/ml
13) N-TRIACONTANE	17.810	459275	3.107 ug/ml
14) N-DOTRIACONTANE	18.637	452239	3.259 ug/ml
15) N-TETRATRIACONTANE	19.429	209418	1.659 ug/ml
16) N-HEXATRIACONTANE	20.181	272669	2.282 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091720\
Data File : FF007597.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2020 18:18
Operator : DD\AJ
Sample : L4062-02
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 18 01:59:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

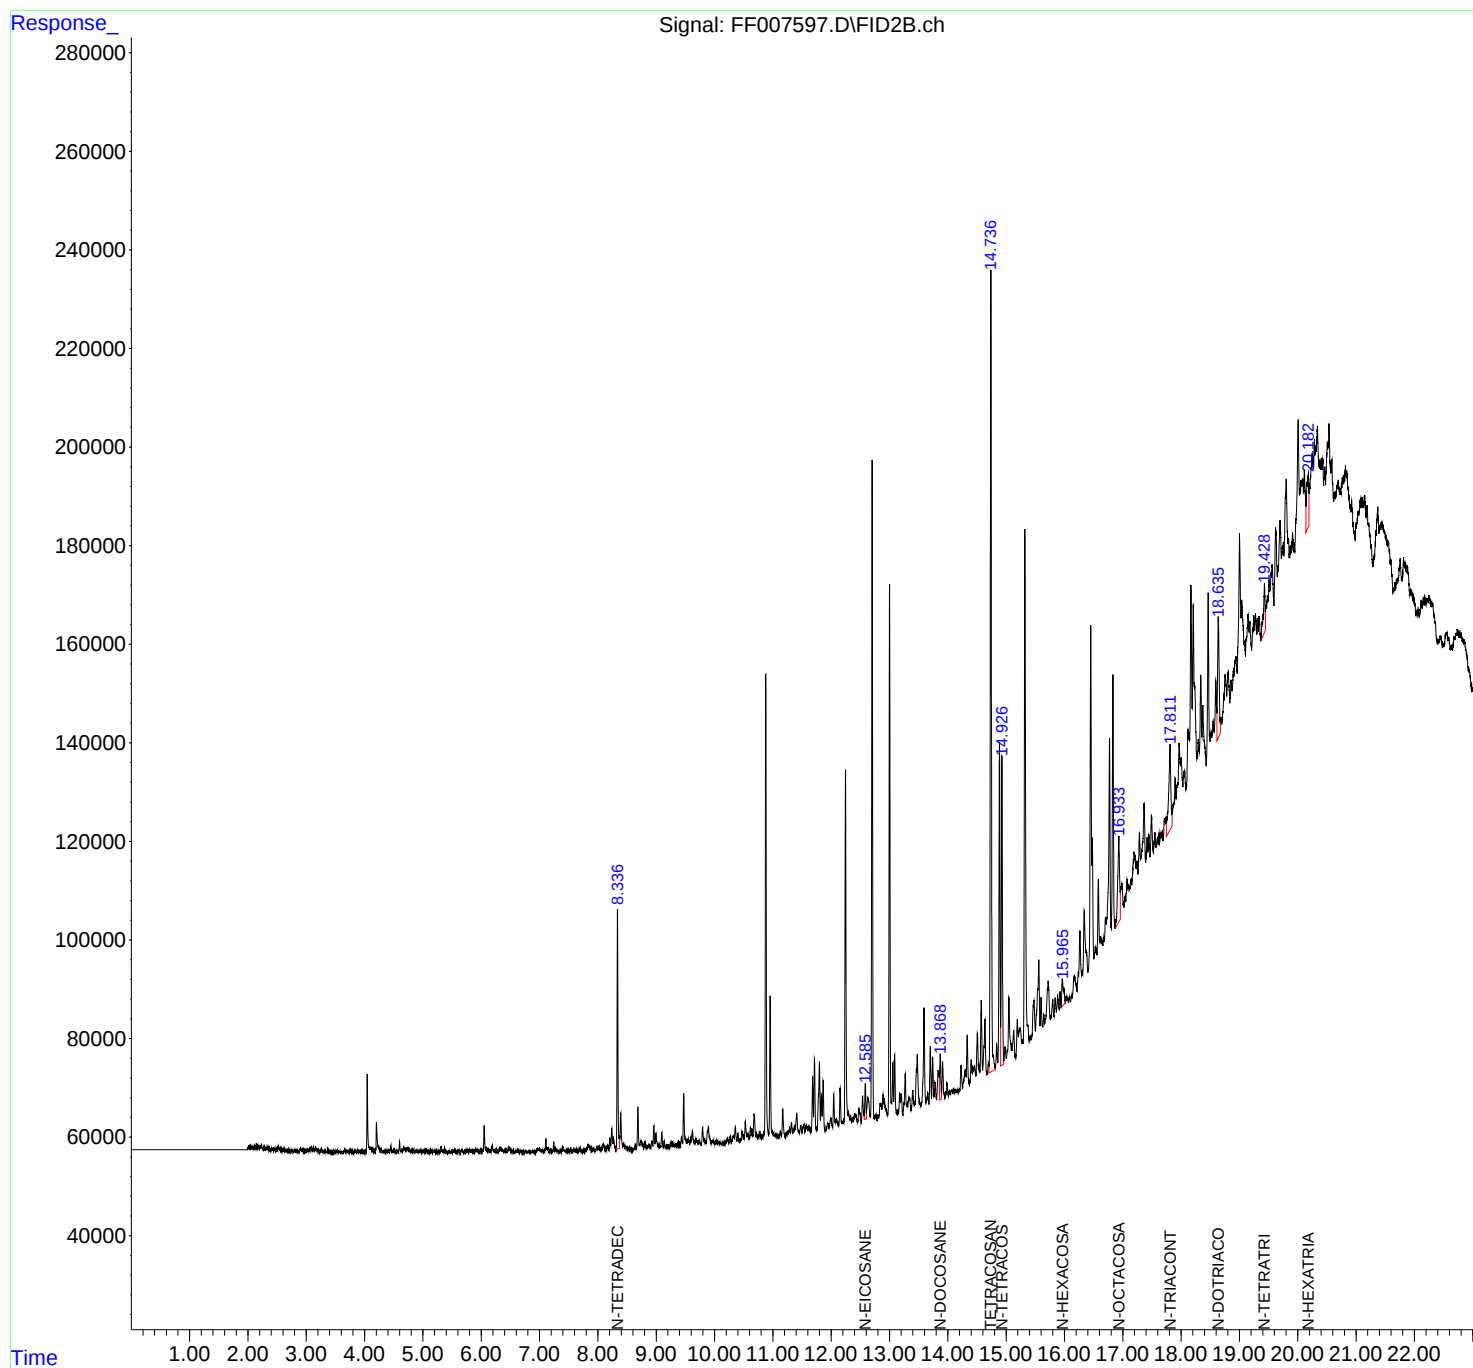


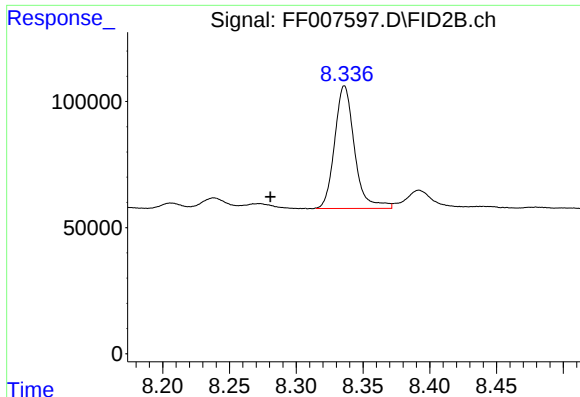

#4 N-TETRADECANE


R.T.: 8.336 min
Delta R.T.: 0.055 min
Response: 503211
Conc: 3.06 ug/ml

Instrument :
FID_F
ClientSampleId :

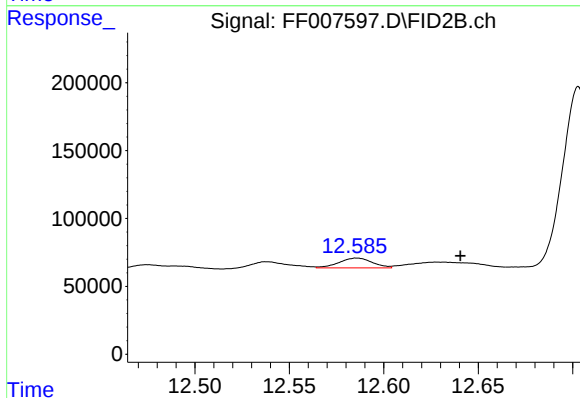


#7 N-EICOSANE

R.T.: 12.586 min
Delta R.T.: -0.055 min
Response: 89154
Conc: 0.53 ug/ml

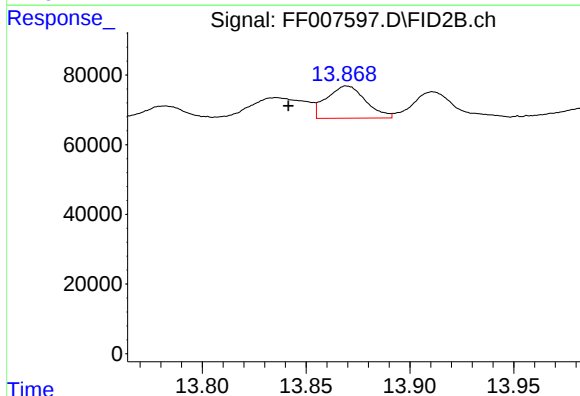


#8 N-DOCOSANE

R.T.: 13.870 min
Delta R.T.: 0.028 min
Response: 121214
Conc: 0.74 ug/ml

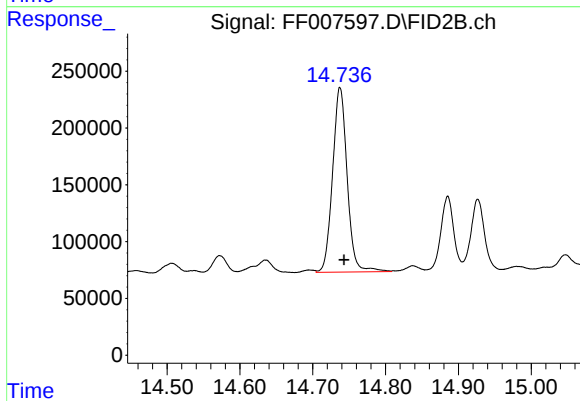

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.738 min
Delta R.T.: -0.006 min
Response: 2257387
Conc: 15.35 ug/ml

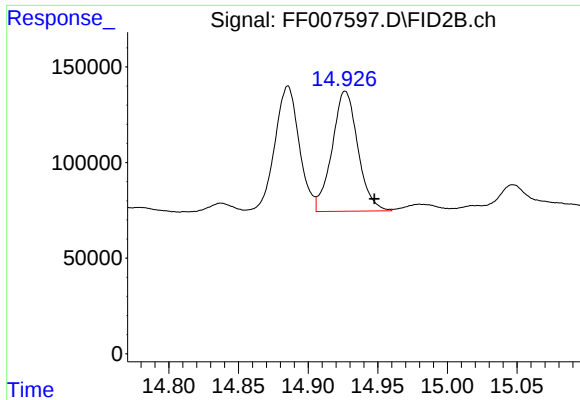

#10 N-TETRACOSANE


R.T.: 14.927 min
Delta R.T.: -0.021 min
Response: 810713
Conc: 4.97 ug/ml

Instrument :
FID_F
ClientSampleId :

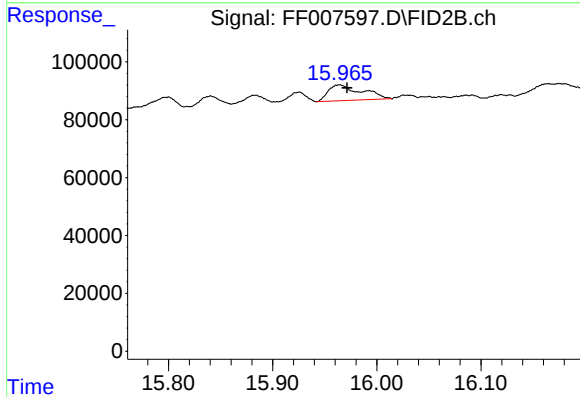


#11 N-HEXACOSANE

R.T.: 15.964 min
Delta R.T.: -0.007 min
Response: 120454
Conc: 0.76 ug/ml

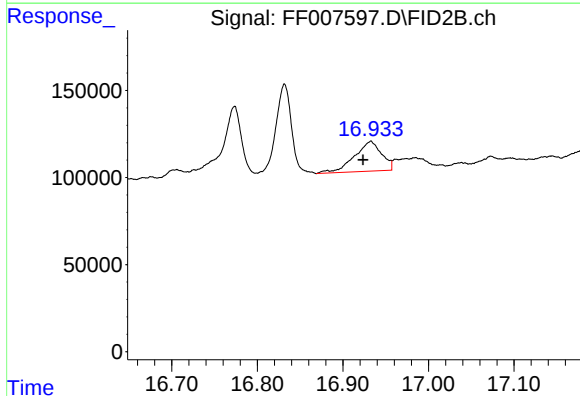


#12 N-OCTACOSANE

R.T.: 16.932 min
Delta R.T.: 0.009 min
Response: 378375
Conc: 2.47 ug/ml

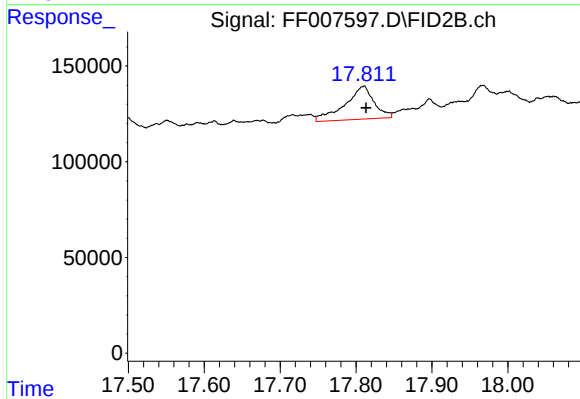

#13 N-TRIACONTANE


R.T.: 17.810 min
Delta R.T.: -0.004 min
Response: 459275
Conc: 3.11 ug/ml

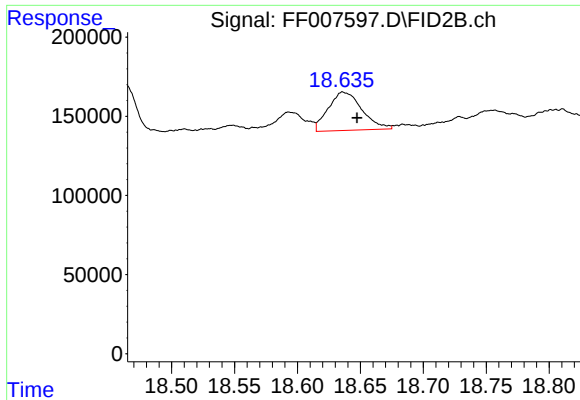

#14 N-DOTRIACONTANE


R.T.: 18.637 min
Delta R.T.: -0.010 min
Response: 452239
Conc: 3.26 ug/ml

Instrument :
FID_F
ClientSampleId :

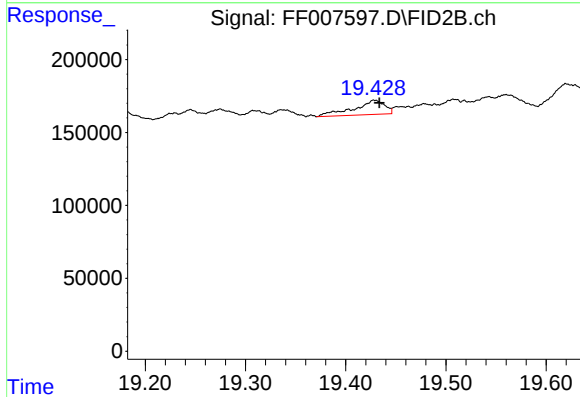

#15 N-TETRATRIACONTANE

R.T.: 19.429 min
Delta R.T.: -0.004 min
Response: 209418
Conc: 1.66 ug/ml

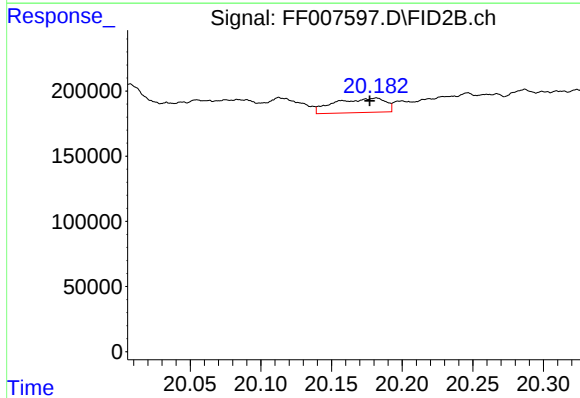

#16 N-HEXATRIACONTANE

R.T.: 20.181 min
Delta R.T.: 0.003 min
Response: 272669
Conc: 2.28 ug/ml