

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091720\
 Data File : FF007598.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2020 18:49
 Operator : DD\AJ
 Sample : L4062-03
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 18 01:59:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	2086374	14.186 ug/ml
Target Compounds			
4) N-TETRADECANE	8.337f	316624	1.924 ug/ml
10) N-TETRACOSANE	14.939	113441	0.696 ug/ml
11) N-HEXACOSANE	15.964	81944	0.518 ug/ml
12) N-OCTACOSANE	16.917	67839	0.442 ug/ml
13) N-TRIACONTANE	17.807	87872	0.595 ug/ml
14) N-DOTRIACONTANE	18.635	201804	1.454 ug/ml
15) N-TETRATRIACONTANE	19.428	124758	0.989 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091720\
Data File : FF007598.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2020 18:49
Operator : DD\AJ
Sample : L4062-03
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 18 01:59:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

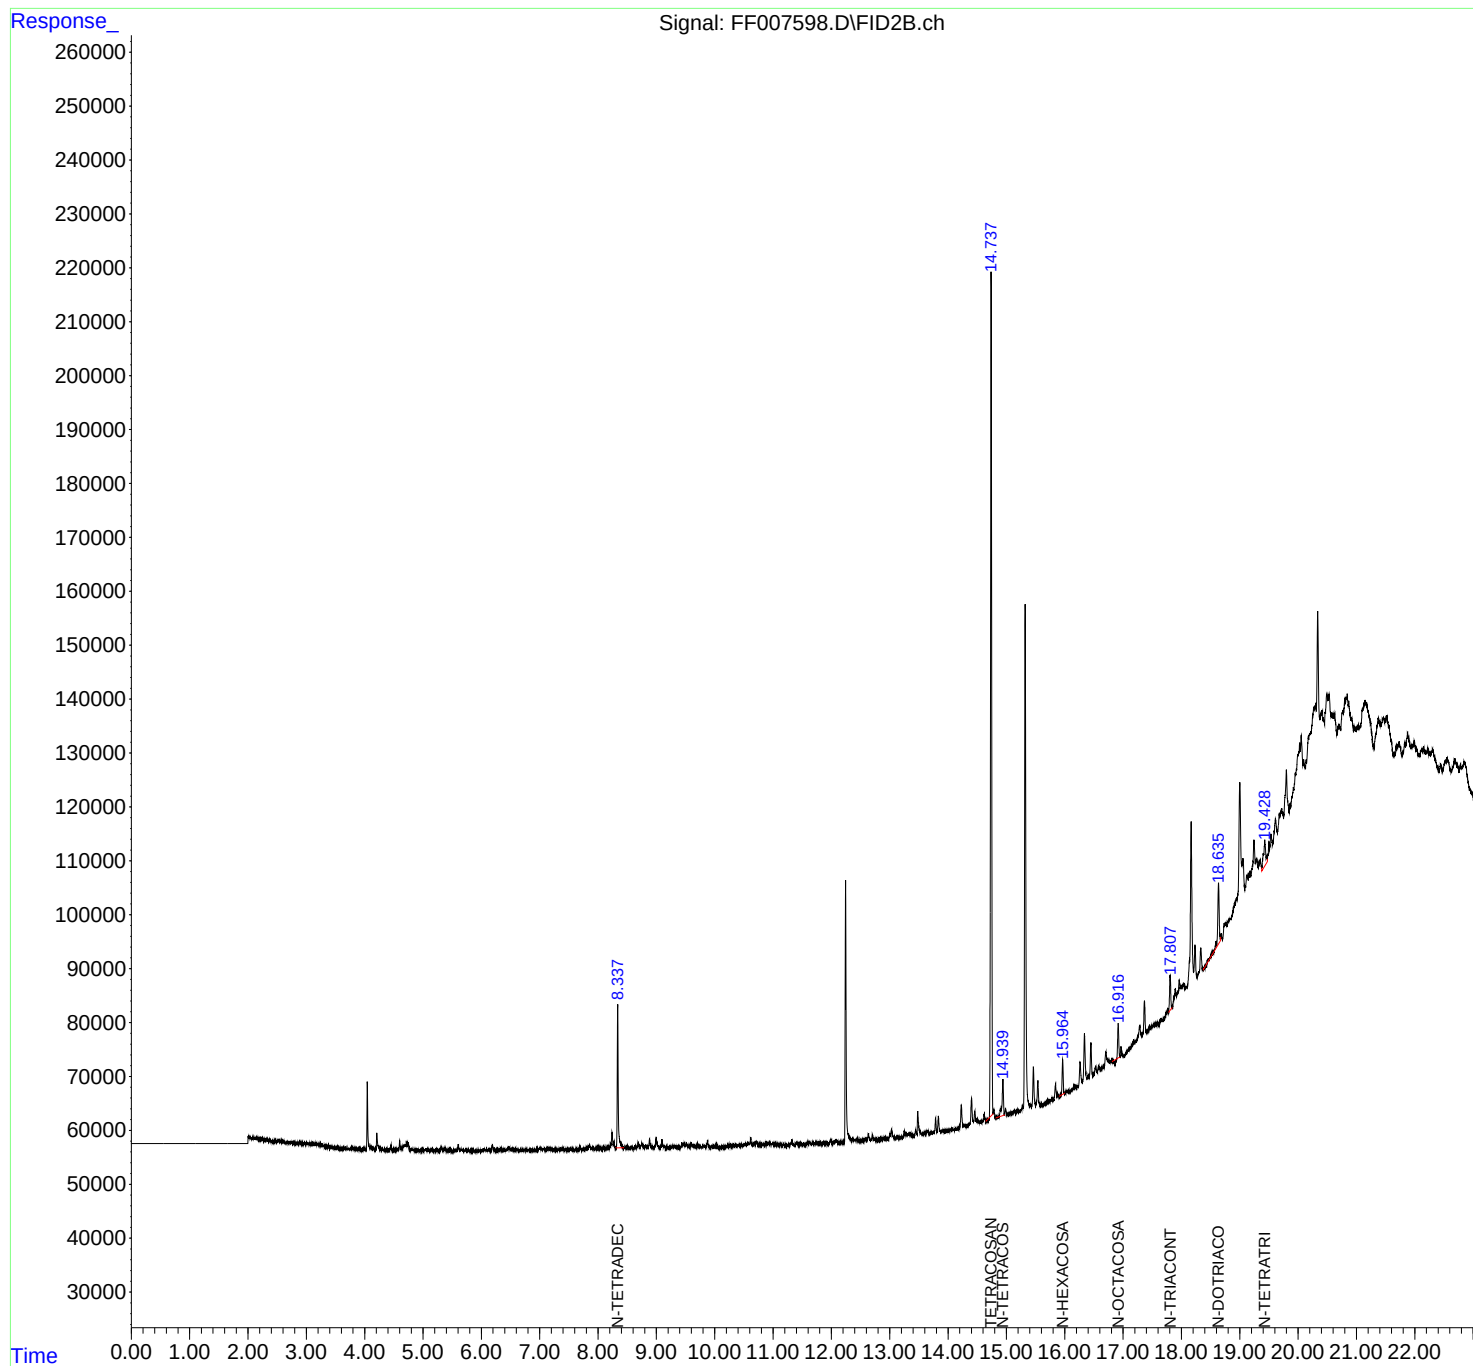


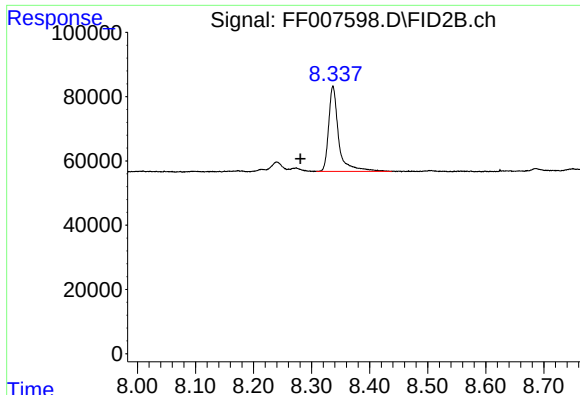

#4 N-TETRADECANE


R.T.: 8.337 min
Delta R.T.: 0.056 min
Response: 316624
Conc: 1.92 ug/ml

Instrument :
FID_F
ClientSampleId :

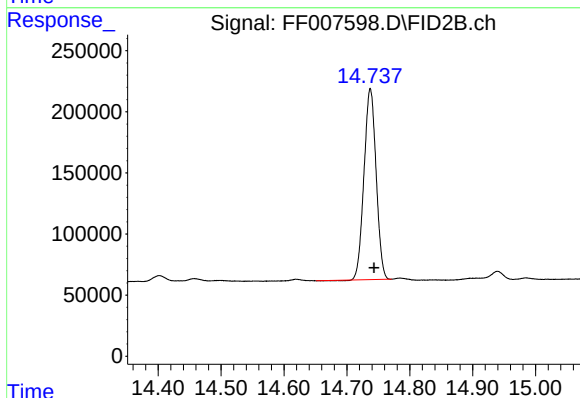


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.737 min
Delta R.T.: -0.006 min
Response: 2086374
Conc: 14.19 ug/ml

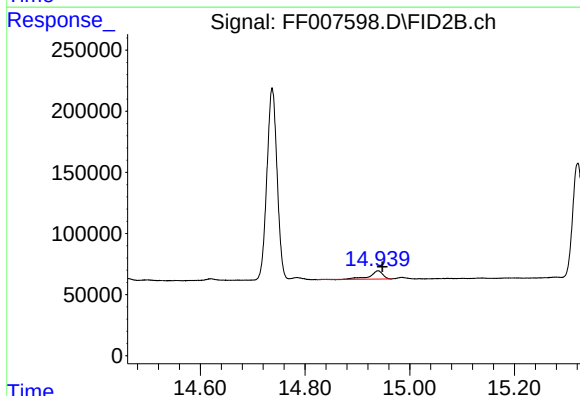


#10 N-TETRACOSANE

R.T.: 14.939 min
Delta R.T.: -0.008 min
Response: 113441
Conc: 0.70 ug/ml

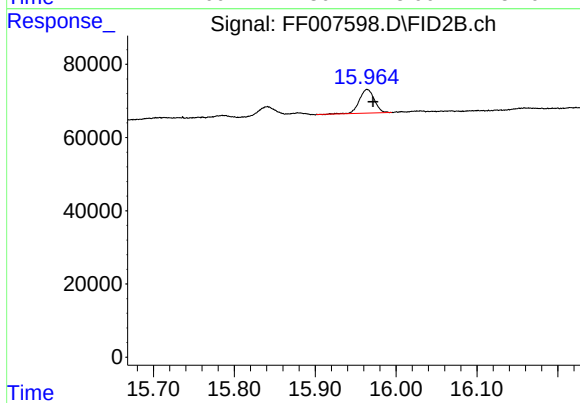

#11 N-HEXACOSANE


R.T.: 15.964 min
Delta R.T.: -0.007 min
Response: 81944
Conc: 0.52 ug/ml

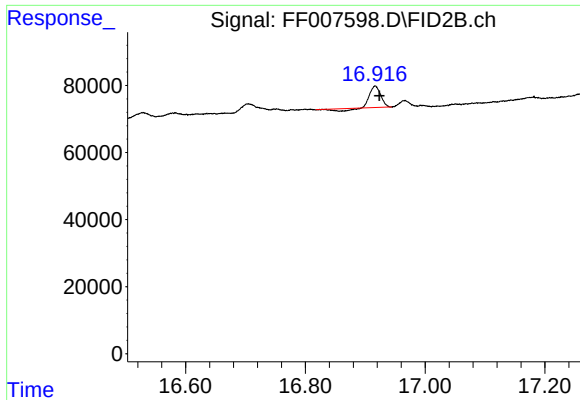

#12 N-OCTACOSANE


R.T.: 16.917 min
Delta R.T.: -0.007 min
Response: 67839
Conc: 0.44 ug/ml

Instrument :
FID_F
ClientSampleId :

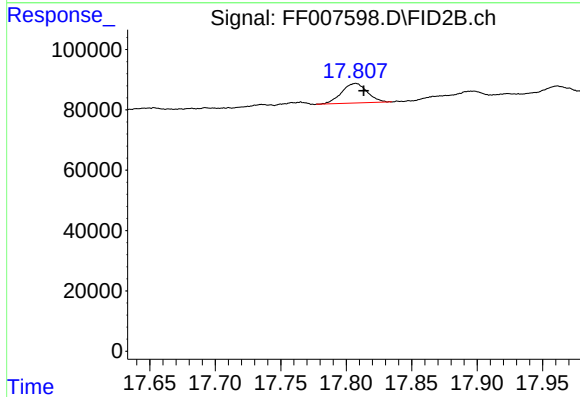


#13 N-TRIACONTANE

R.T.: 17.807 min
Delta R.T.: -0.007 min
Response: 87872
Conc: 0.59 ug/ml

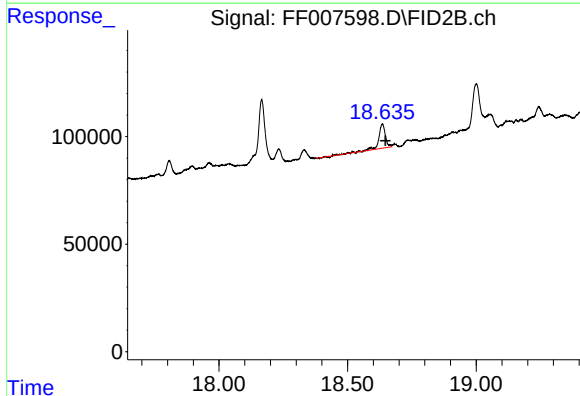

#14 N-DOTRIACONTANE

R.T.: 18.635 min
Delta R.T.: -0.012 min
Response: 201804
Conc: 1.45 ug/ml

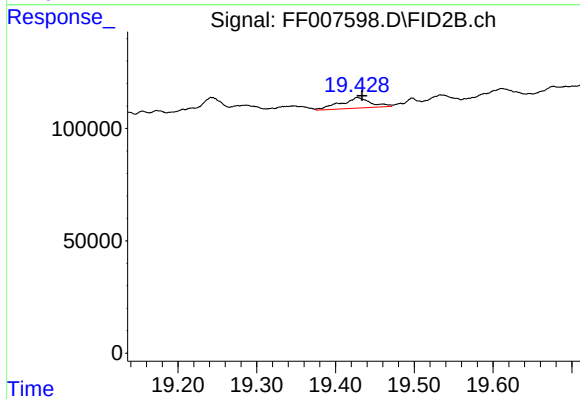

#15 N-TETRATRIACONTANE

R.T.: 19.428 min
Delta R.T.: -0.005 min
Response: 124758
Conc: 0.99 ug/ml