

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091720\
 Data File : FF007601.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2020 20:23
 Operator : DD\AJ
 Sample : L4062-01 2X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 18 02:00:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	901103	6.127 ug/ml
Target Compounds			
4) N-TETRADECANE	8.337f	173243	1.053 ug/ml
7) N-EICOSANE	12.702f	282606	1.681 ug/ml
10) N-TETRACOSANE	14.927	205390	1.259 ug/ml
12) N-OCTACOSANE	16.925	308933	2.013 ug/ml
13) N-TRIACONTANE	17.809	336901	2.279 ug/ml
14) N-DOTRIACONTANE	18.639	347936	2.508 ug/ml
15) N-TETRATRIACONTANE	19.429	121051	0.959 ug/ml
16) N-HEXATRIACONTANE	20.176	189771	1.588 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091720\
Data File : FF007601.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2020 20:23
Operator : DD\AJ
Sample : L4062-01 2X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 18 02:00:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

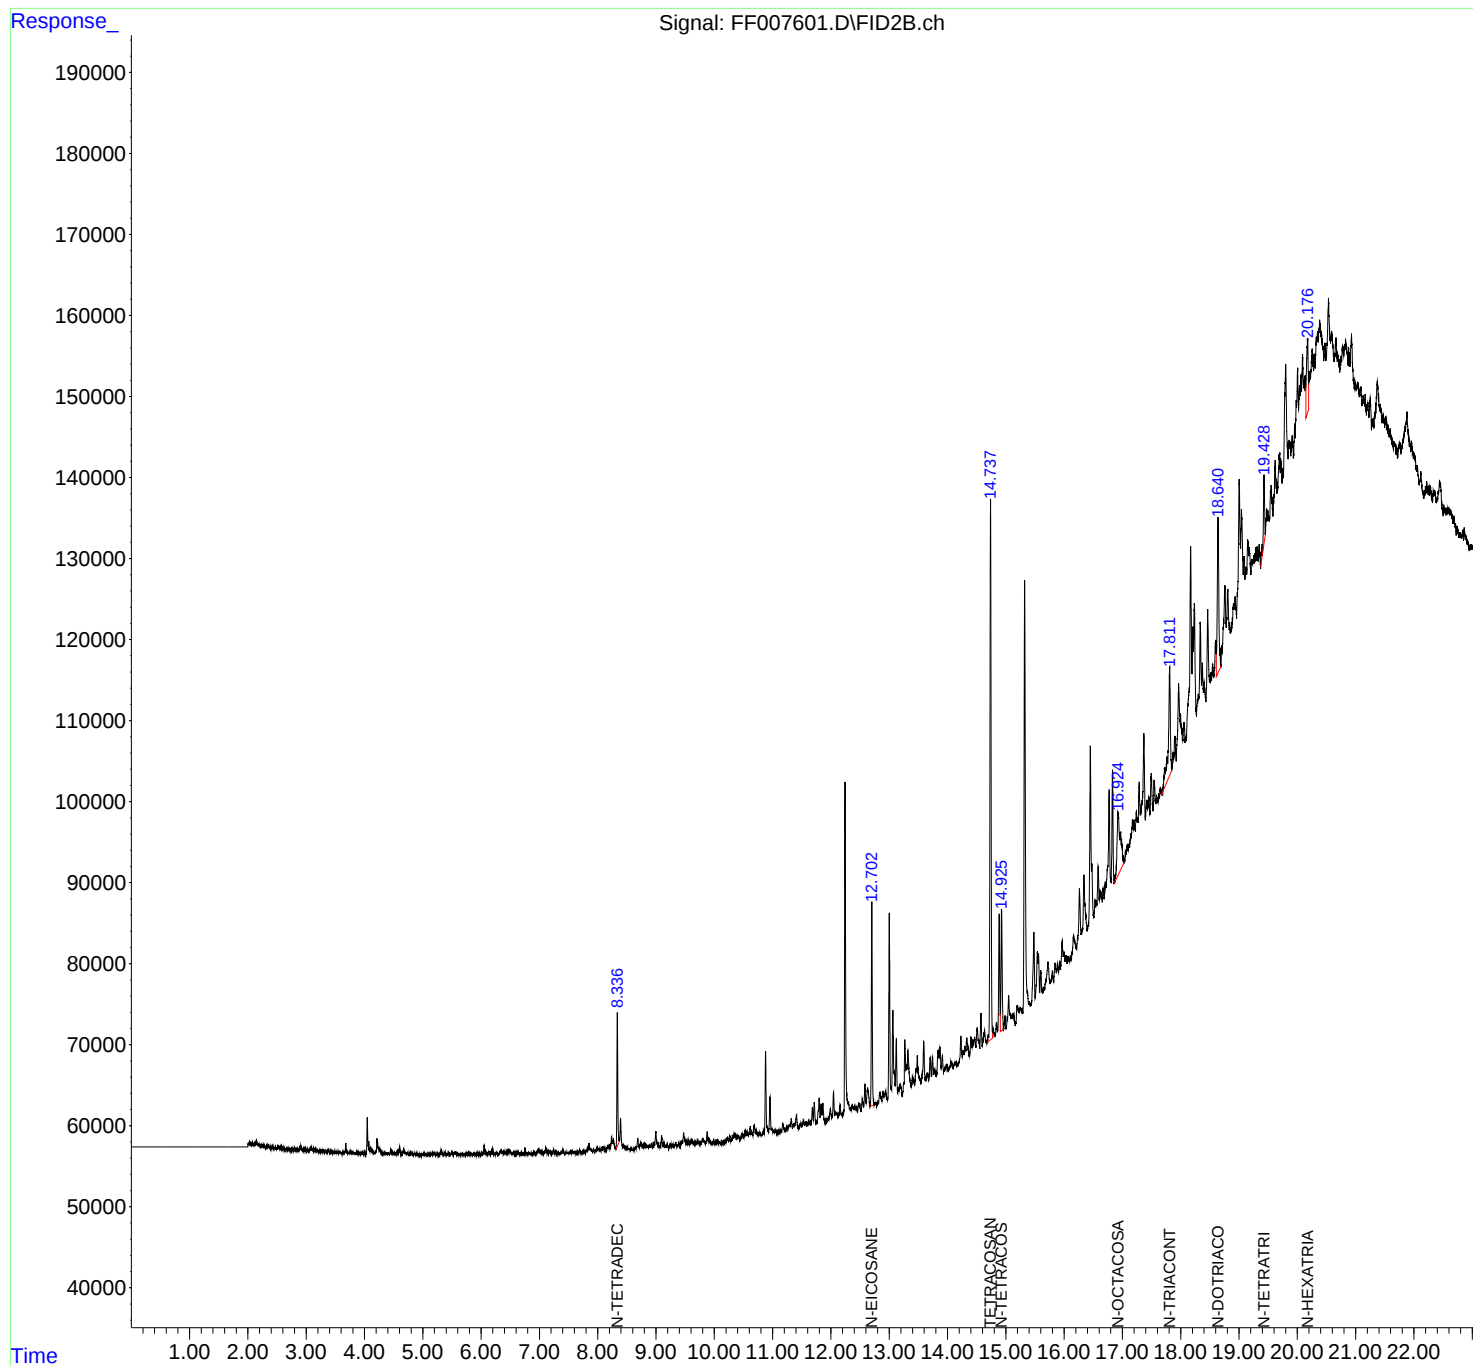


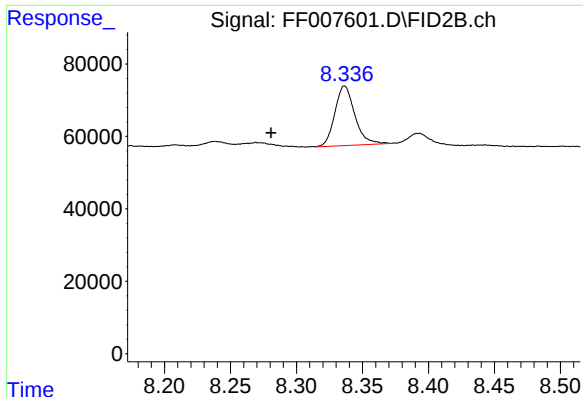

#4 N-TETRADECANE


R.T.: 8.337 min
Delta R.T.: 0.056 min
Response: 173243
Conc: 1.05 ug/ml

Instrument :
FID_F
ClientSampleId :

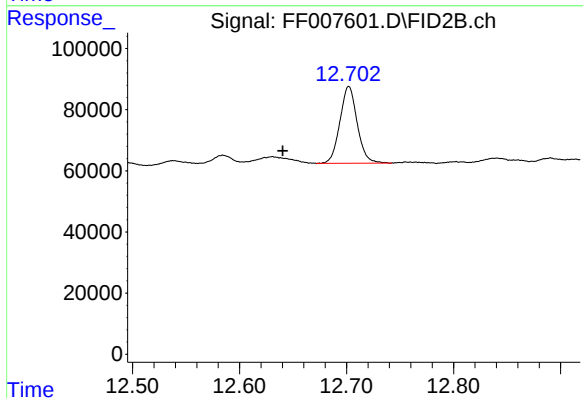


#7 N-EICOSANE

R.T.: 12.702 min
Delta R.T.: 0.062 min
Response: 282606
Conc: 1.68 ug/ml

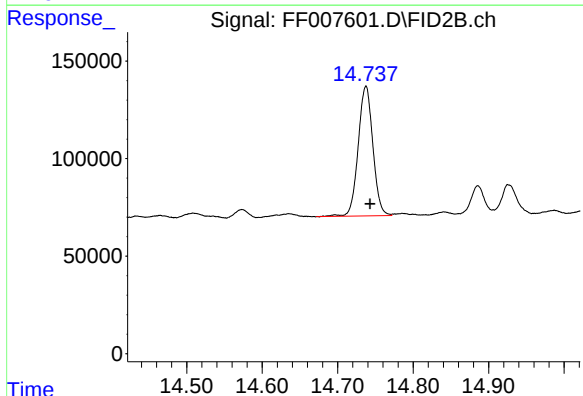


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.737 min
Delta R.T.: -0.006 min
Response: 901103
Conc: 6.13 ug/ml

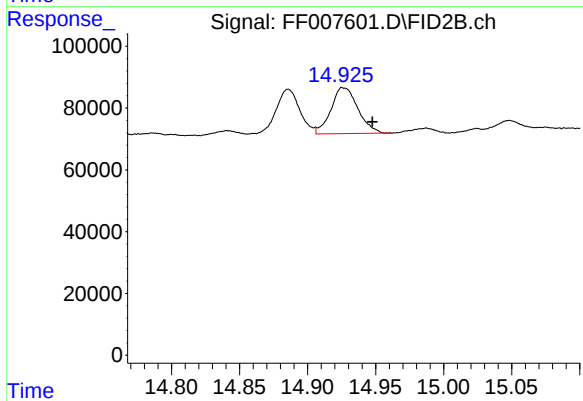

#10 N-TETRACOSANE


R.T.: 14.927 min
Delta R.T.: -0.021 min
Response: 205390
Conc: 1.26 ug/ml

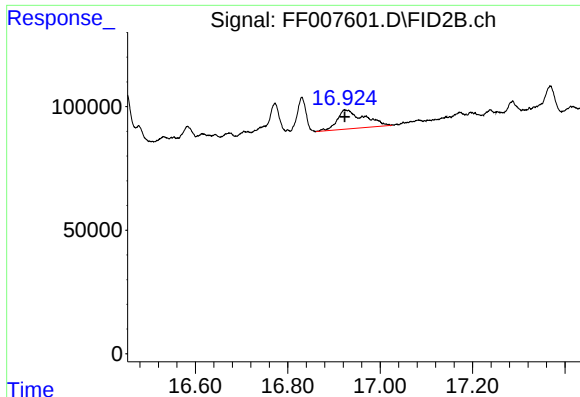

#12 N-OCTACOSANE


R.T.: 16.925 min
Delta R.T.: 0.002 min
Response: 308933
Conc: 2.01 ug/ml

Instrument :
FID_F
ClientSampleId :

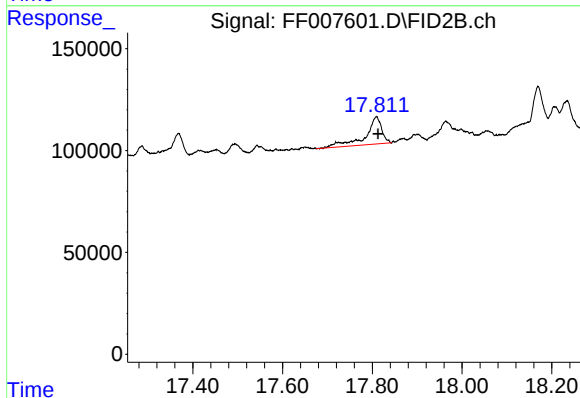


#13 N-TRIACONTANE

R.T.: 17.809 min
Delta R.T.: -0.004 min
Response: 336901
Conc: 2.28 ug/ml

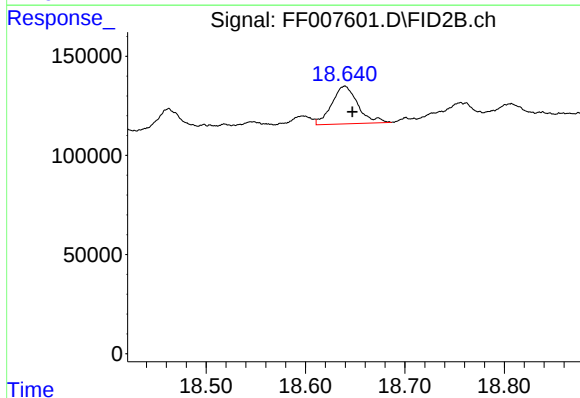


#14 N-DOTRIACONTANE

R.T.: 18.639 min
Delta R.T.: -0.008 min
Response: 347936
Conc: 2.51 ug/ml

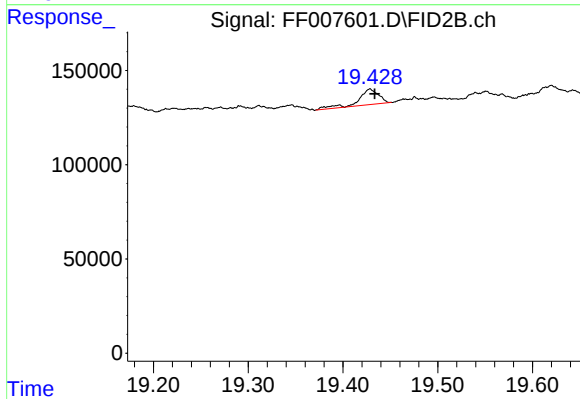

#15 N-TETRATRIACONTANE

R.T.: 19.429 min
Delta R.T.: -0.005 min
Response: 121051
Conc: 0.96 ug/ml

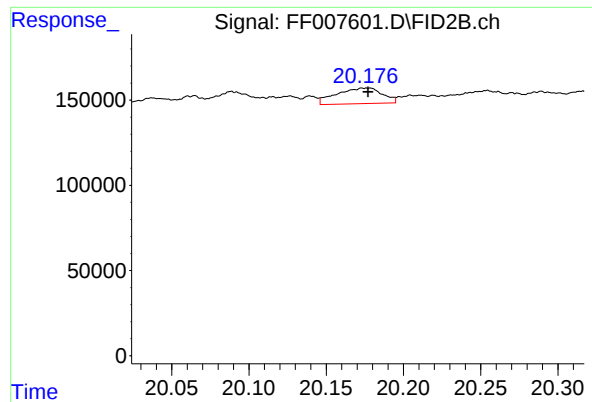

#16 N-HEXATRIACONTANE

R.T.: 20.176 min
Delta R.T.: -0.001 min
Response: 189771
Conc: 1.59 ug/ml

Instrument :
FID_F
ClientSampleId :