

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091720\
 Data File : FF007602.D
 Signal(s) : FID2B.ch
 Acq On : 17 Sep 2020 20:54
 Operator : DD\AJ
 Sample : L4062-02 2X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 18 02:00:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	1059342	7.203 ug/ml
Target Compounds			
4) N-TETRADECANE	8.336f	206604	1.256 ug/ml
7) N-EICOSANE	12.702f	691744	4.114 ug/ml
10) N-TETRACOSANE	14.926	375252	2.301 ug/ml
12) N-OCTACOSANE	16.931	187379	1.221 ug/ml
13) N-TRIACONTANE	17.808	174603	1.181 ug/ml
14) N-DOTRIACONTANE	18.636	201486	1.452 ug/ml
15) N-TETRATRIACONTANE	19.426	59553	0.472 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091720\
Data File : FF007602.D
Signal(s) : FID2B.ch
Acq On : 17 Sep 2020 20:54
Operator : DD\AJ
Sample : L4062-02 2X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 18 02:00:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

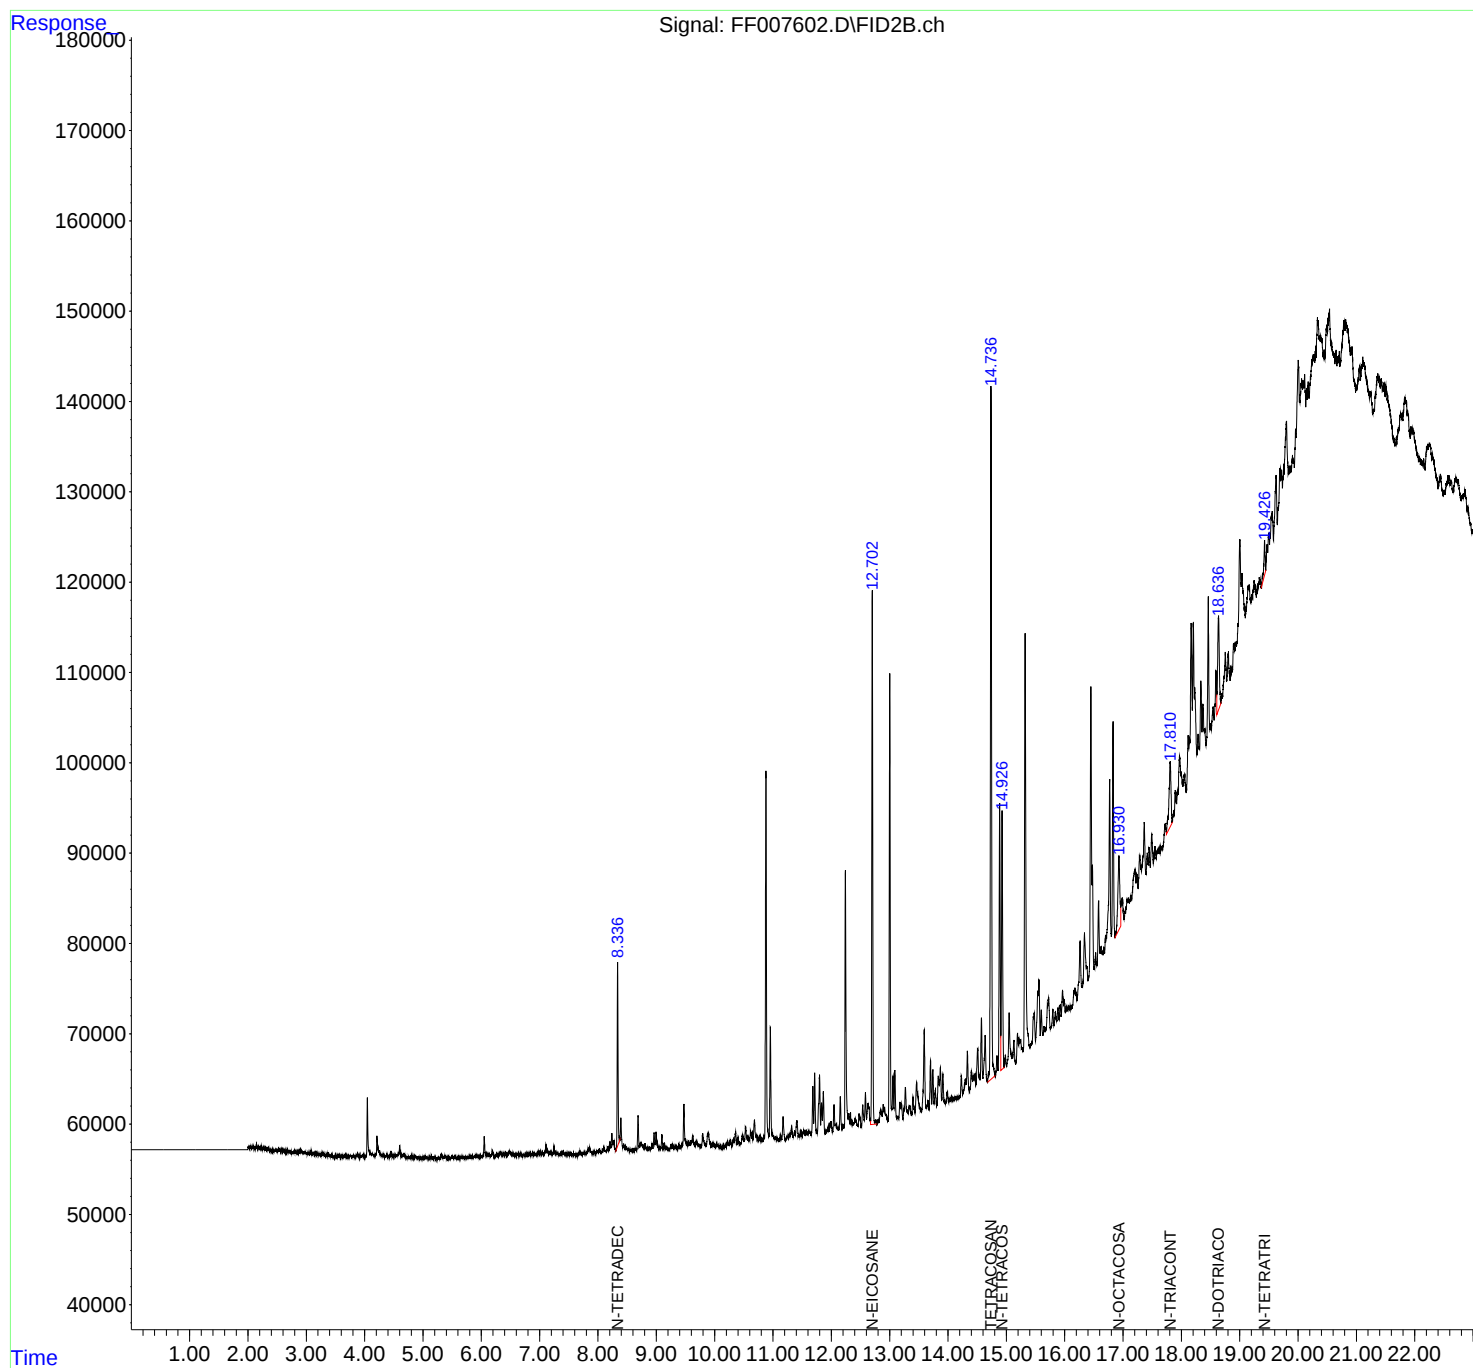


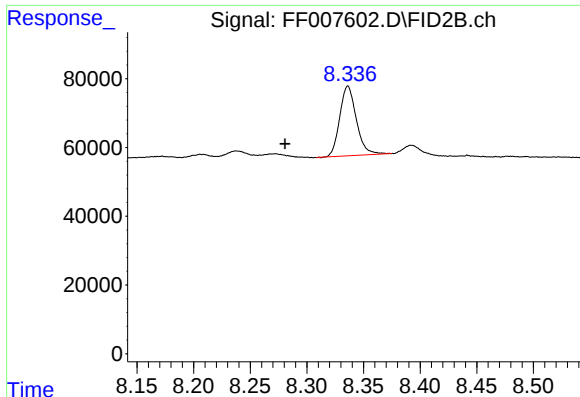

#4 N-TETRADECANE


R.T.: 8.336 min
Delta R.T.: 0.056 min
Response: 206604
Conc: 1.26 ug/ml

Instrument :
FID_F
ClientSampleId :

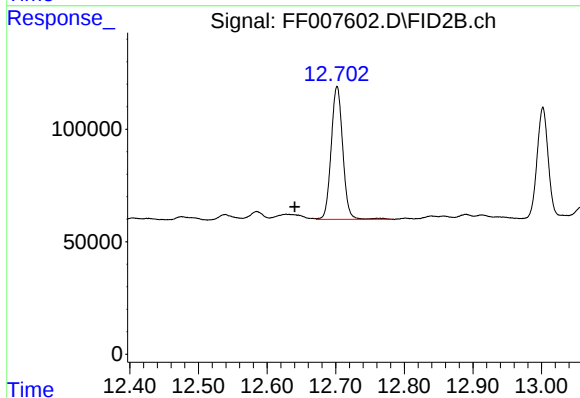


#7 N-EICOSANE

R.T.: 12.702 min
Delta R.T.: 0.062 min
Response: 691744
Conc: 4.11 ug/ml

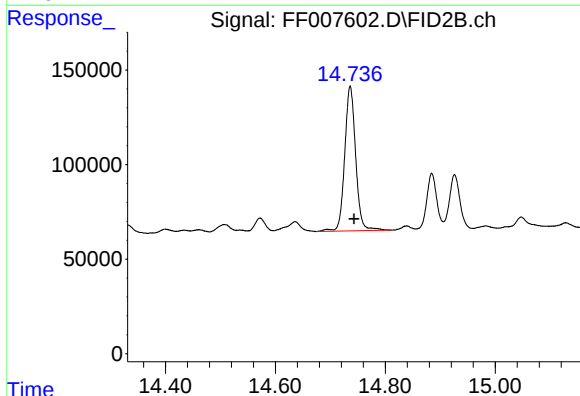


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.736 min
Delta R.T.: -0.007 min
Response: 1059342
Conc: 7.20 ug/ml

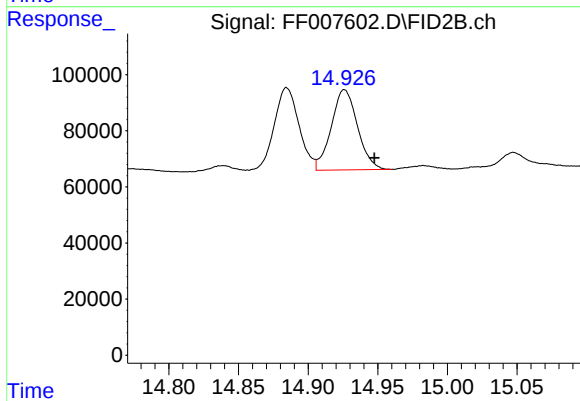

#10 N-TETRACOSANE


R.T.: 14.926 min
Delta R.T.: -0.021 min
Response: 375252
Conc: 2.30 ug/ml

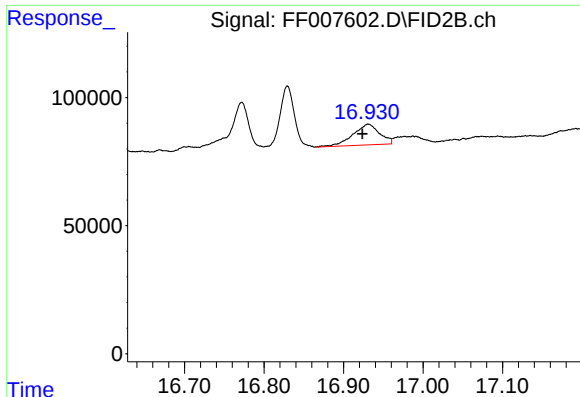

#12 N-OCTACOSANE


R.T.: 16.931 min
Delta R.T.: 0.008 min
Response: 187379
Conc: 1.22 ug/ml

Instrument :
FID_F
ClientSampleId :

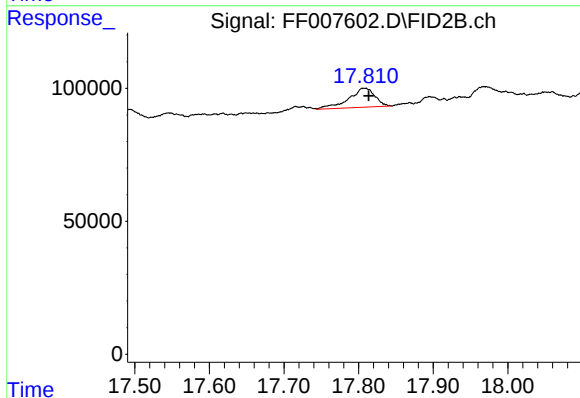


#13 N-TRIACONTANE

R.T.: 17.808 min
Delta R.T.: -0.005 min
Response: 174603
Conc: 1.18 ug/ml

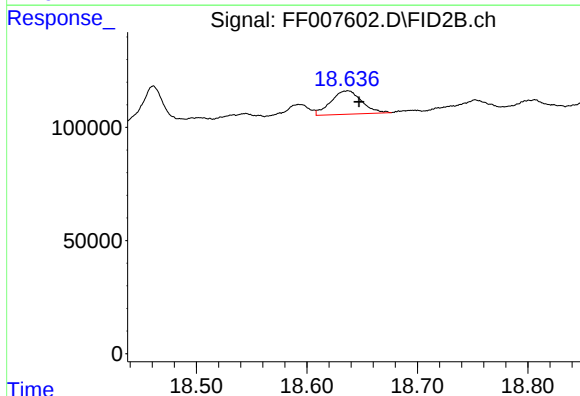

#14 N-DOTRIACONTANE

R.T.: 18.636 min
Delta R.T.: -0.011 min
Response: 201486
Conc: 1.45 ug/ml

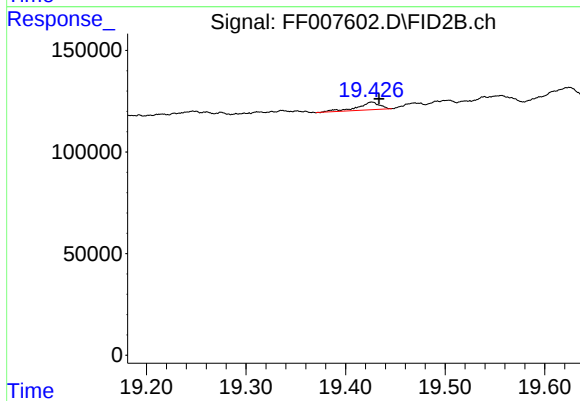

#15 N-TETRATRIACONTANE

R.T.: 19.426 min
Delta R.T.: -0.007 min
Response: 59553
Conc: 0.47 ug/ml