

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091819\
 Data File : FF005616.D
 Signal(s) : FID2B.ch
 Acq On : 18 Sep 2019 15:25
 Operator : DD\AJ
 Sample : PB123113BS
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB123113BS

Integration File: autoint1.e
 Quant Time: Sep 18 16:34:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.623	2347401	21.937 ug/ml
Target Compounds			
2) N-DECANE	4.347	2938335	20.552 ug/ml
3) N-DODECANE	6.368	2867145	20.001 ug/ml
4) N-TETRADECANE	8.160	2723982	19.320 ug/ml
5) N-HEXADECANE	9.762	2795099	19.985 ug/ml
6) N-OCTADECANE	11.205	2727917	20.275 ug/ml
7) N-EICOSANE	12.518	2701435	20.599 ug/ml
8) N-DOCOSANE	13.720	2674692	21.243 ug/ml
10) N-TETRACOSANE	14.828	2720300	22.244 ug/ml
11) N-HEXACOSANE	15.853	2757409	23.035 ug/ml
12) N-OCTACOSANE	16.807	2820800	23.640 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091819\
Data File : FF005616.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2019 15:25
Operator : DD\AJ
Sample : PB123113BS
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB123113BS

Integration File: autoint1.e
Quant Time: Sep 18 16:34:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

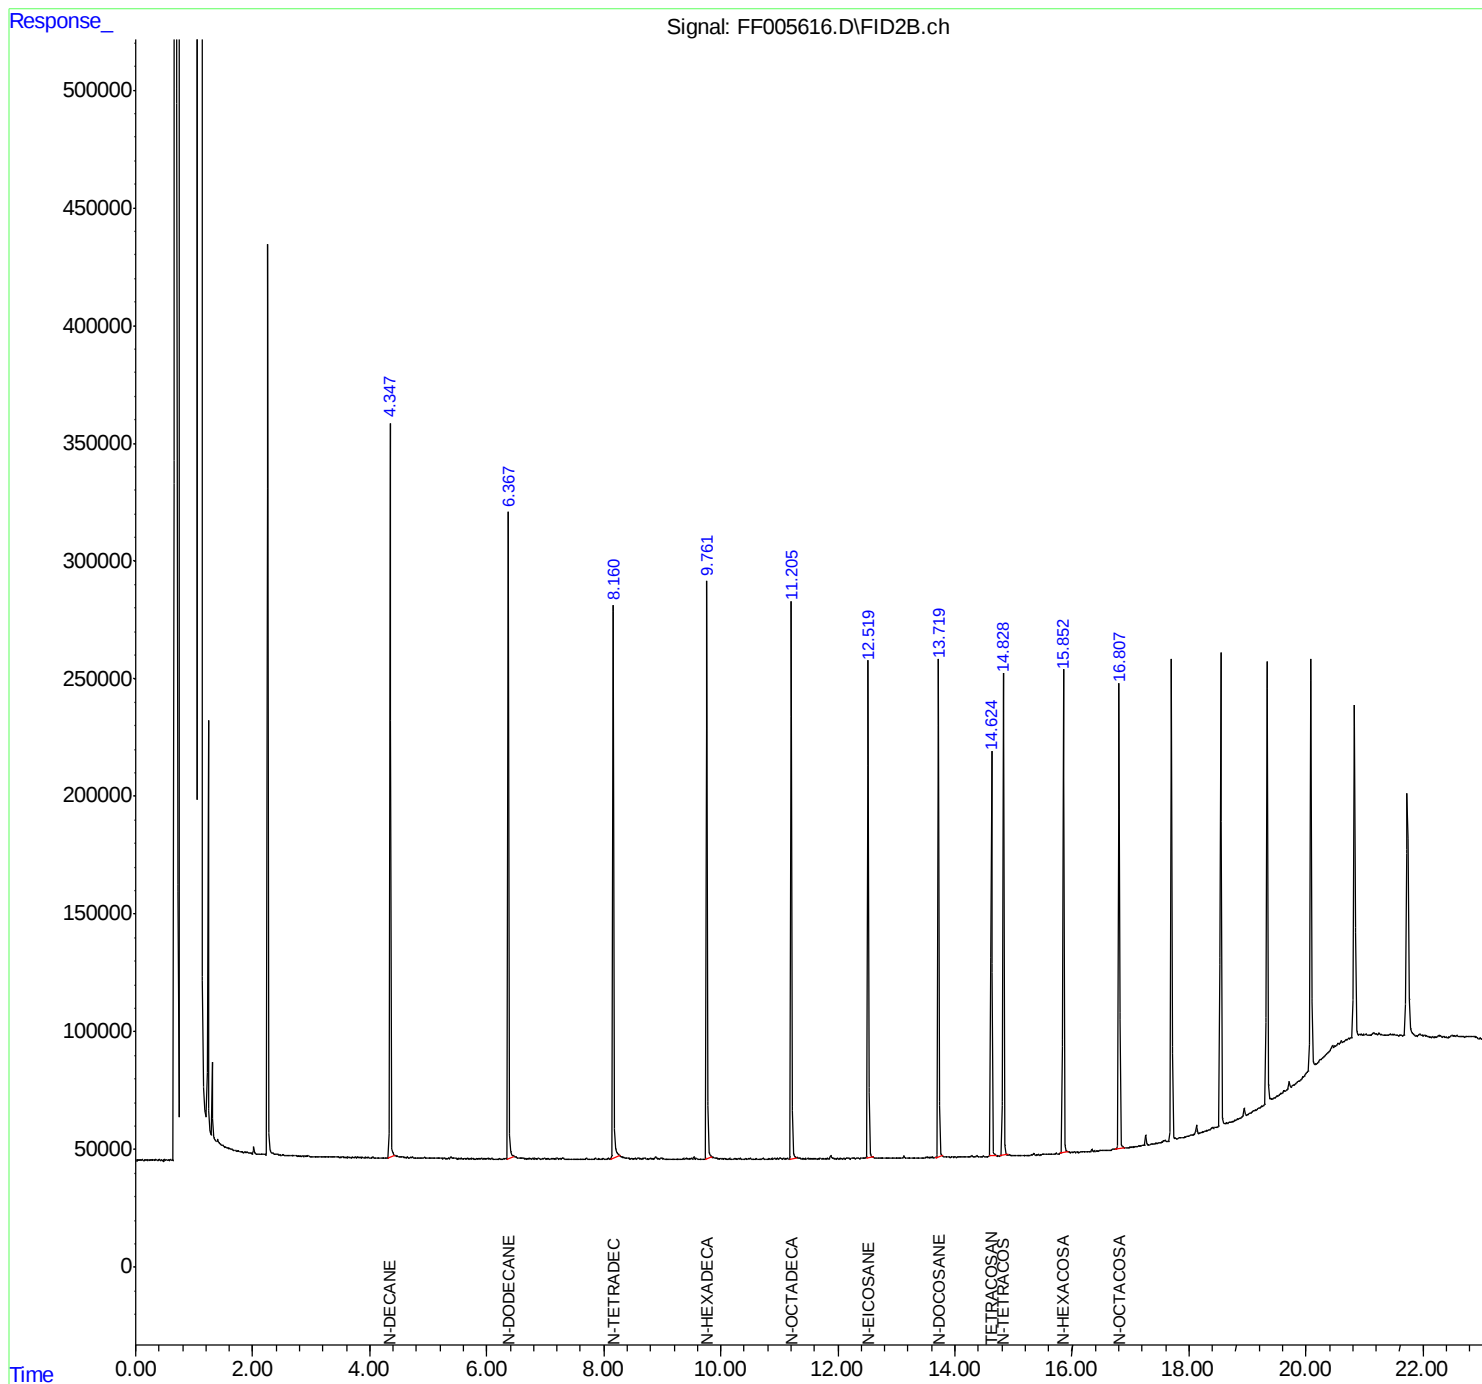


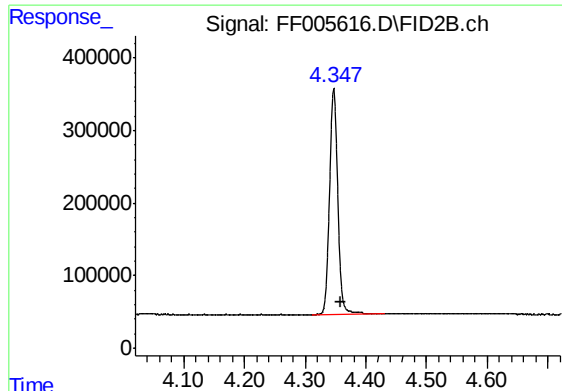

#2 N-DECANE


R.T.: 4.347 min
Delta R.T.: -0.012 min
Response: 2938335
Conc: 20.55 ug/ml

Instrument :
FID_F
ClientSampleId :
PB123113BS

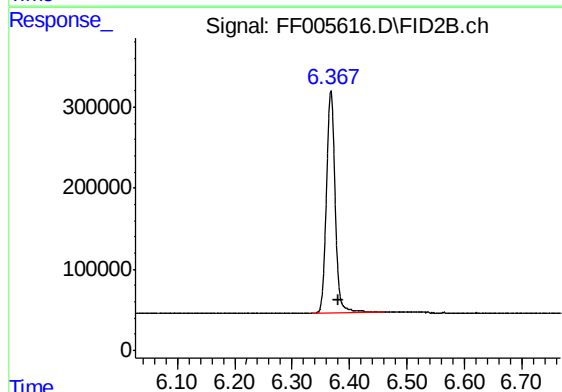


#3 N-DODECANE

R.T.: 6.368 min
Delta R.T.: -0.012 min
Response: 2867145
Conc: 20.00 ug/ml

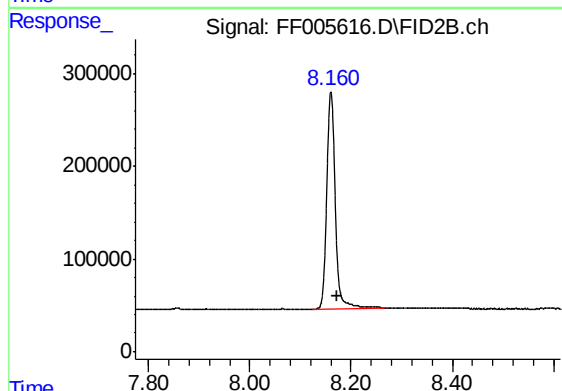


#4 N-TETRADECANE

R.T.: 8.160 min
Delta R.T.: -0.012 min
Response: 2723982
Conc: 19.32 ug/ml

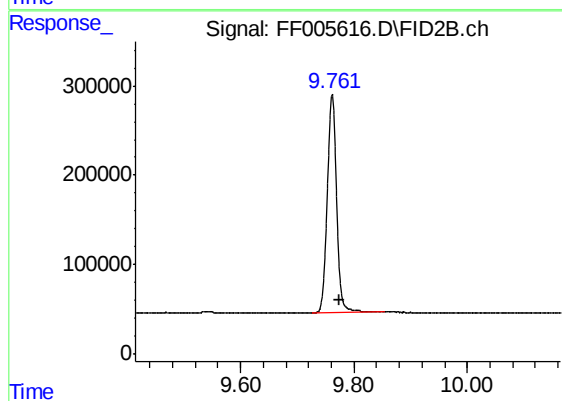

#5 N-HEXADECANE


R.T.: 9.762 min
Delta R.T.: -0.012 min
Response: 2795099
Conc: 19.98 ug/ml

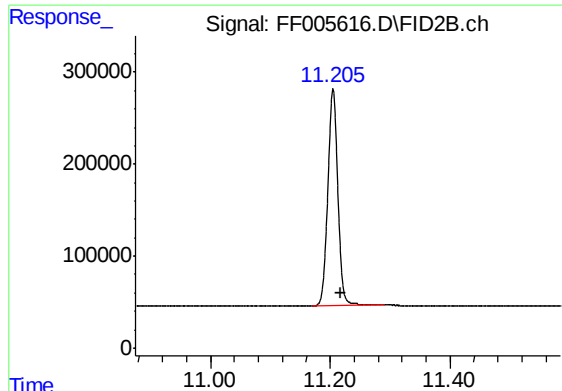

#6 N-OCTADECANE


R.T.: 11.205 min
Delta R.T.: -0.012 min
Response: 2727917
Conc: 20.28 ug/ml

Instrument :
FID_F
ClientSampleId :
PB123113BS

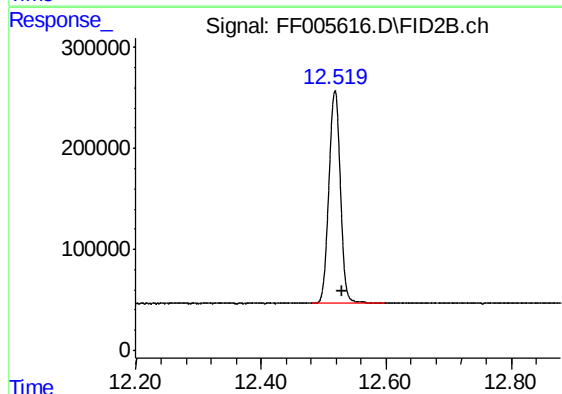


#7 N-EICOSANE

R.T.: 12.518 min
Delta R.T.: -0.012 min
Response: 2701435
Conc: 20.60 ug/ml

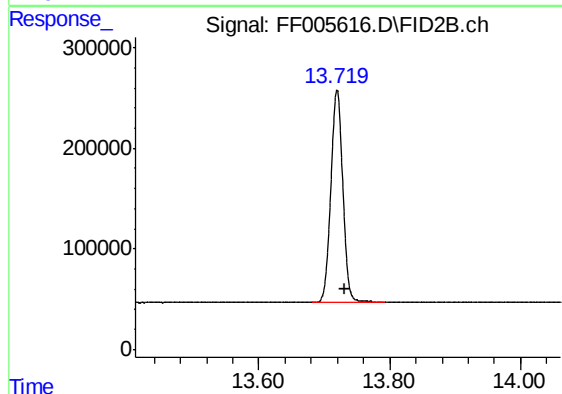


#8 N-DOCOSANE

R.T.: 13.720 min
Delta R.T.: -0.012 min
Response: 2674692
Conc: 21.24 ug/ml

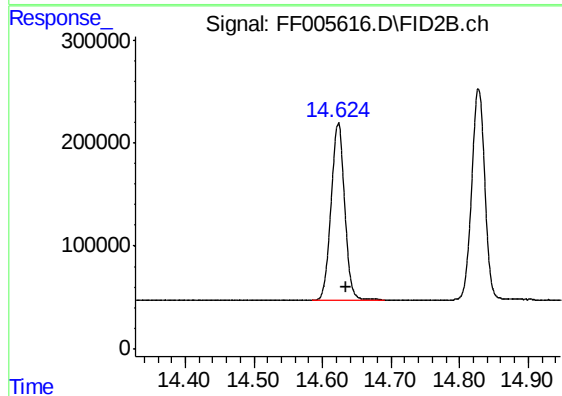

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.623 min
Delta R.T.: -0.011 min
Response: 2347401
Conc: 21.94 ug/ml

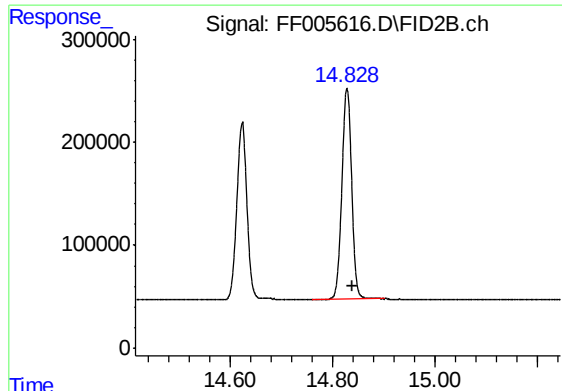

#10 N-TETRACOSANE


R.T.: 14.828 min
Delta R.T.: -0.012 min
Response: 2720300
Conc: 22.24 ug/ml

Instrument :
FID_F
ClientSampleId :
PB123113BS

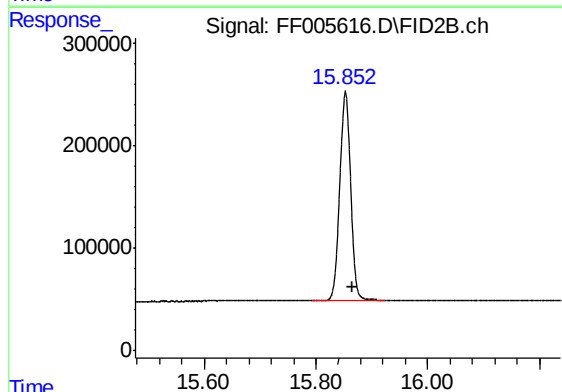

#11 N-HEXACOSANE

R.T.: 15.853 min
Delta R.T.: -0.011 min
Response: 2757409
Conc: 23.04 ug/ml

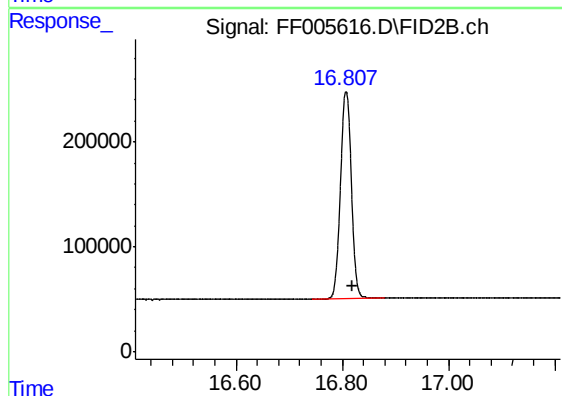

#12 N-OCTACOSANE

R.T.: 16.807 min
Delta R.T.: -0.012 min
Response: 2820800
Conc: 23.64 ug/ml