

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
 Data File : FF007608.D
 Signal(s) : FID2B.ch
 Acq On : 18 Sep 2020 11:12
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 19 00:31:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.776	146726	0.998 ug/ml
Target Compounds			
3) N-DODECANE	6.471	4035697	24.807 ug/ml
11) N-HEXACOSANE	15.962	88002	0.557 ug/ml
12) N-OCTACOSANE	16.917	3440614	22.419 ug/ml
13) N-TRIACONTANE	17.804	434867	2.942 ug/ml
14) N-DOTRIACONTANE	18.641	490207	3.533 ug/ml
15) N-TETRATRIACONTANE	19.429	356392	2.824 ug/ml
16) N-HEXATRIACONTANE	20.173	257911	2.158 ug/ml
17) N-OCTATRIACONTANE	20.932	249898	2.340 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007608.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 11:12
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 19 00:31:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

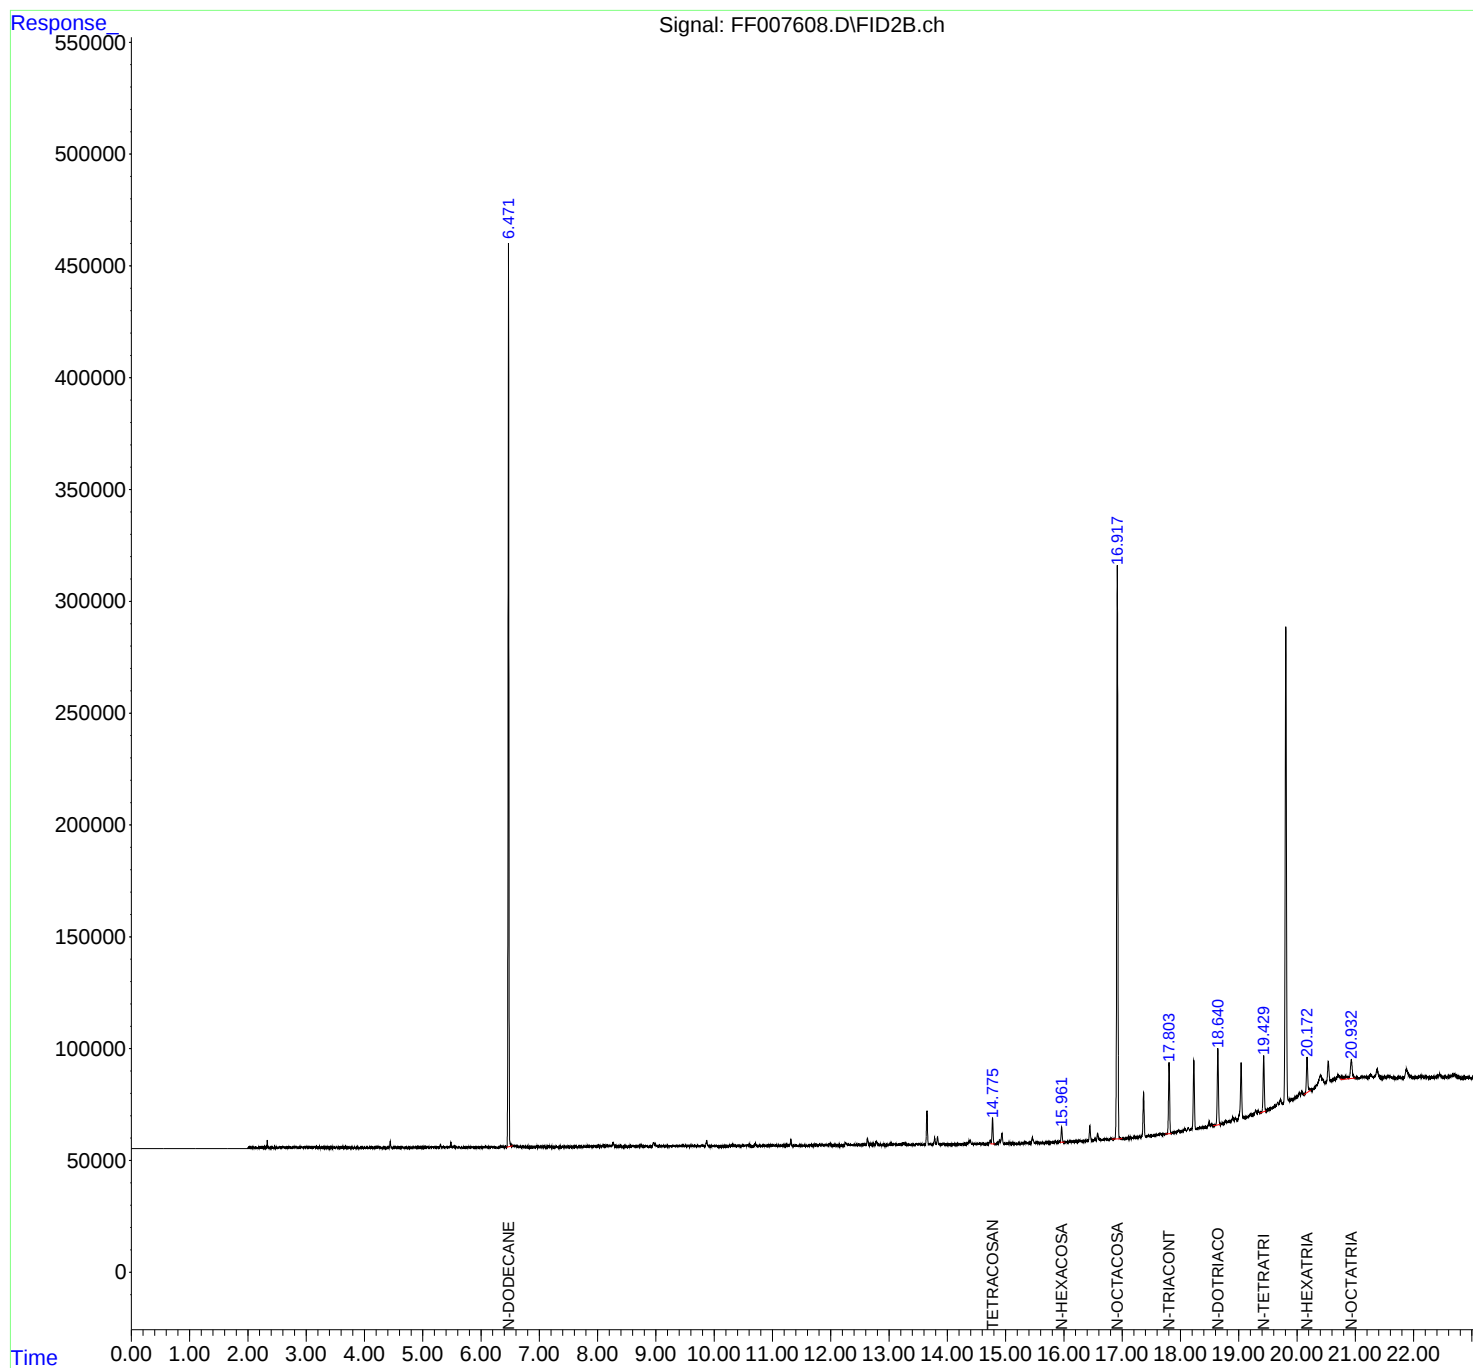


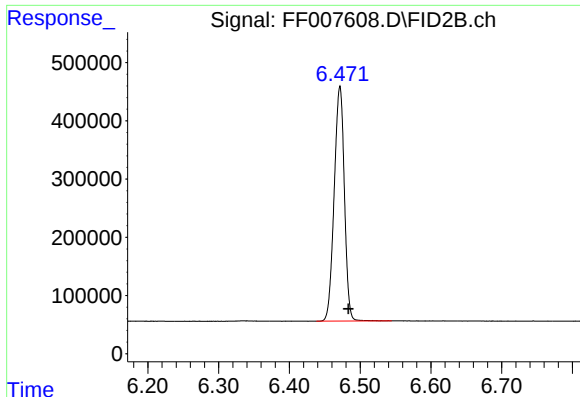

#3 N-DODECANE


R.T.: 6.471 min
Delta R.T.: -0.012 min
Response: 4035697
Conc: 24.81 ug/ml

Instrument :
FID_F
ClientSampleId :

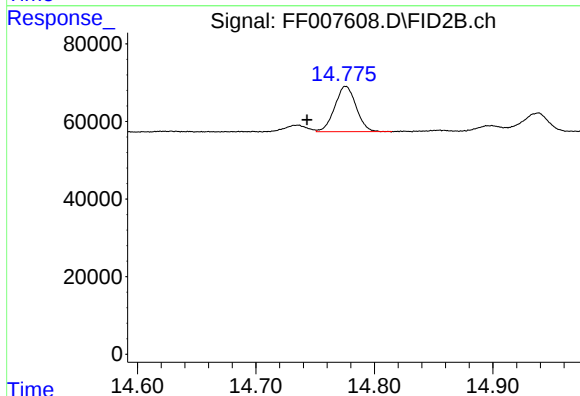


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.776 min
Delta R.T.: 0.033 min
Response: 146726
Conc: 1.00 ug/ml

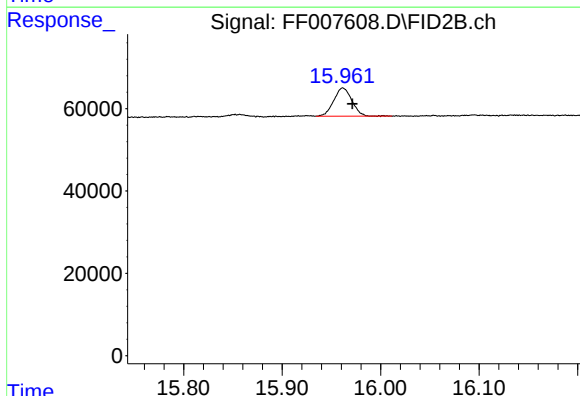


#11 N-HEXACOSANE

R.T.: 15.962 min
Delta R.T.: -0.010 min
Response: 88002
Conc: 0.56 ug/ml

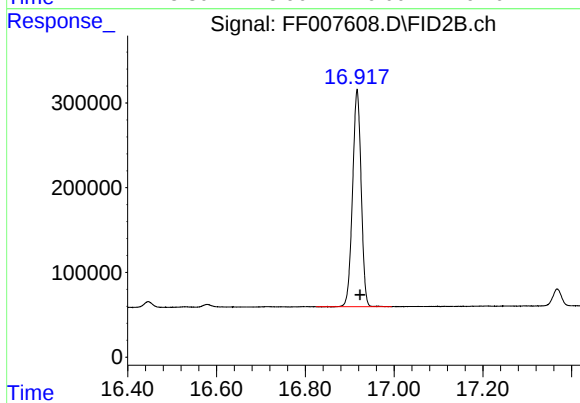

#12 N-OCTACOSANE


R.T.: 16.917 min
Delta R.T.: -0.007 min
Response: 3440614
Conc: 22.42 ug/ml

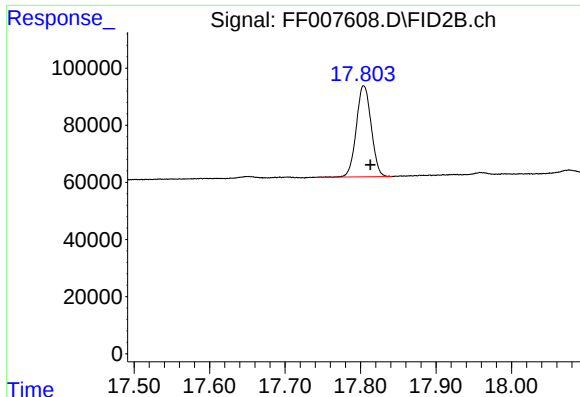

#13 N-TRIACONTANE


R.T.: 17.804 min
Delta R.T.: -0.009 min
Response: 434867
Conc: 2.94 ug/ml

Instrument :
FID_F
ClientSampleId :

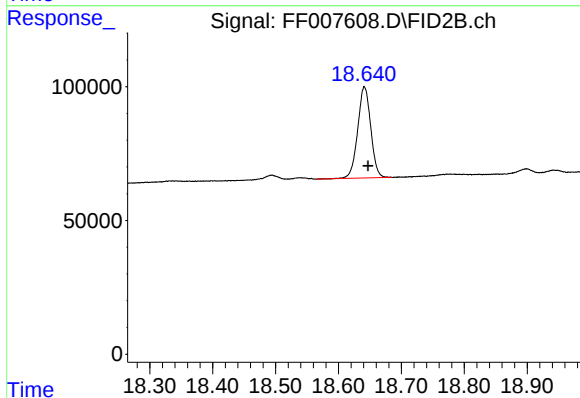


#14 N-DOTRIACONTANE

R.T.: 18.641 min
Delta R.T.: -0.006 min
Response: 490207
Conc: 3.53 ug/ml

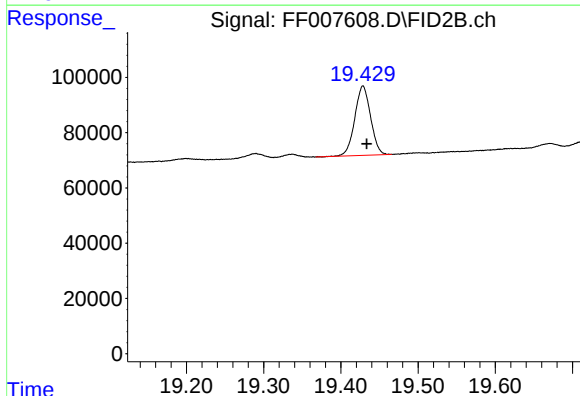


#15 N-TETRATRIACONTANE

R.T.: 19.429 min
Delta R.T.: -0.005 min
Response: 356392
Conc: 2.82 ug/ml

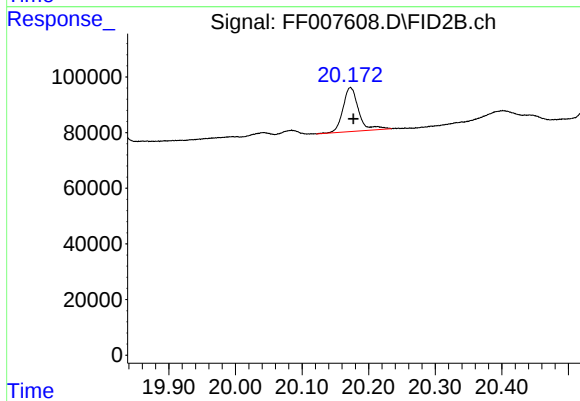

#16 N-HEXATRIACONTANE

R.T.: 20.173 min
Delta R.T.: -0.004 min
Response: 257911
Conc: 2.16 ug/ml

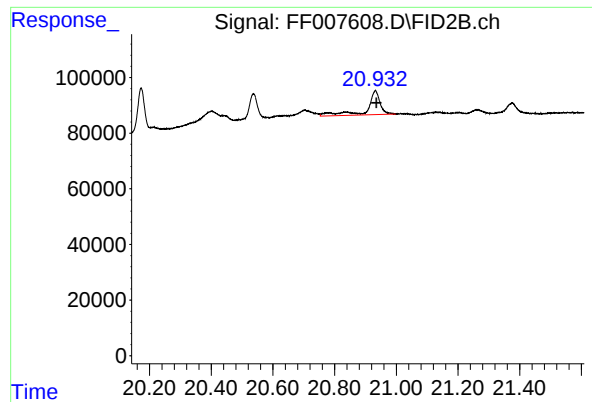

#17 N-OCTATRIACONTANE

R.T.: 20.932 min
Delta R.T.: -0.004 min
Response: 249898
Conc: 2.34 ug/ml

Instrument :
FID_F
ClientSampleId :