

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
 Data File : FF007609.D
 Signal(s) : FID2B.ch
 Acq On : 18 Sep 2020 11:42
 Operator : DD\AJ
 Sample : L4034-01 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 19 00:31:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.734	334897	2.277 ug/ml
Target Compounds				
3)	N-DODECANE	6.432f	126918	0.780 ug/ml
4)	N-TETRADECANE	8.334f	108707	0.661 ug/ml
7)	N-EICOSANE	12.699f	335240	1.994 ug/ml
10)	N-TETRACOSANE	14.924	230298	1.412 ug/ml
14)	N-DOTRIACONTANE	18.630	175487	1.265 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007609.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 11:42
Operator : DD\AJ
Sample : L4034-01 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 19 00:31:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

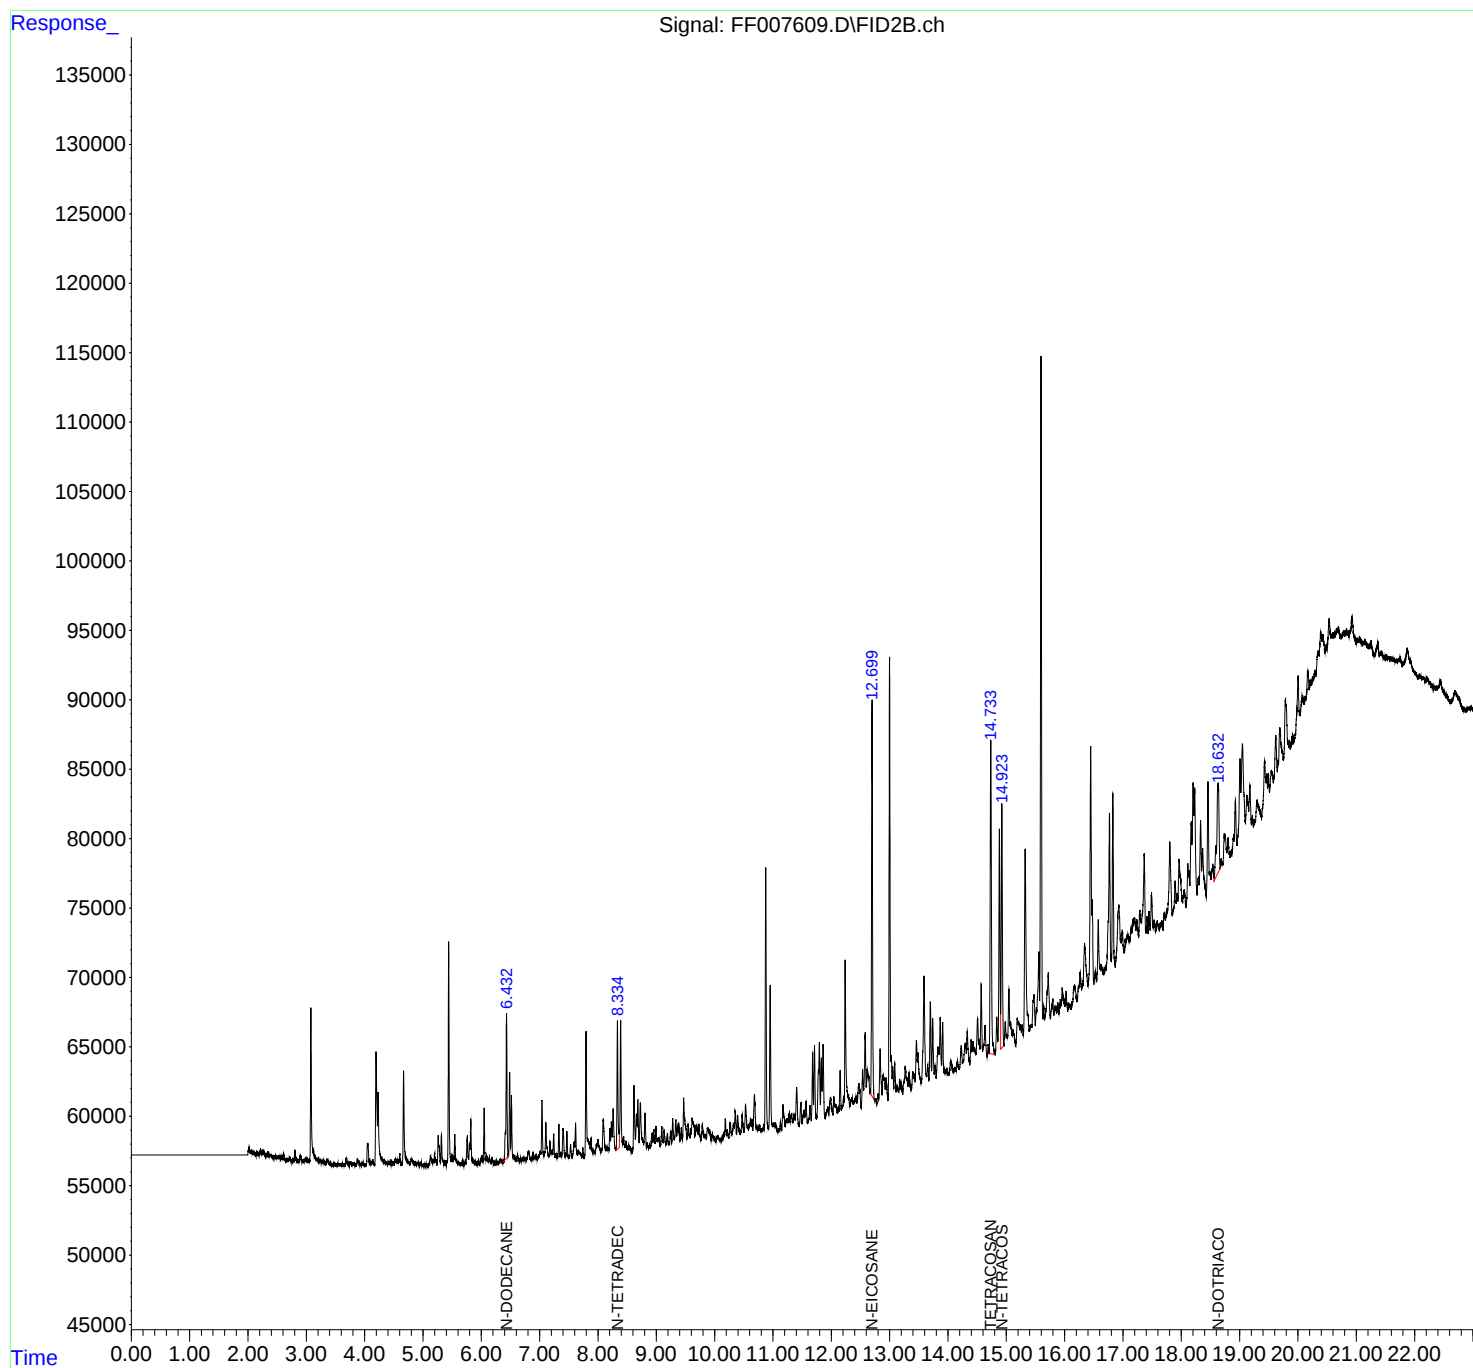


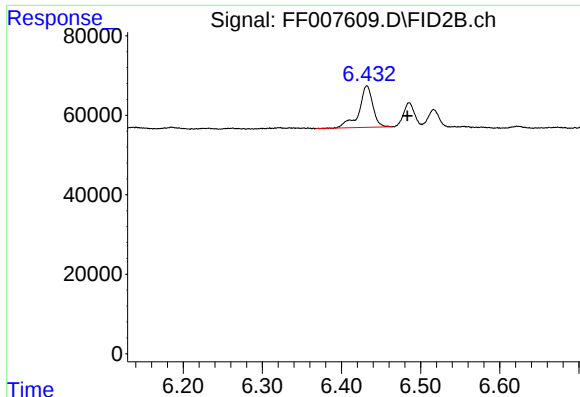

#3 N-DODECANE


R.T.: 6.432 min
Delta R.T.: -0.051 min
Response: 126918
Conc: 0.78 ug/ml

Instrument :
FID_F
ClientSampleId :

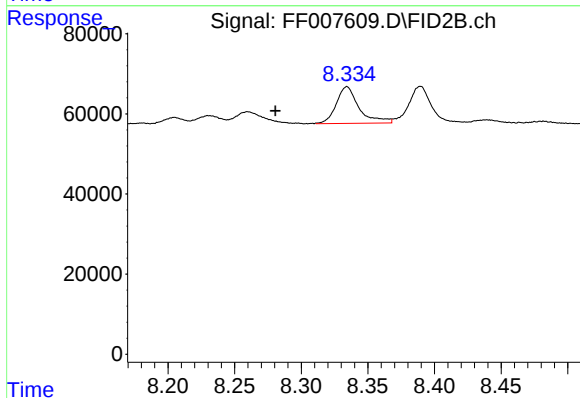


#4 N-TETRADECANE

R.T.: 8.334 min
Delta R.T.: 0.054 min
Response: 108707
Conc: 0.66 ug/ml

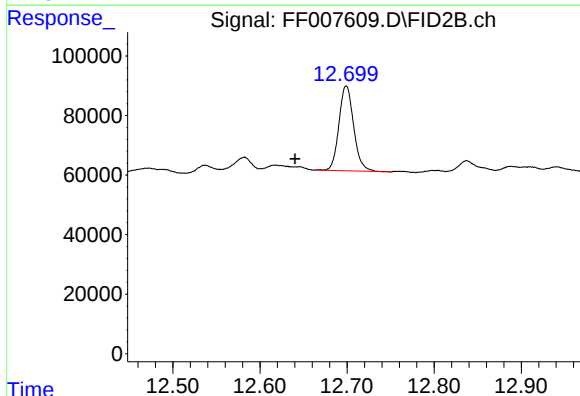


#7 N-EICOSANE

R.T.: 12.699 min
Delta R.T.: 0.059 min
Response: 335240
Conc: 1.99 ug/ml

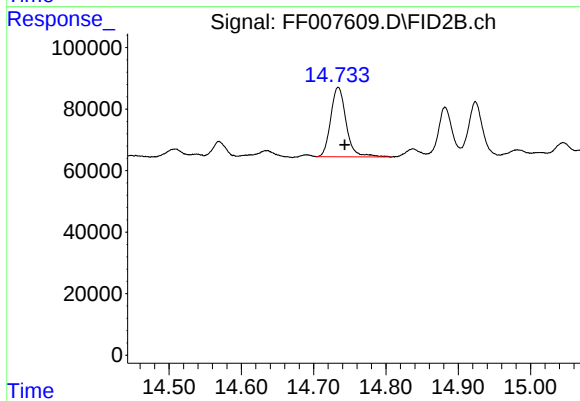

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.734 min
Delta R.T.: -0.009 min
Response: 334897
Conc: 2.28 ug/ml

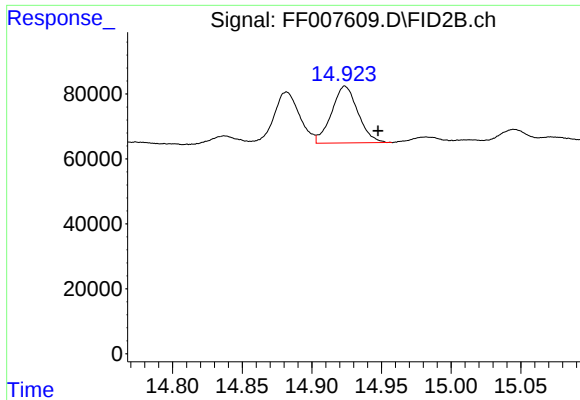

#10 N-TETRACOSANE

R.T.: 14.924 min
Delta R.T.: -0.024 min
Response: 230298
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :

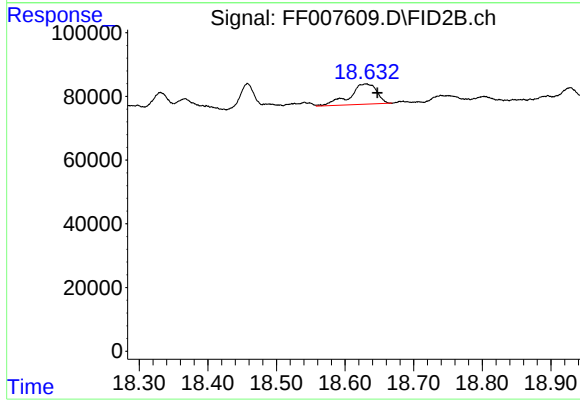

#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: -0.017 min
Response: 175487
Conc: 1.26 ug/ml