

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
 Data File : FF007610.D
 Signal(s) : FID2B.ch
 Acq On : 18 Sep 2020 12:13
 Operator : DD\AJ
 Sample : L4062-01 5X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 19 00:31:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.735	385333	2.620 ug/ml
Target Compounds			
7) N-EICOSANE	12.699f	112339	0.668 ug/ml
13) N-TRIACONTANE	17.805	156918	1.062 ug/ml
14) N-DOTRIACONTANE	18.638	139988	1.009 ug/ml
15) N-TETRATRIACONTANE	19.426	32749	0.259 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007610.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 12:13
Operator : DD\AJ
Sample : L4062-01 5X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 19 00:31:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

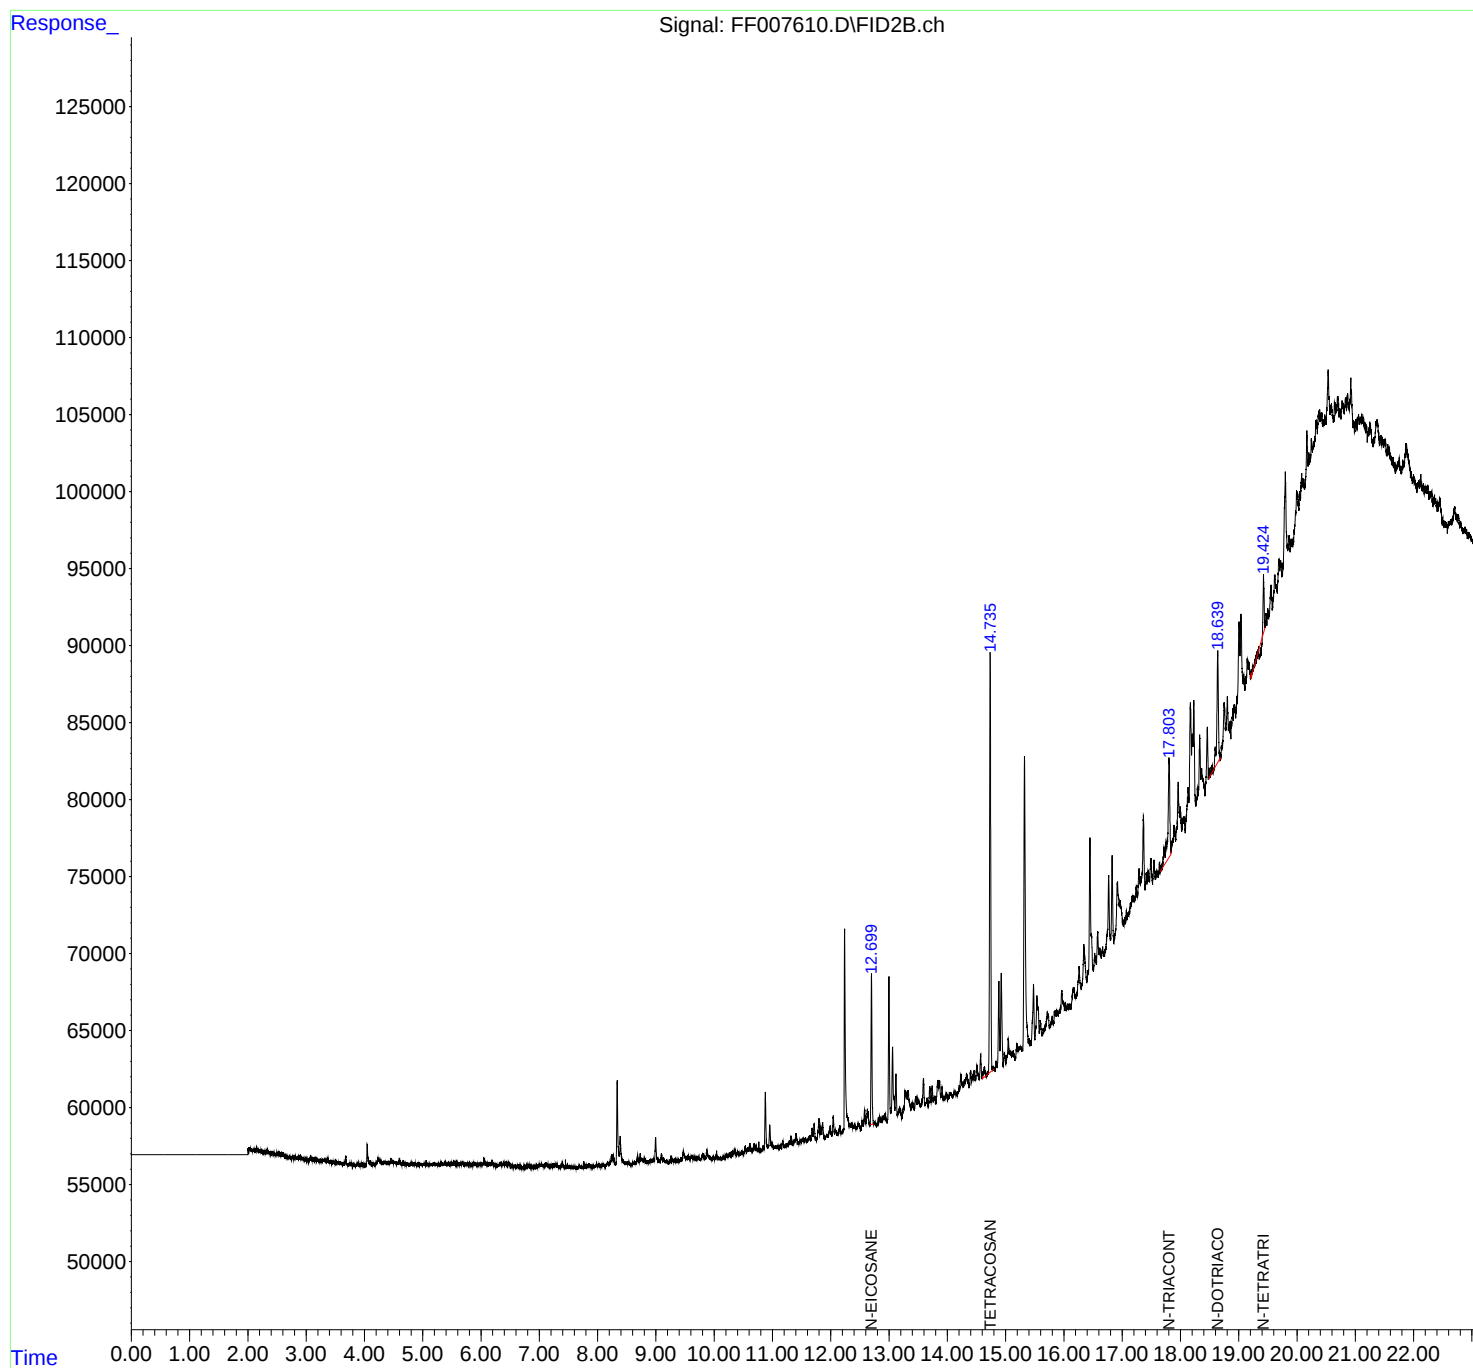


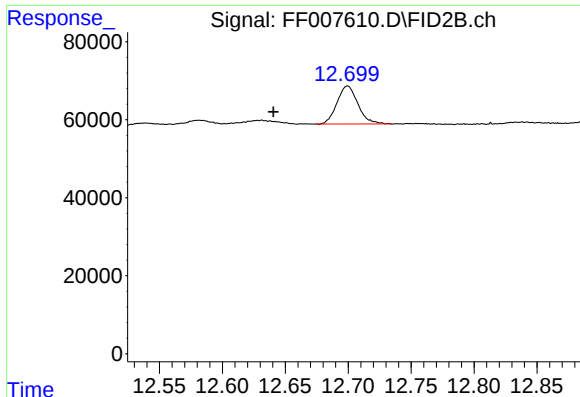

#7 N-EICOSANE


R.T.: 12.699 min
Delta R.T.: 0.059 min
Response: 112339
Conc: 0.67 ug/ml

Instrument :
FID_F
ClientSampleId :

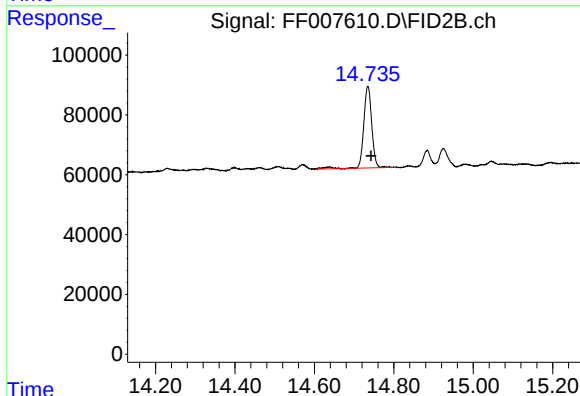


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.735 min
Delta R.T.: -0.008 min
Response: 385333
Conc: 2.62 ug/ml

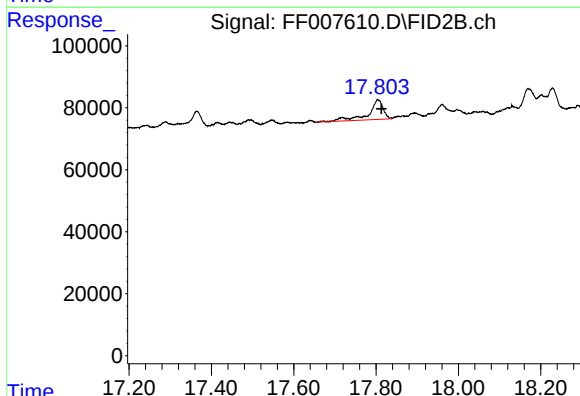


#13 N-TRIACONTANE

R.T.: 17.805 min
Delta R.T.: -0.008 min
Response: 156918
Conc: 1.06 ug/ml

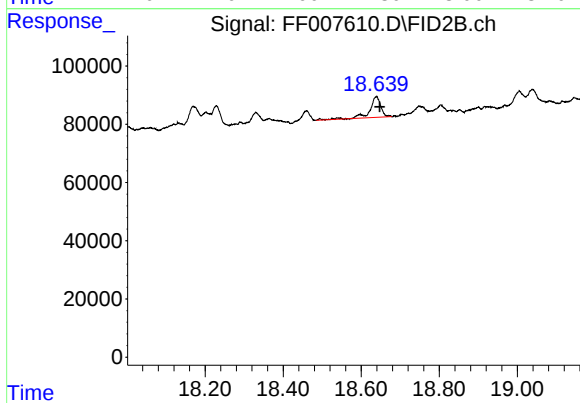

#14 N-DOTRIACONTANE

R.T.: 18.638 min
Delta R.T.: -0.009 min
Response: 139988
Conc: 1.01 ug/ml

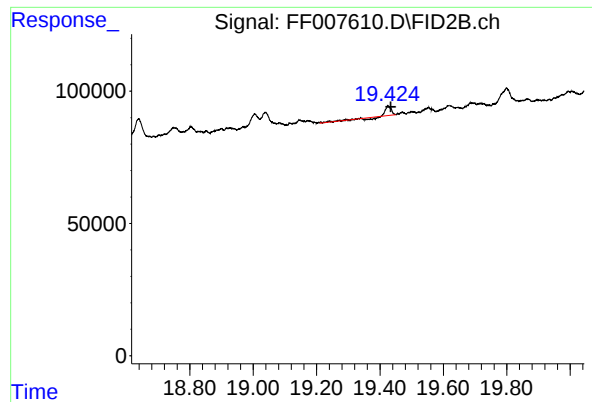

#15 N-TETRATRIACONTANE

R.T.: 19.426 min

Delta R.T.: -0.008 min

Response: 32749

Conc: 0.26 ug/ml

Instrument :
FID_F
ClientSampleId :