

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
 Data File : FF007622.D
 Signal(s) : FID2B.ch
 Acq On : 18 Sep 2020 19:21
 Operator : DD\AJ
 Sample : L4074-02 10X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 19 00:34:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.739	303847	2.066 ug/ml
Target Compounds			
4) N-TETRADECANE	8.337f	57991	0.352 ug/ml
7) N-EICOSANE	12.704f	167717	0.998 ug/ml
14) N-DOTRIACONTANE	18.641	133248	0.960 ug/ml
15) N-TETRATRIACONTANE	19.432	126593	1.003 ug/ml
16) N-HEXATRIACONTANE	20.173	142684	1.194 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007622.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 19:21
Operator : DD\AJ
Sample : L4074-02 10X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 19 00:34:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

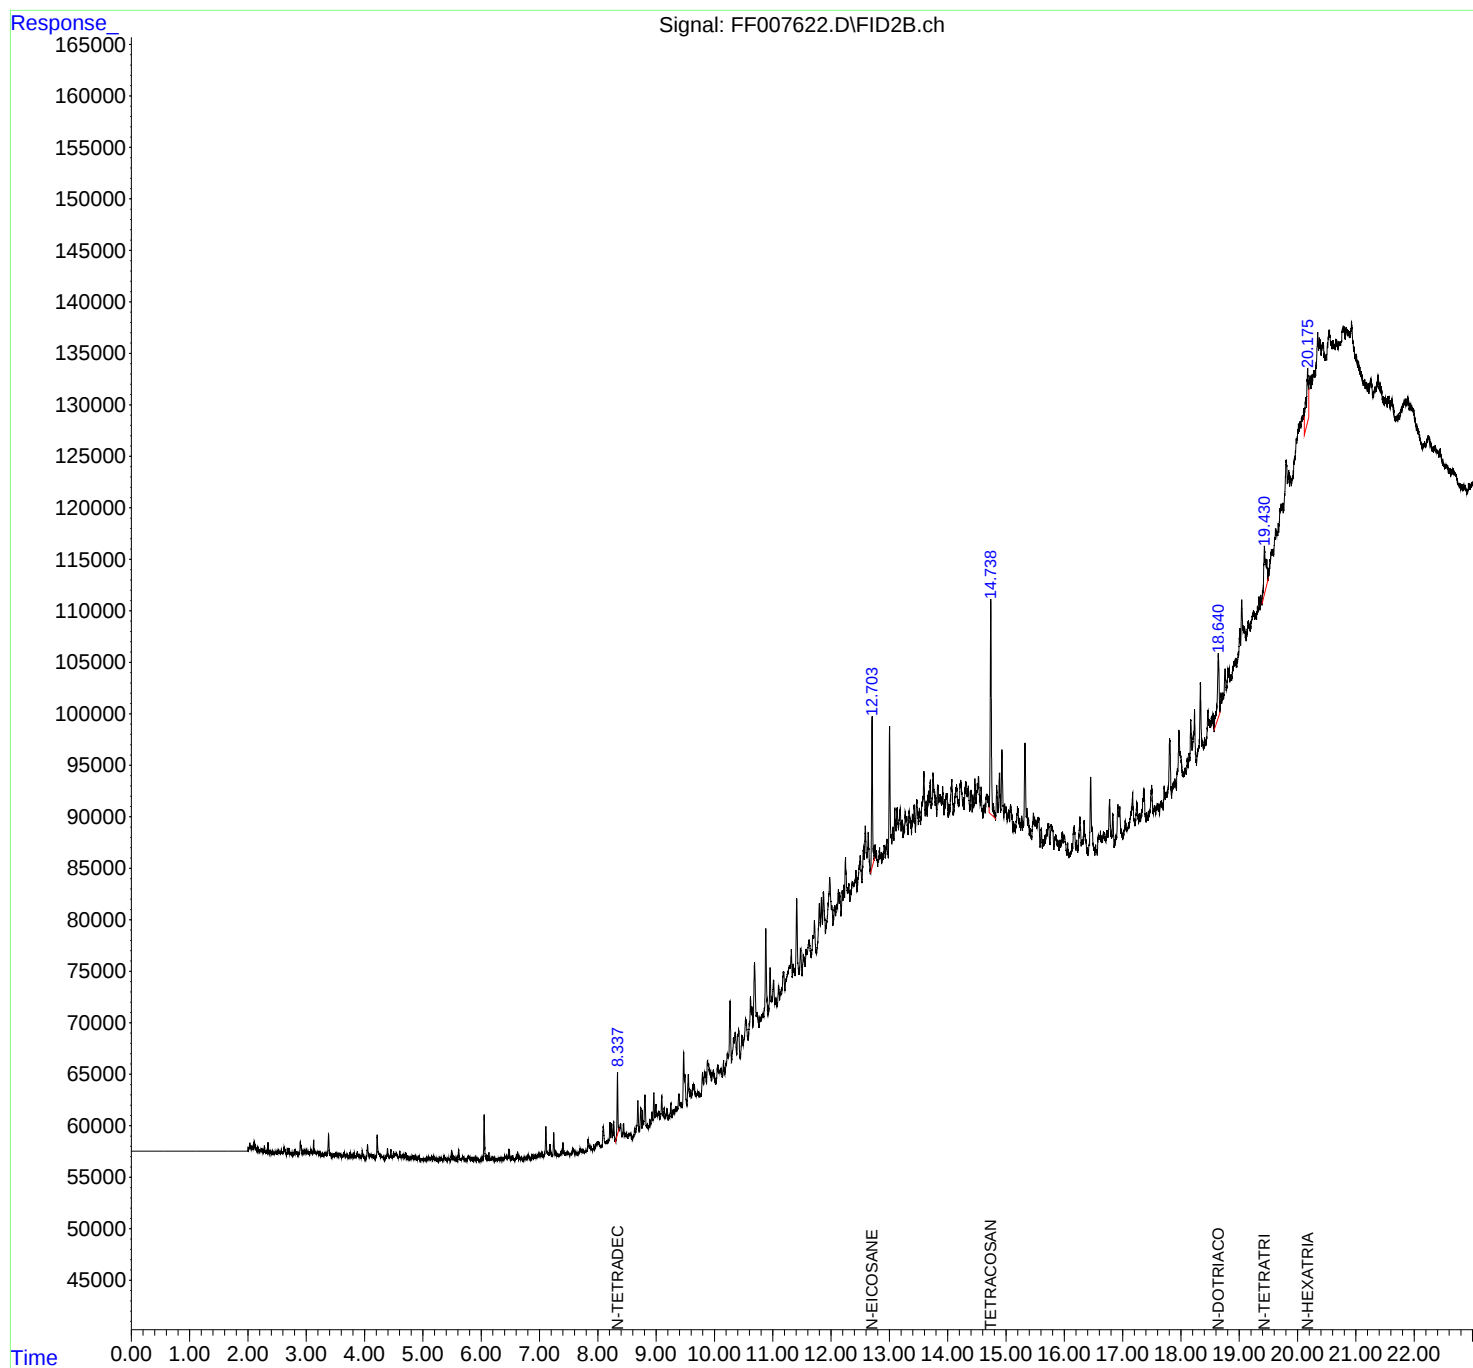


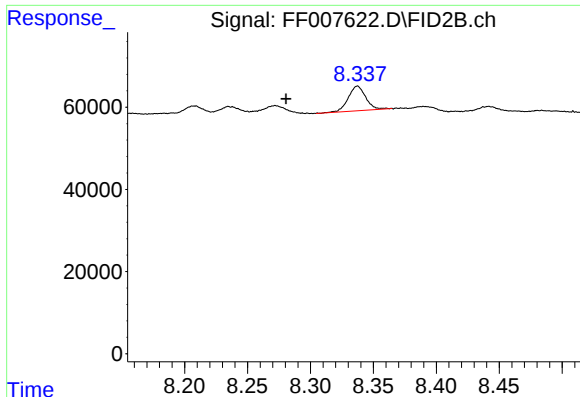

#4 N-TETRADECANE


R.T.: 8.337 min
Delta R.T.: 0.057 min
Response: 57991
Conc: 0.35 ug/ml

Instrument :
FID_F
ClientSampleId :

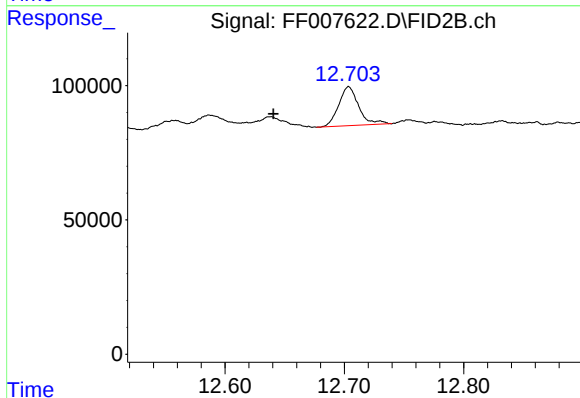


#7 N-EICOSANE

R.T.: 12.704 min
Delta R.T.: 0.063 min
Response: 167717
Conc: 1.00 ug/ml

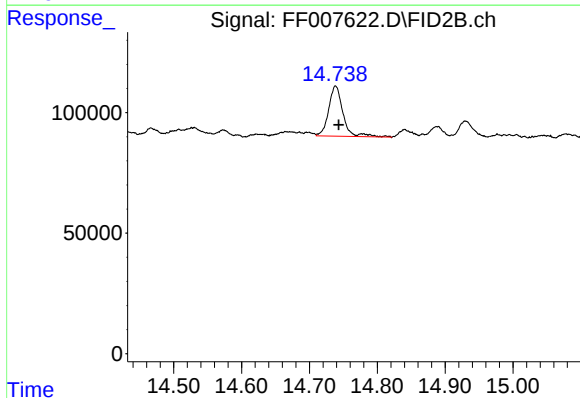


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.739 min
Delta R.T.: -0.005 min
Response: 303847
Conc: 2.07 ug/ml

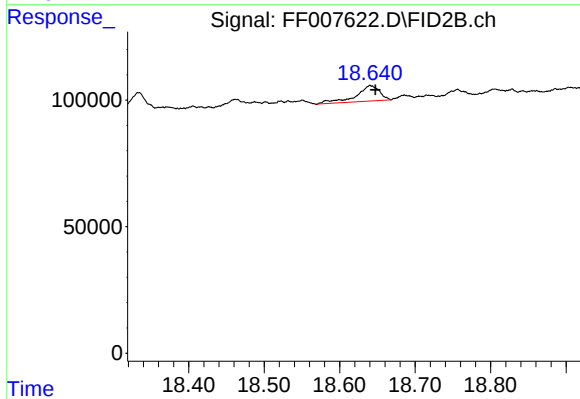

#14 N-DOTRIACONTANE


R.T.: 18.641 min
Delta R.T.: -0.006 min
Response: 133248
Conc: 0.96 ug/ml

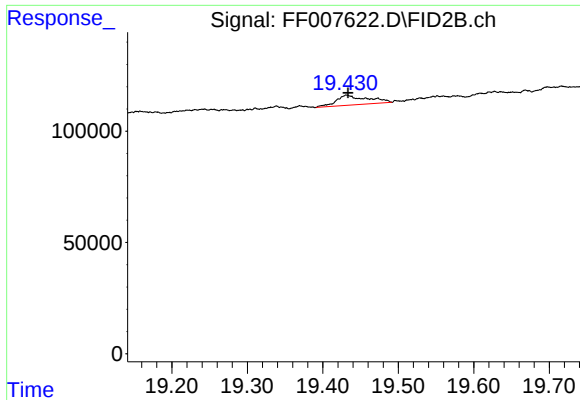

#15 N-TETRATRIACONTANE

R.T.: 19.432 min
Delta R.T.: -0.001 min
Response: 126593
Conc: 1.00 ug/ml

Instrument :
FID_F
ClientSampleId :

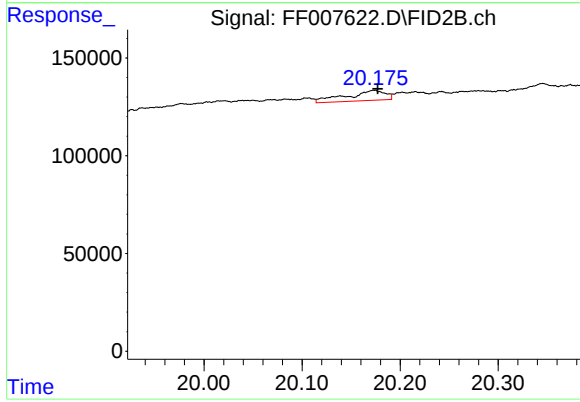

#16 N-HEXATRIACONTANE

R.T.: 20.173 min
Delta R.T.: -0.004 min
Response: 142684
Conc: 1.19 ug/ml