

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
 Data File : FF007623.D
 Signal(s) : FID2B.ch
 Acq On : 18 Sep 2020 19:53
 Operator : DD\AJ
 Sample : L4075-01 10X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 19 00:34:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	253460	1.723 ug/ml
Target Compounds			
7) N-EICOSANE	12.703f	143032	0.851 ug/ml
13) N-TRIACONTANE	17.810	238663	1.615 ug/ml
14) N-DOTRIACONTANE	18.639	106213	0.765 ug/ml
15) N-TETRATRIACONTANE	19.457	178333	1.413 ug/ml
16) N-HEXATRIACONTANE	20.181	239239	2.002 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007623.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 19:53
Operator : DD\AJ
Sample : L4075-01 10X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Sep 19 00:34:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

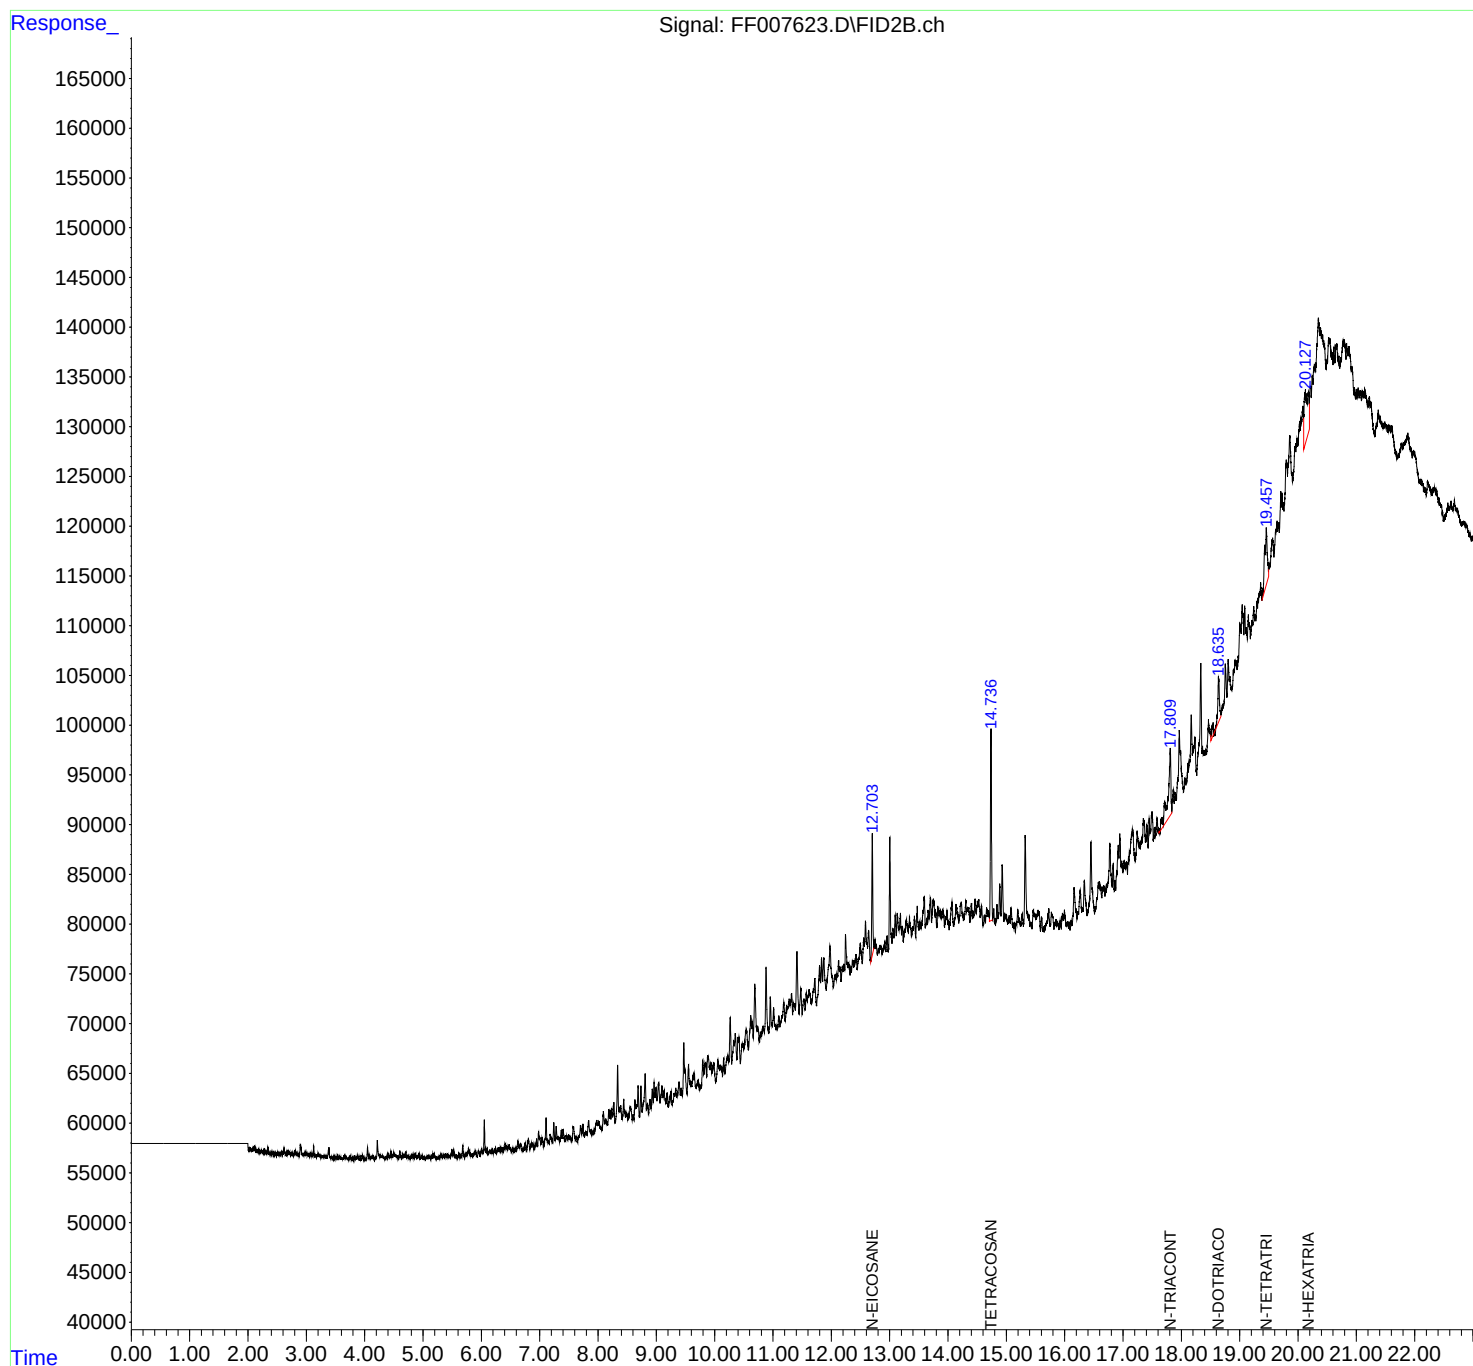


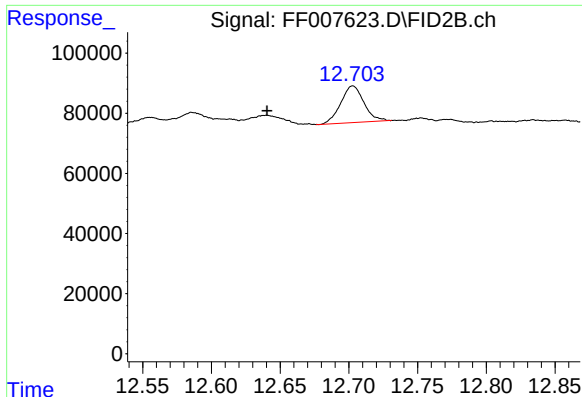

#7 N-EICOSANE


R.T.: 12.703 min
Delta R.T.: 0.062 min
Response: 143032
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :

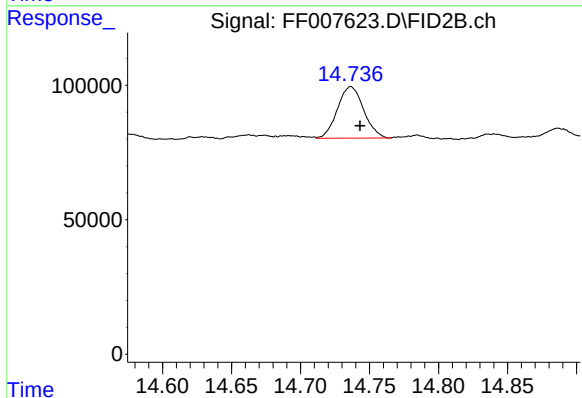


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.736 min
Delta R.T.: -0.007 min
Response: 253460
Conc: 1.72 ug/ml

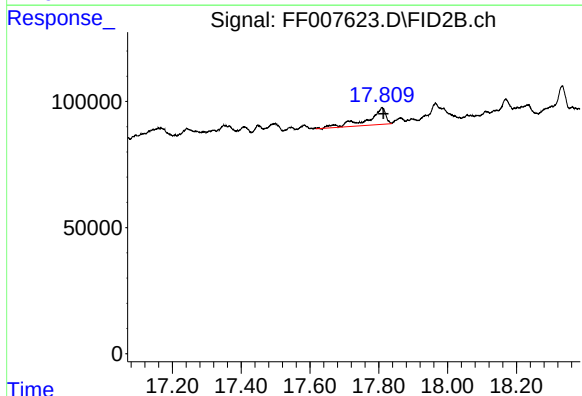


#13 N-TRIACONTANE

R.T.: 17.810 min
Delta R.T.: -0.004 min
Response: 238663
Conc: 1.61 ug/ml

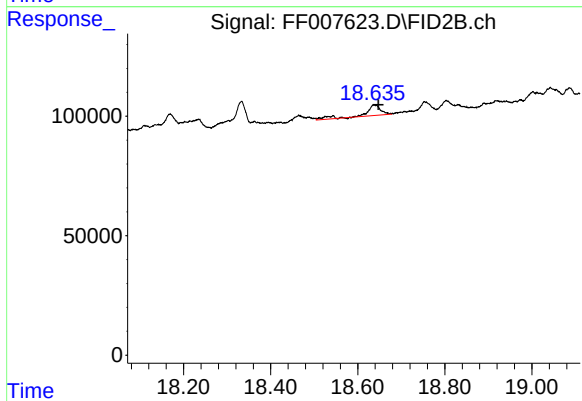

#14 N-DOTRIACONTANE


R.T.: 18.639 min
Delta R.T.: -0.009 min
Response: 106213
Conc: 0.77 ug/ml

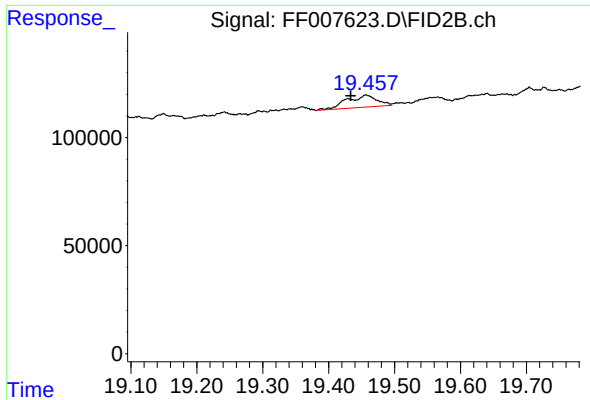

#15 N-TETRATRIACONTANE

R.T.: 19.457 min
Delta R.T.: 0.024 min
Response: 178333
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :

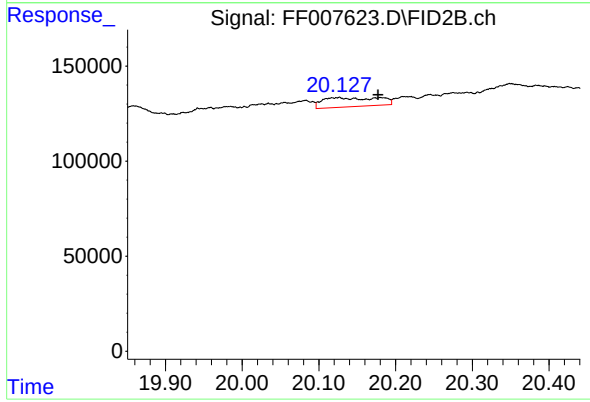

#16 N-HEXATRIACONTANE

R.T.: 20.181 min
Delta R.T.: 0.004 min
Response: 239239
Conc: 2.00 ug/ml