

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
 Data File : FF007624.D
 Signal(s) : FID2B.ch
 Acq On : 18 Sep 2020 20:23
 Operator : DD\AJ
 Sample : L4074-02 20X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 19 00:34:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	157714	1.072 ug/ml
Target Compounds			
7) N-EICOSANE	12.702f	78592	0.467 ug/ml
14) N-DOTRIACONTANE	18.640	97216	0.701 ug/ml
15) N-TETRATRIACONTANE	19.426	110622	0.877 ug/ml
16) N-HEXATRIACONTANE	20.169	403787	3.379 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007624.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 20:23
Operator : DD\AJ
Sample : L4074-02 20X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 19 00:34:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

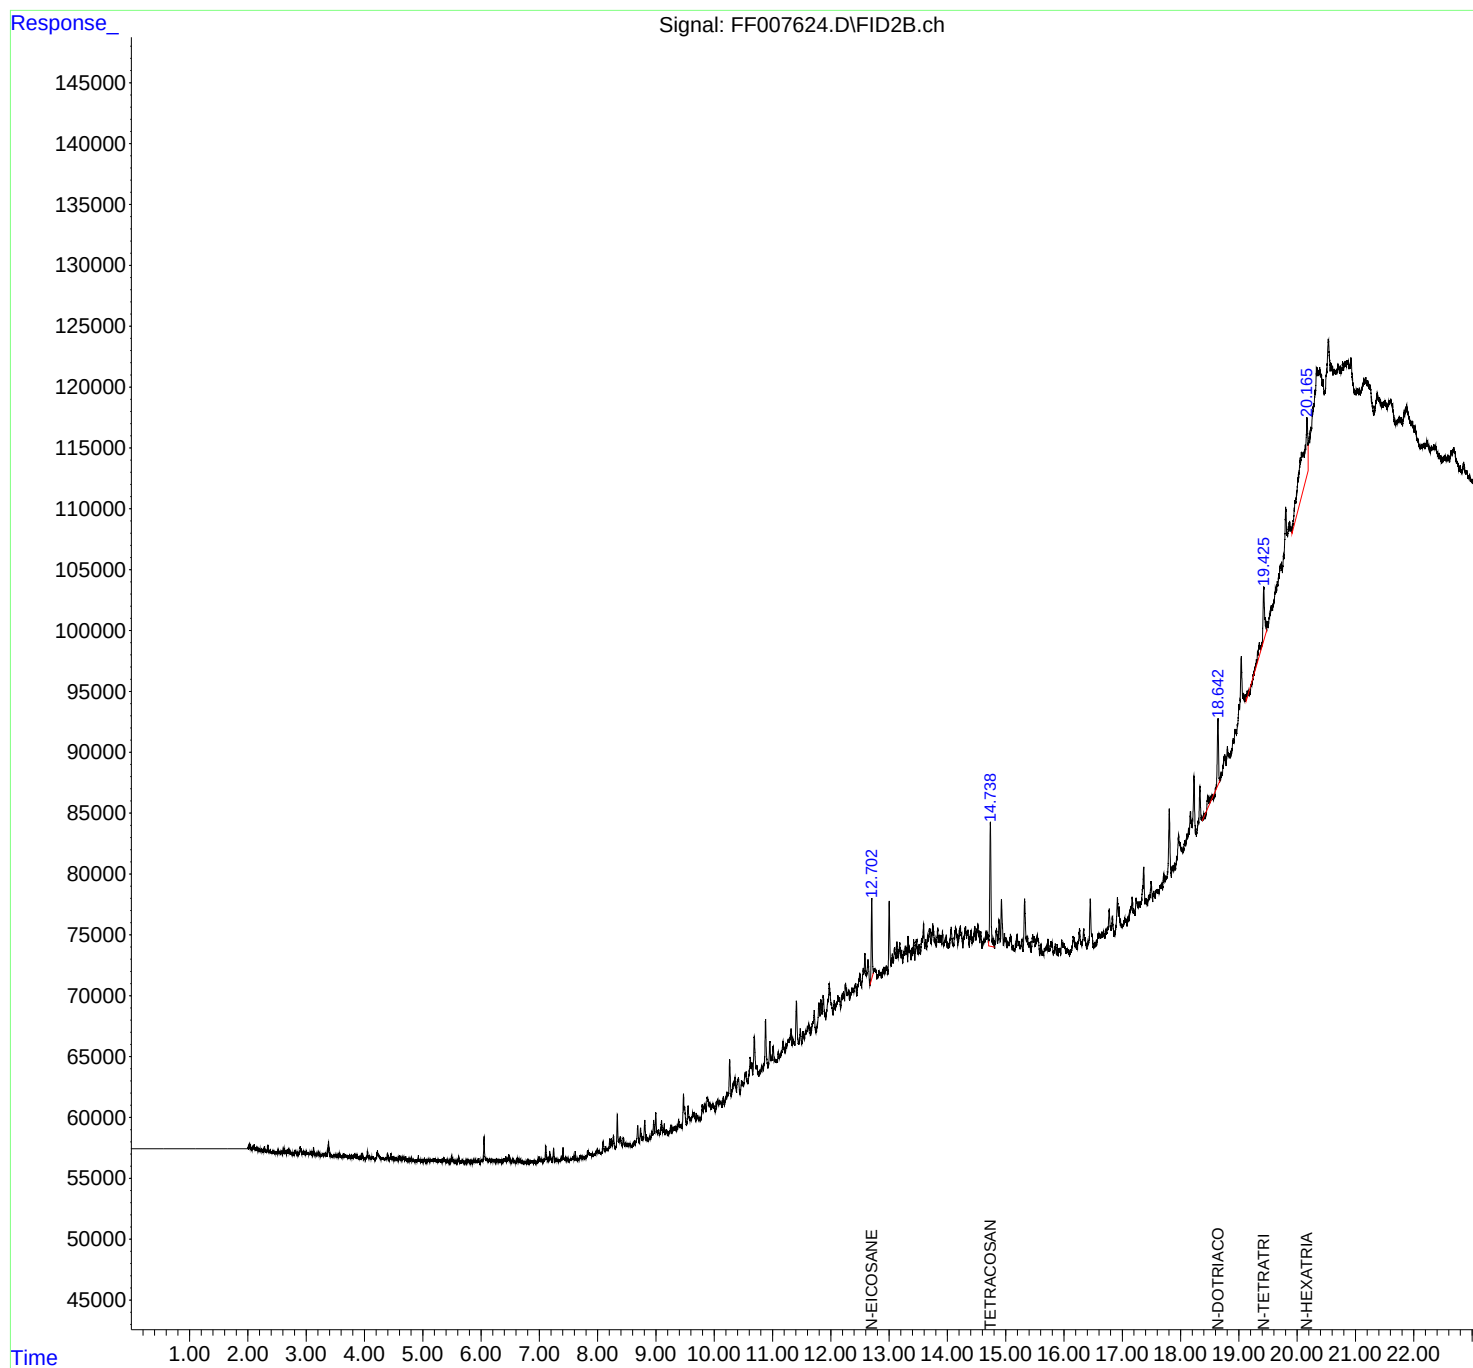


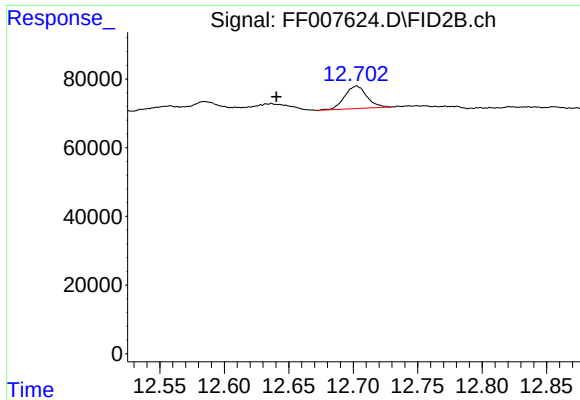

#7 N-EICOSANE


R.T.: 12.702 min
Delta R.T.: 0.062 min
Response: 78592
Conc: 0.47 ug/ml

Instrument :
FID_F
ClientSampleId :

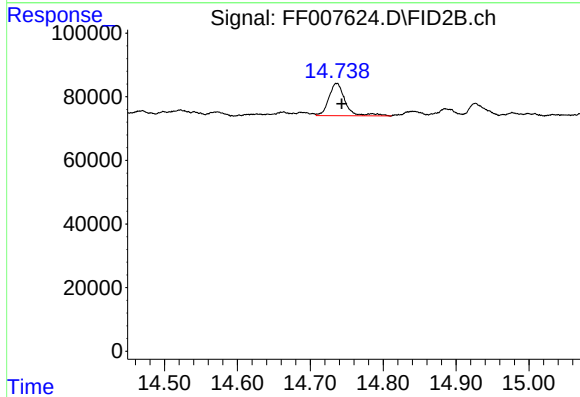


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.736 min
Delta R.T.: -0.007 min
Response: 157714
Conc: 1.07 ug/ml

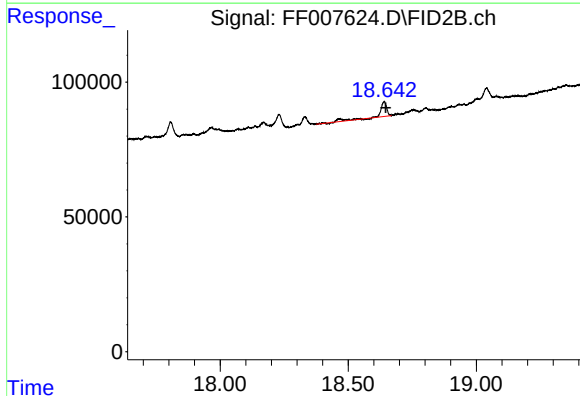


#14 N-DOTRIACONTANE

R.T.: 18.640 min
Delta R.T.: -0.007 min
Response: 97216
Conc: 0.70 ug/ml

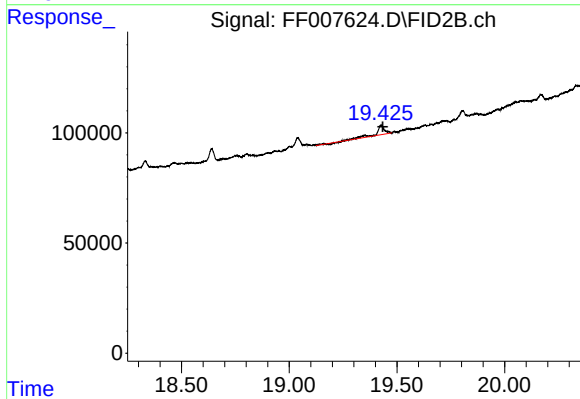

#15 N-TETRATRIACONTANE

R.T.: 19.426 min
Delta R.T.: -0.007 min
Response: 110622
Conc: 0.88 ug/ml

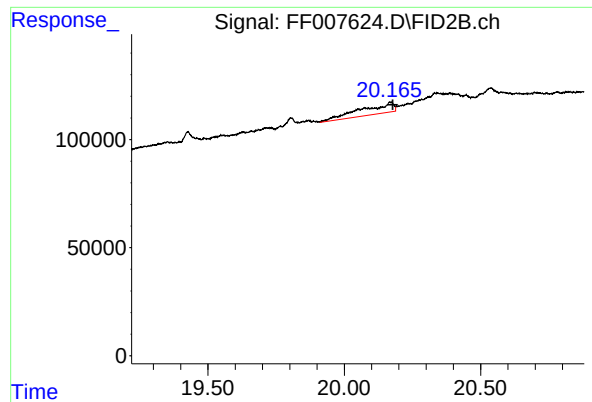

#16 N-HEXATRIACONTANE

R.T.: 20.169 min
Delta R.T.: -0.008 min
Response: 403787
Conc: 3.38 ug/ml

Instrument :
FID_F
ClientSampleId :