

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
 Data File : FF007625.D
 Signal(s) : FID2B.ch
 Acq On : 18 Sep 2020 20:54
 Operator : DD\AJ
 Sample : L4075-01 20X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 19 00:34:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.735	139931	0.951 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.641	85900	0.619 ug/ml
15) N-TETRATRIACONTANE	19.427	178321	1.413 ug/ml
16) N-HEXATRIACONTANE	20.169	463133	3.875 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007625.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 20:54
Operator : DD\AJ
Sample : L4075-01 20X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Sep 19 00:34:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

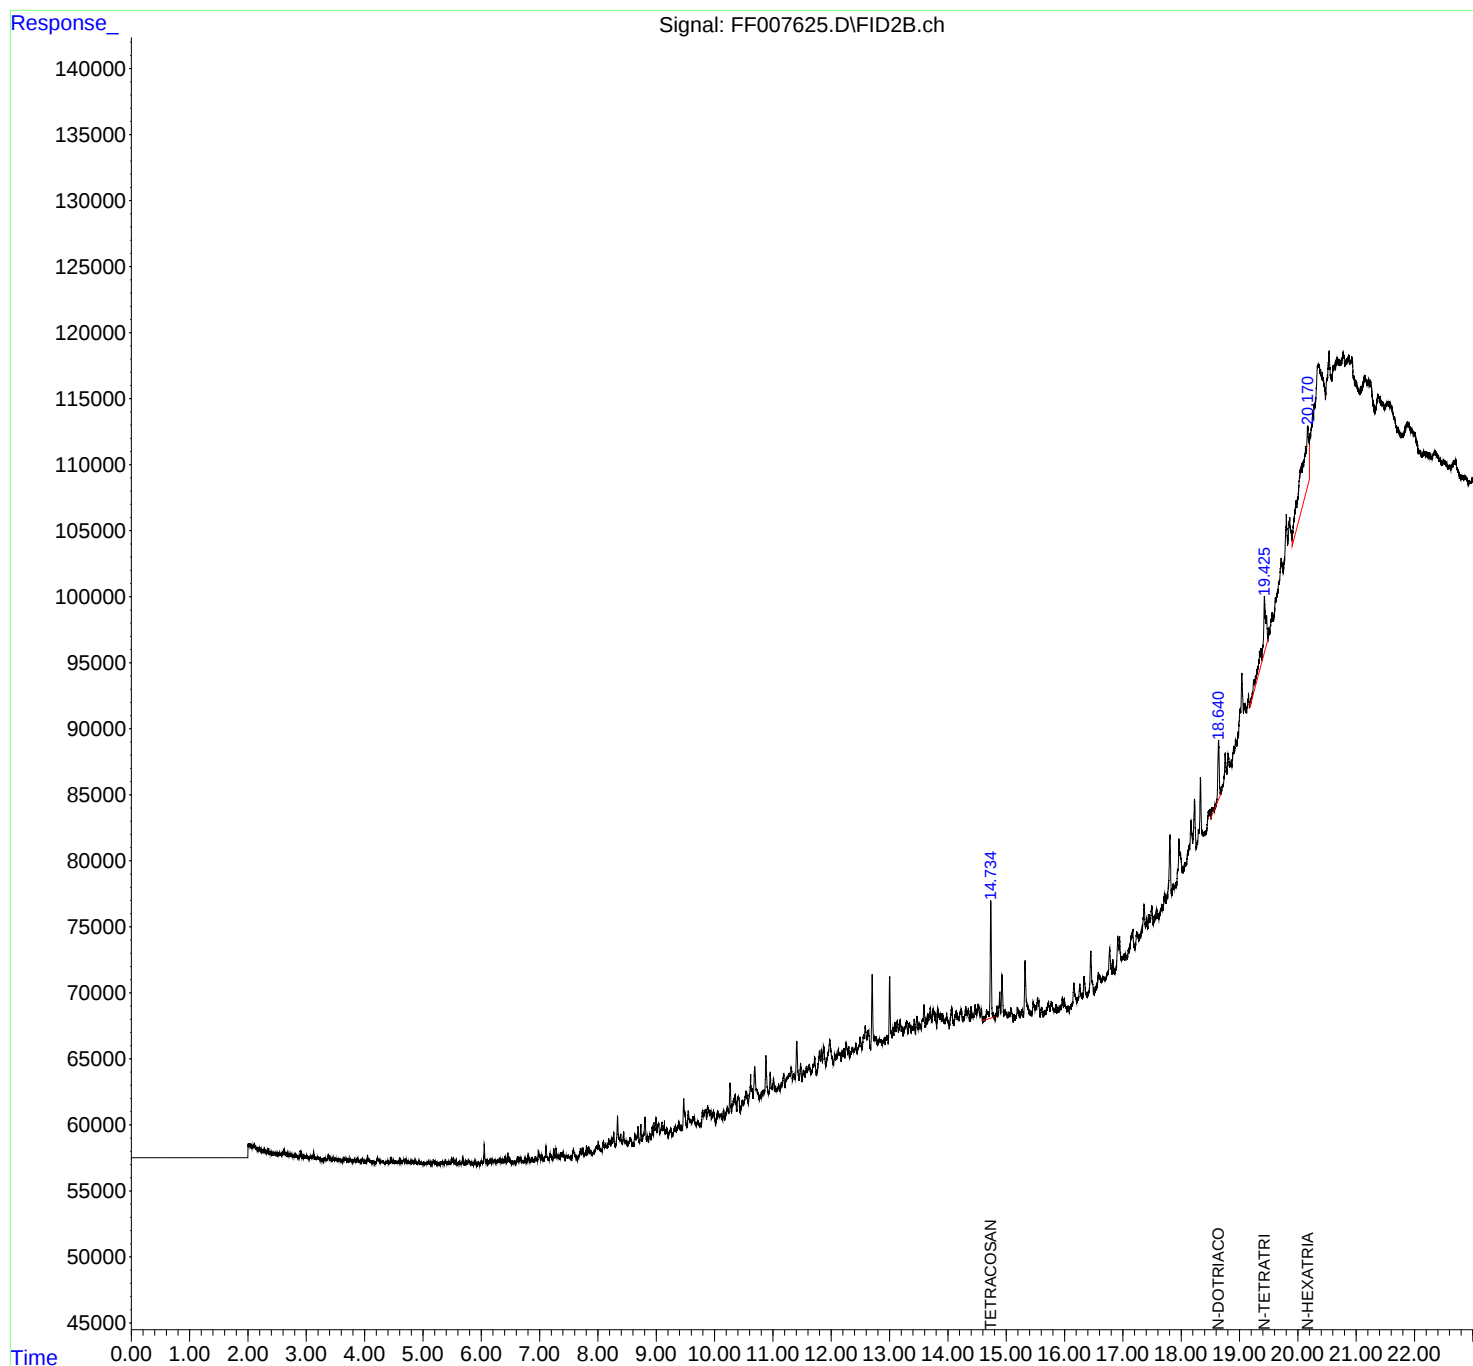


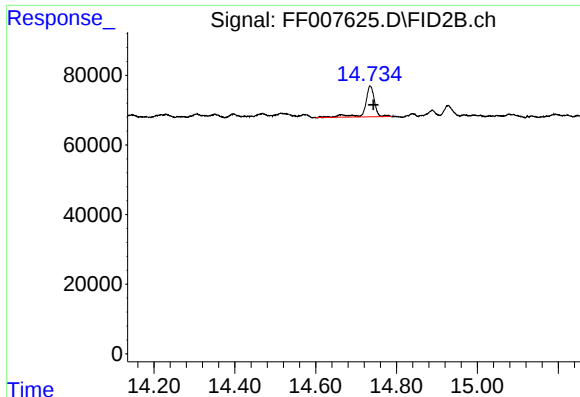

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.735 min
Delta R.T.: -0.008 min
Response: 139931
Conc: 0.95 ug/ml

Instrument :
FID_F
ClientSampleId :

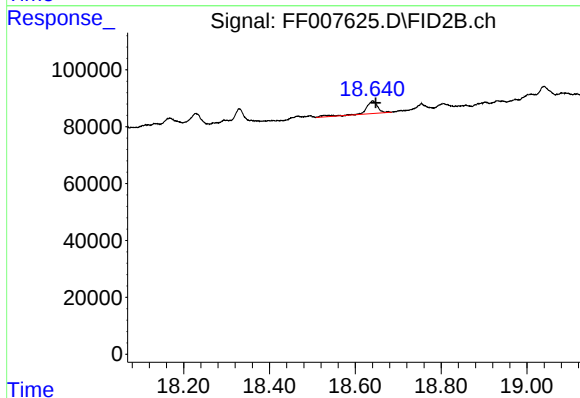


#14 N-DOTRIACONTANE

R.T.: 18.641 min
Delta R.T.: -0.007 min
Response: 85900
Conc: 0.62 ug/ml

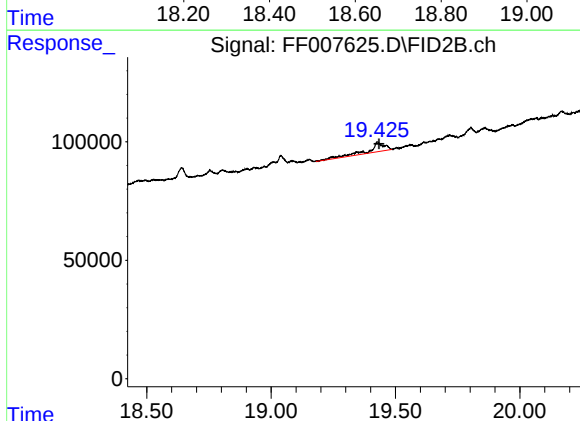

#15 N-TETRATRIACONTANE

R.T.: 19.427 min
Delta R.T.: -0.006 min
Response: 178321
Conc: 1.41 ug/ml

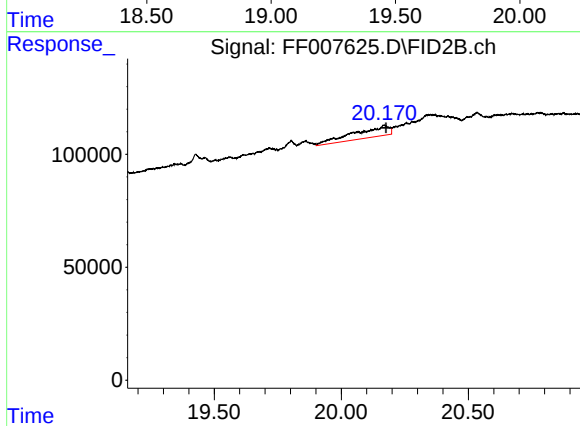

#16 N-HEXATRIACONTANE

R.T.: 20.169 min
Delta R.T.: -0.008 min
Response: 463133
Conc: 3.88 ug/ml