

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007615.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 15:45
Operator : DD\AJ
Sample : L4075-01
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTS-WC-S-IB-ST

Manual Integrations
APPROVED

Ankita
9/21/2020 1:03:50 PM

Integration File: autoint1.e
Quant Time: Sep 19 00:32:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.745	2787601	18.954 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007615.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 15:45
Operator : DD\AJ
Sample : L4075-01
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
KTS-WC-S-IB-ST


Manual Integrations
APPROVED

Ankita
9/21/2020 1:03:50 PM

Integration File: autoint1.e
Quant Time: Sep 19 00:32:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

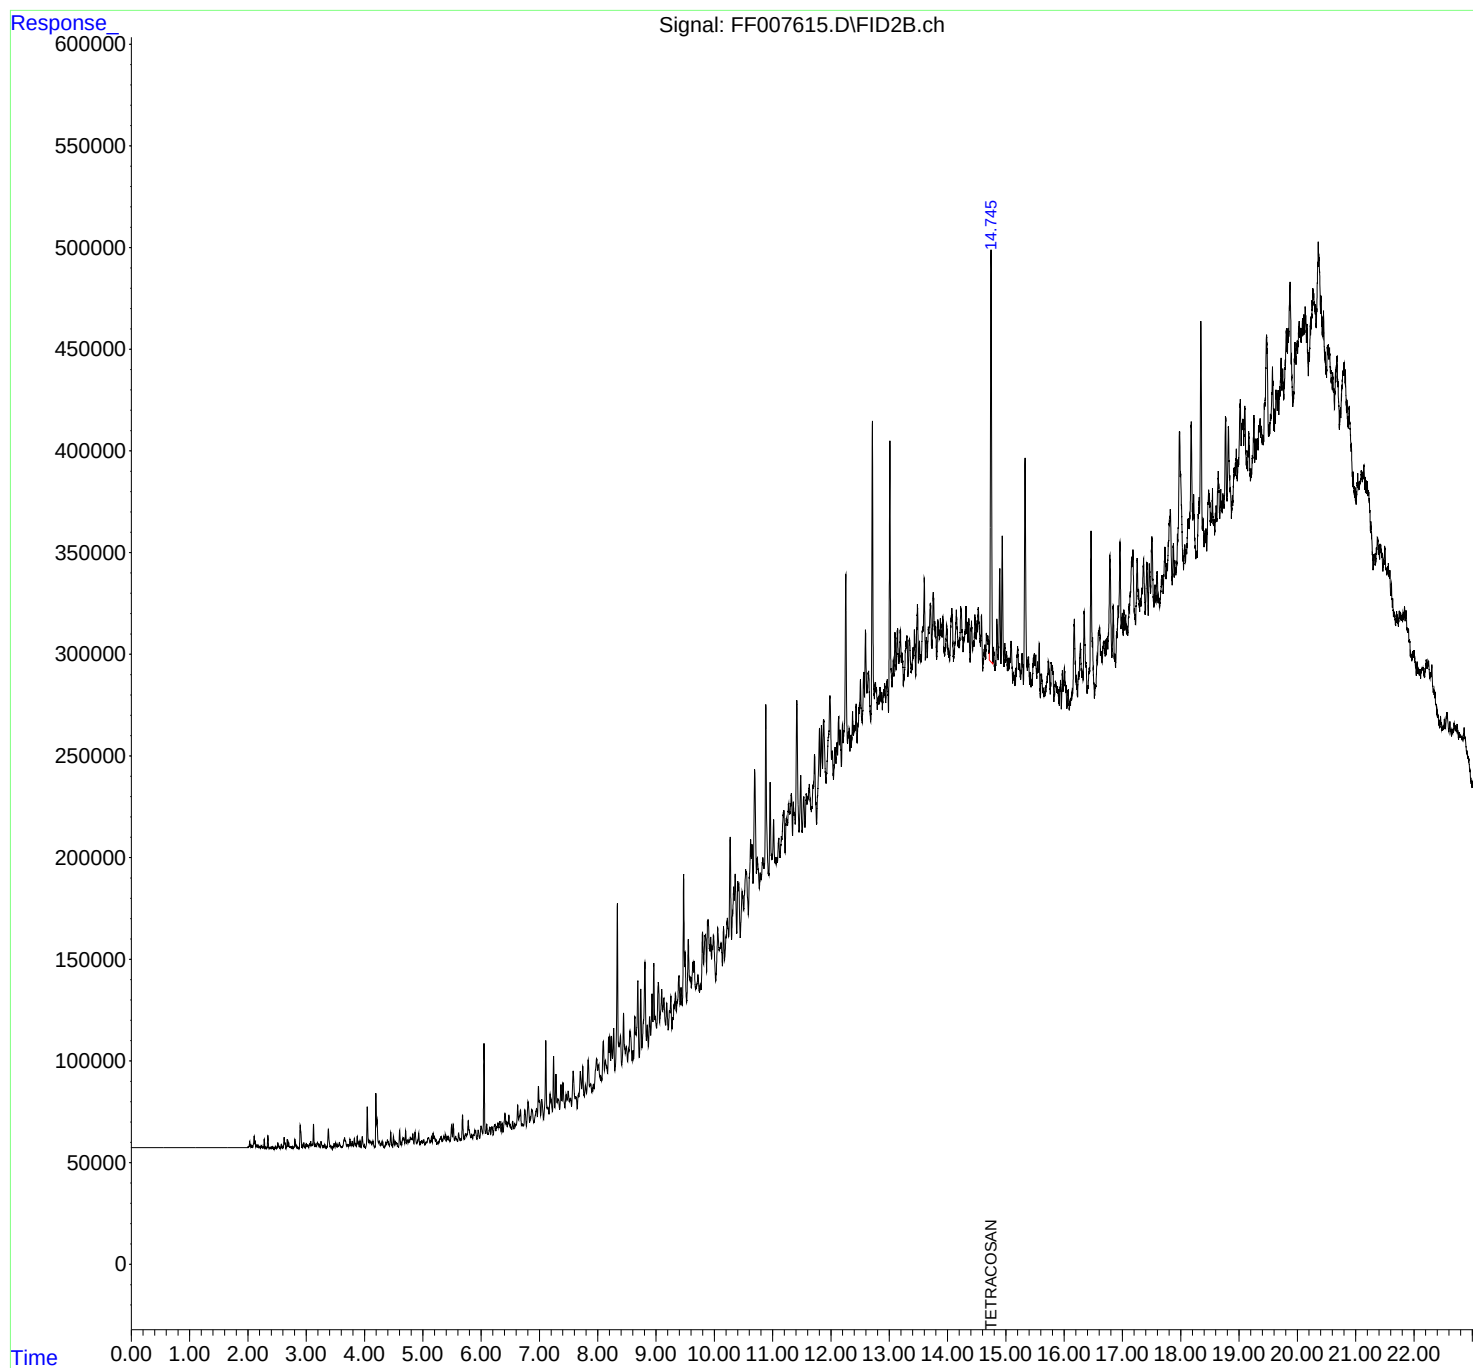

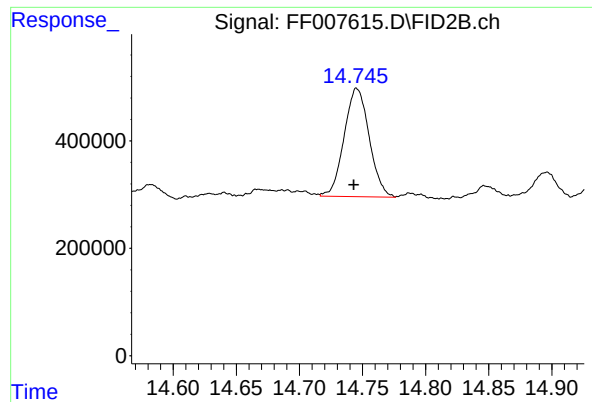

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.745 min
Delta R.T.: 0.002 min
Response: 2787601
Conc: 18.95 ug/ml m

Instrument :
FID_F
ClientSampleId :
KTS-WC-S-IB-ST

Manual Integrations
APPROVED

Ankita
9/21/2020 1:03:50 PM