

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007623.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 19:53
Operator : DD\AJ
Sample : L4075-01 10X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTS-WC-S-IB-ST

Integration File: autoint1.e
Quant Time: Sep 19 00:34:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	253460	1.723 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007623.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 19:53
Operator : DD\AJ
Sample : L4075-01 10X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTS-WC-S-IB-ST

Integration File: autoint1.e
Quant Time: Sep 19 00:34:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

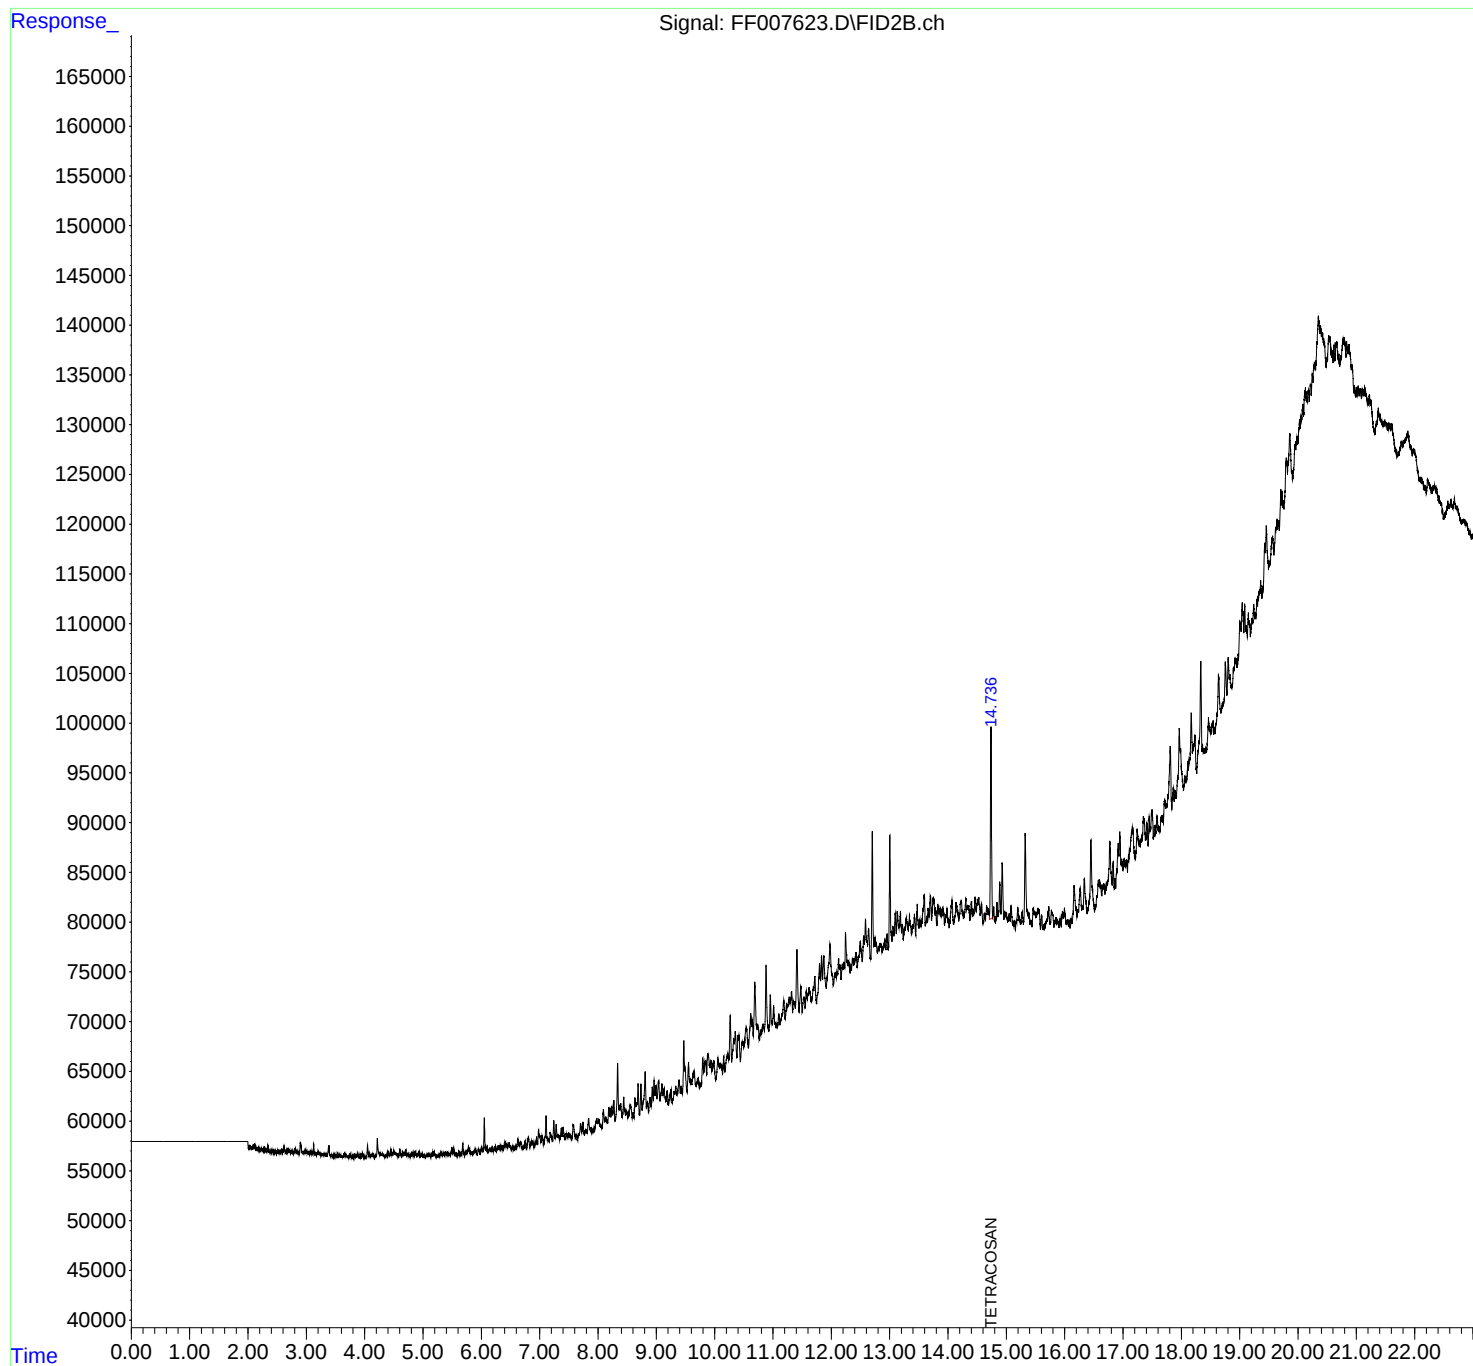

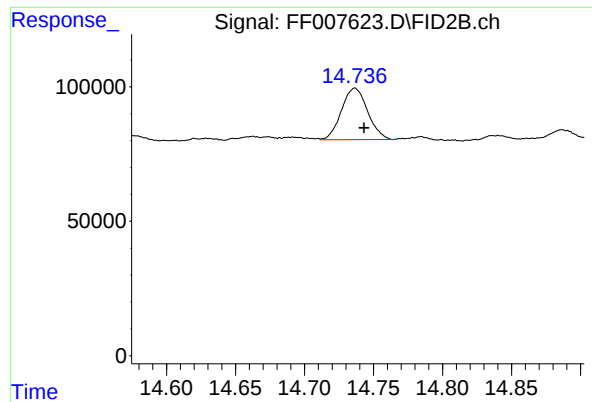

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.736 min
Delta R.T.: -0.007 min
Response: 253460
Conc: 1.72 ug/ml

Instrument :
FID_F
ClientSampleId :
KTS-WC-S-IB-ST