

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007624.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 20:23
Operator : DD\AJ
Sample : L4074-02 20X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTS-ST-0102-0-6

Manual Integrations
APPROVED

Ankita
9/21/2020 1:04:10 PM

Integration File: autoint1.e
Quant Time: Sep 19 00:34:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	138194	0.940 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091820\
Data File : FF007624.D
Signal(s) : FID2B.ch
Acq On : 18 Sep 2020 20:23
Operator : DD\AJ
Sample : L4074-02 20X
Misc :
ALS Vial : 68 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
KTS-ST-0102-0-6


Manual Integrations
APPROVED

Ankita
9/21/2020 1:04:10 PM

Integration File: autoint1.e
Quant Time: Sep 19 00:34:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

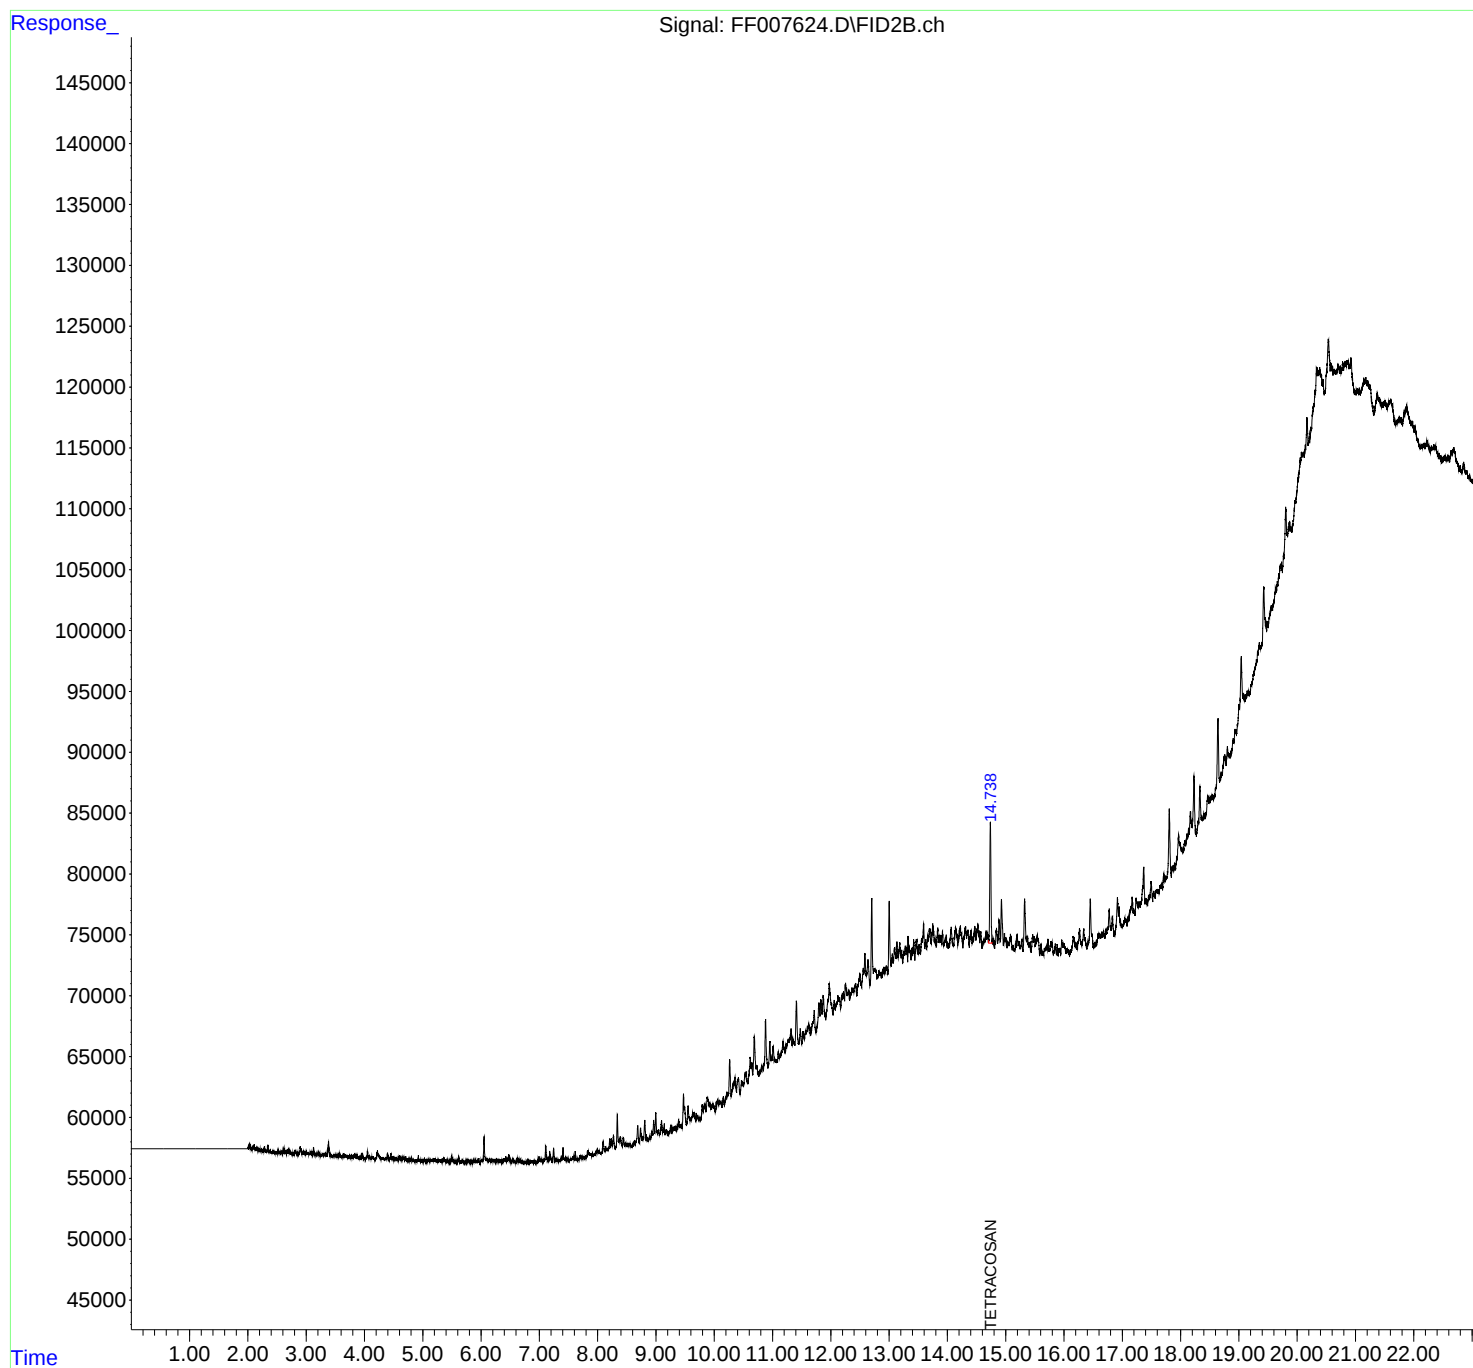

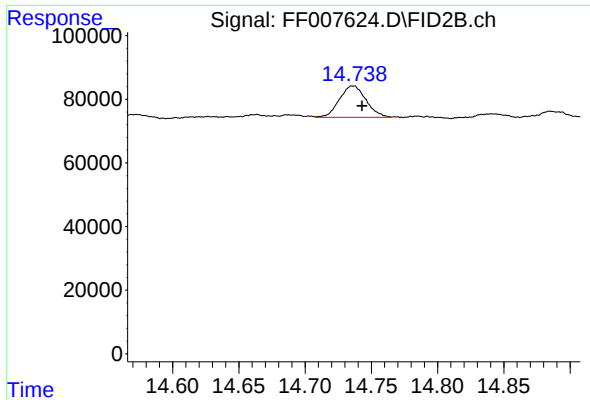

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.738 min
Delta R.T.: -0.006 min
Response: 138194
Conc: 0.94 ug/ml m

Instrument :
FID_F
ClientSampleId :
KTS-ST-0102-0-6

Manual Integrations
APPROVED

Ankita
9/21/2020 1:04:10 PM