

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF091820\  
Data File : FF007625.D  
Signal(s) : FID2B.ch  
Acq On : 18 Sep 2020 20:54  
Operator : DD\AJ  
Sample : L4075-01 20X  
Misc :  
ALS Vial : 69 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
KTS-WC-S-IB-ST

Manual Integrations  
APPROVED

Ankita  
9/21/2020 1:04:12 PM

Integration File: autoint1.e  
Quant Time: Sep 19 00:34:48 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF090120.M  
Quant Title :  
QLast Update : Wed Sep 02 11:29:30 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.734 | 115929   | 0.788 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF091820\  
Data File : FF007625.D  
Signal(s) : FID2B.ch  
Acq On : 18 Sep 2020 20:54  
Operator : DD\AJ  
Sample : L4075-01 20X  
Misc :  
ALS Vial : 69 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
KTS-WC-S-IB-ST


Manual Integrations  
APPROVED

Ankita  
9/21/2020 1:04:12 PM

Integration File: autoint1.e  
Quant Time: Sep 19 00:34:48 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF090120.M  
Quant Title :  
QLast Update : Wed Sep 02 11:29:30 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

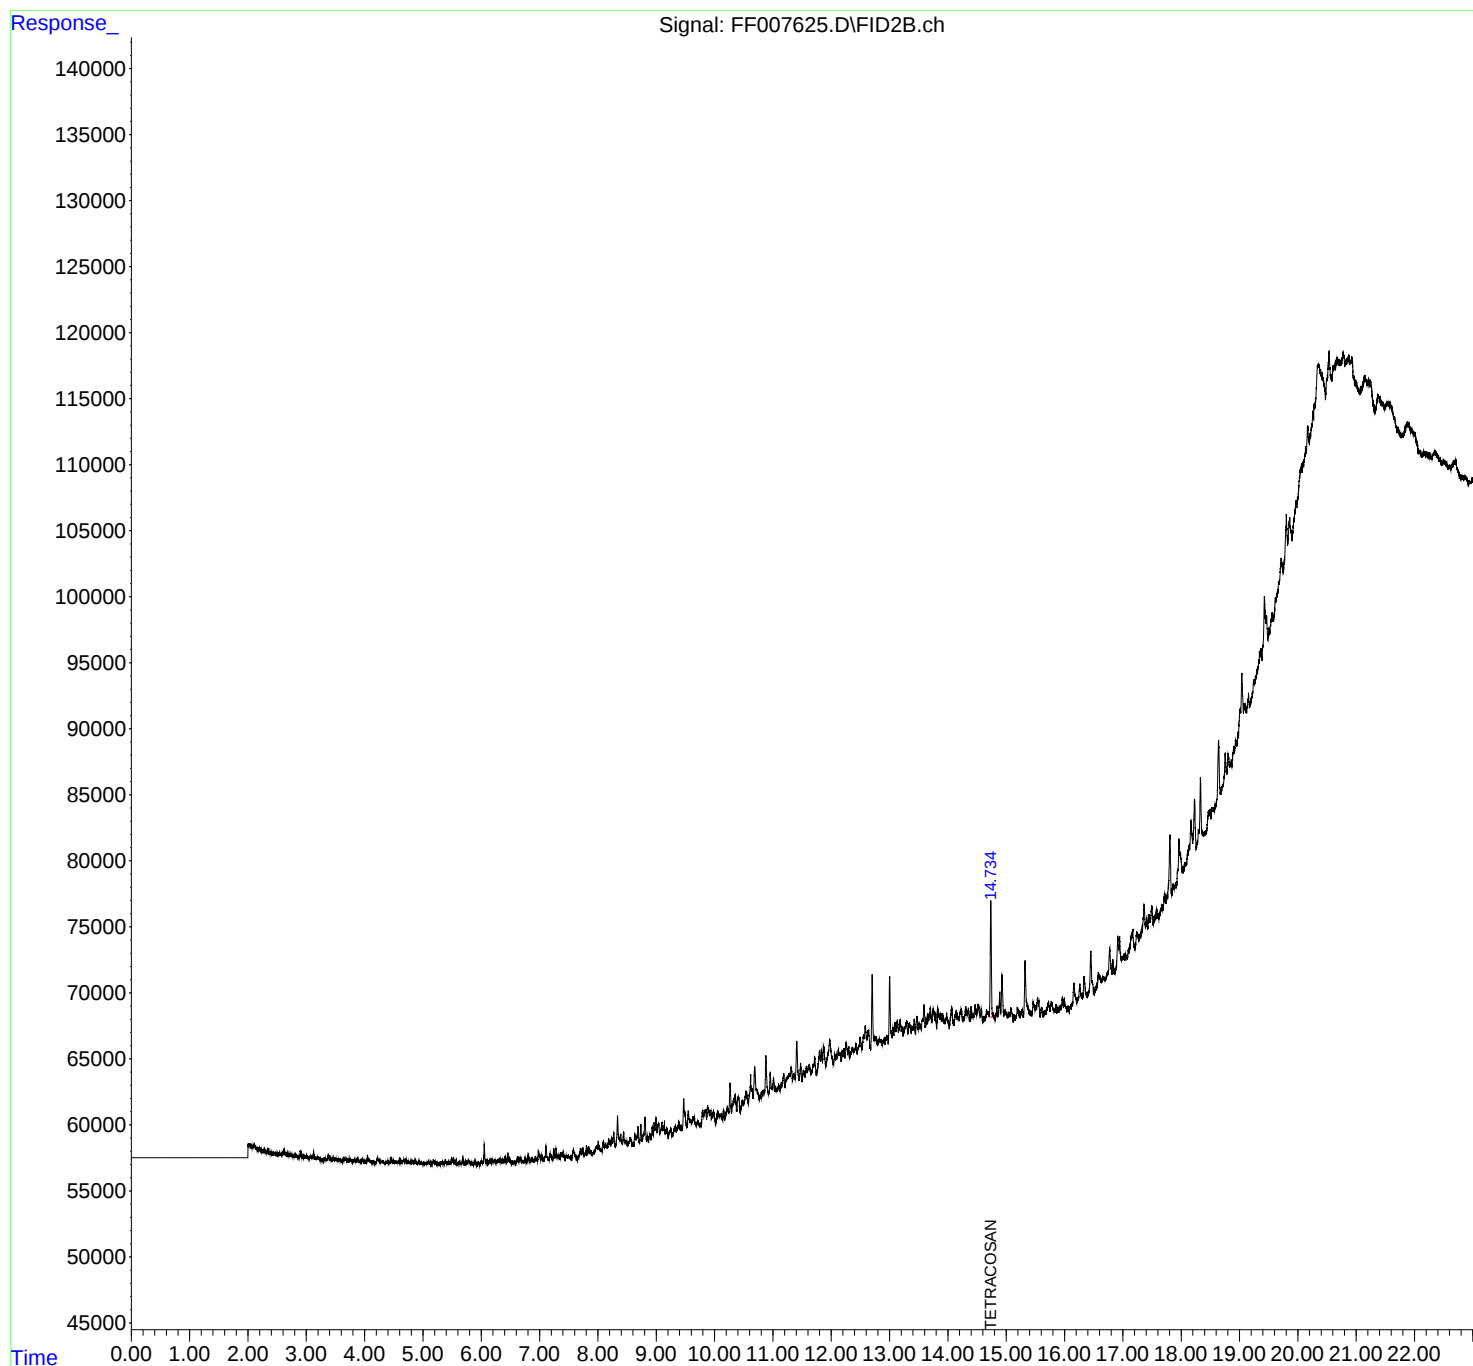

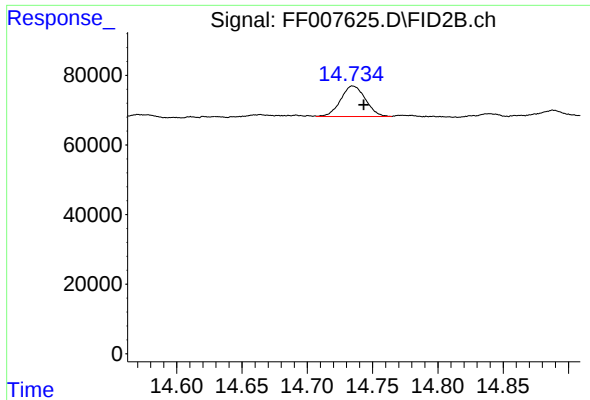

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.734 min  
Delta R.T.: -0.009 min  
Response: 115929  
Conc: 0.79 ug/ml m

Instrument :  
FID\_F  
ClientSampleId :  
KTS-WC-S-IB-ST

Manual Integrations  
APPROVED

Ankita  
9/21/2020 1:04:12 PM