

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091918\
 Data File : FF002141.D
 Signal(s) : FID2B.ch
 Acq On : 19 Sep 2018 10:49
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 20 03:40:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.268	6025015	48.070 ug/ml
Target Compounds			
2) N-DECANE	4.047	6450326	55.657 ug/ml
3) N-DODECANE	6.056	6683400	53.412 ug/ml
4) N-TETRADECANE	7.843	6840840	51.628 ug/ml
5) N-HEXADECANE	9.436	6913313	50.479 ug/ml
6) N-OCTADECANE	10.872	6955062	49.597 ug/ml
7) N-EICOSANE	12.177	6906058	48.451 ug/ml
8) N-DOCOSANE	13.371	6856064	48.122 ug/ml
10) N-TETRACOSANE	14.471	6852539	48.288 ug/ml
11) N-HEXACOSANE	15.489	6774412	47.629 ug/ml
12) N-OCTACOSANE	16.438	6796030	47.370 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091918\
Data File : FF002141.D
Signal(s) : FID2B.ch
Acq On : 19 Sep 2018 10:49
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 20 03:40:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

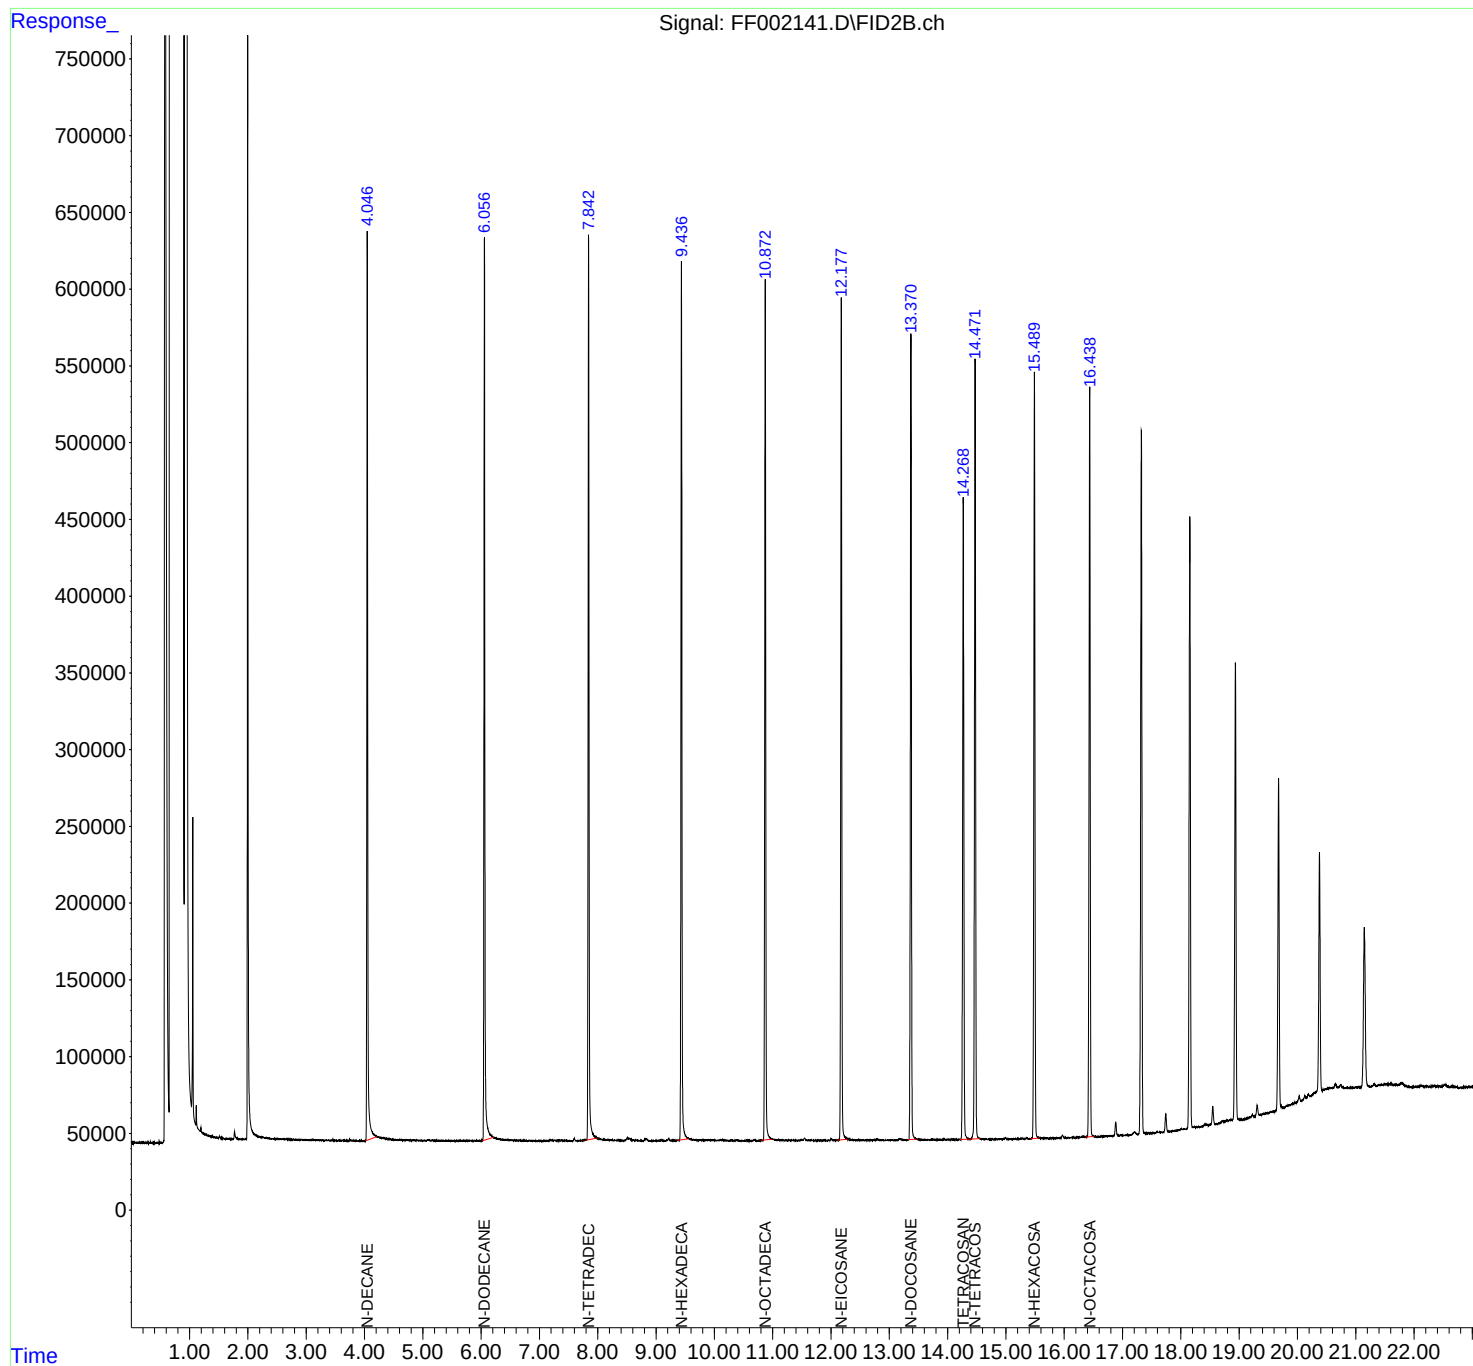

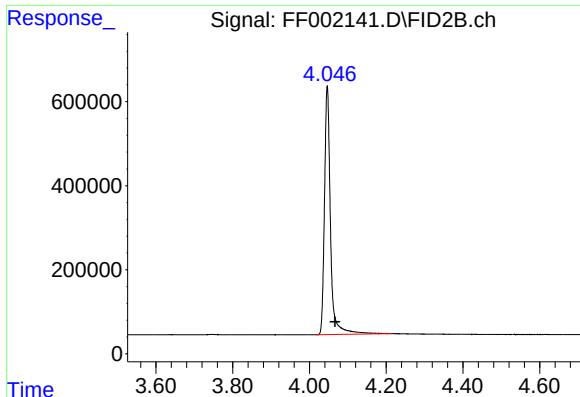


#2 N-DECANE

R.T.: 4.047 min
Delta R.T.: -0.020 min
Response: 6450326
Conc: 55.66 ug/ml

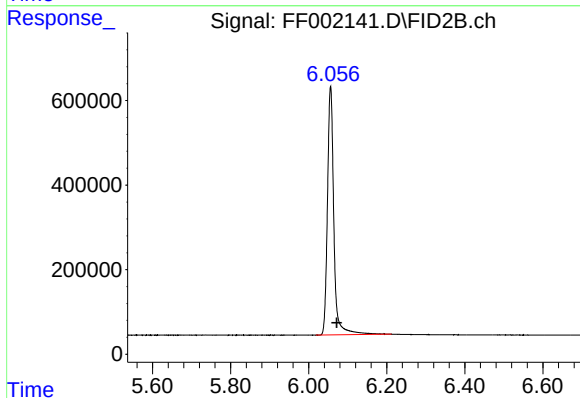


#3 N-DODECANE

R.T.: 6.056 min
Delta R.T.: -0.015 min
Response: 6683400
Conc: 53.41 ug/ml

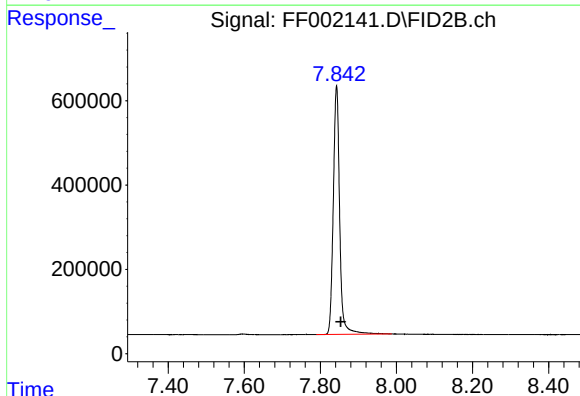


#4 N-TETRADECANE

R.T.: 7.843 min
Delta R.T.: -0.011 min
Response: 6840840
Conc: 51.63 ug/ml

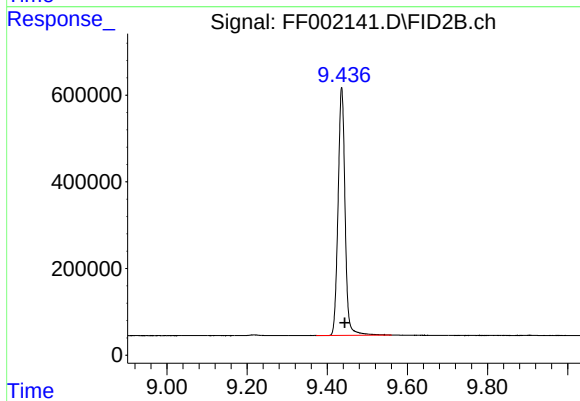


#5 N-HEXADECANE

R.T.: 9.436 min
Delta R.T.: -0.007 min
Response: 6913313
Conc: 50.48 ug/ml

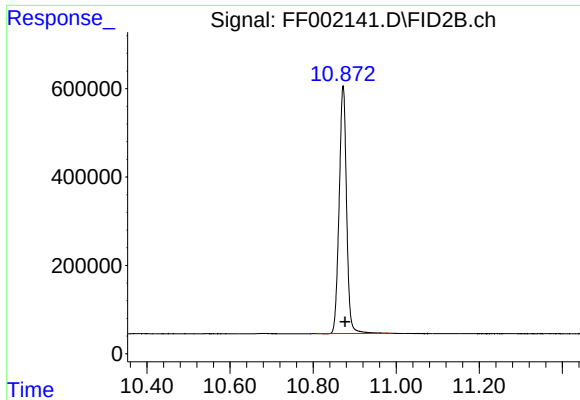


#6 N-OCTADECANE

R.T.: 10.872 min
Delta R.T.: -0.005 min
Response: 6955062
Conc: 49.60 ug/ml

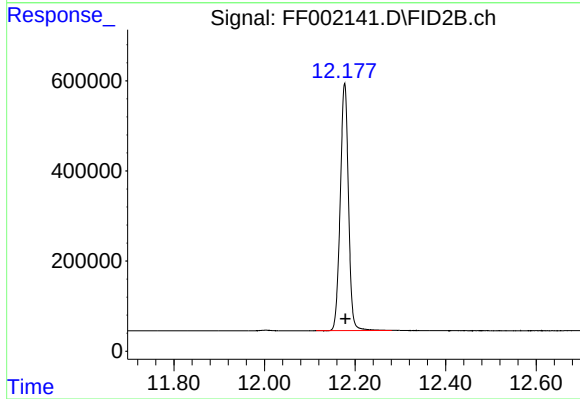


#7 N-EICOSANE

R.T.: 12.177 min
Delta R.T.: -0.002 min
Response: 6906058
Conc: 48.45 ug/ml

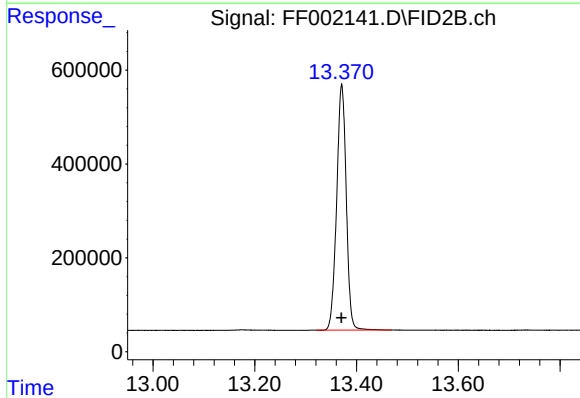


#8 N-DOCOSANE

R.T.: 13.371 min
Delta R.T.: 0.000 min
Response: 6856064
Conc: 48.12 ug/ml

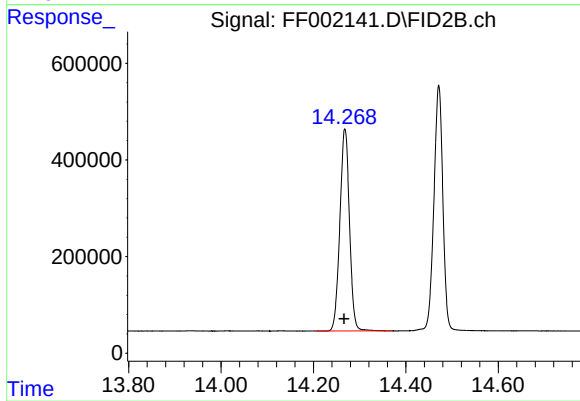


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.268 min
Delta R.T.: 0.002 min
Response: 6025015
Conc: 48.07 ug/ml

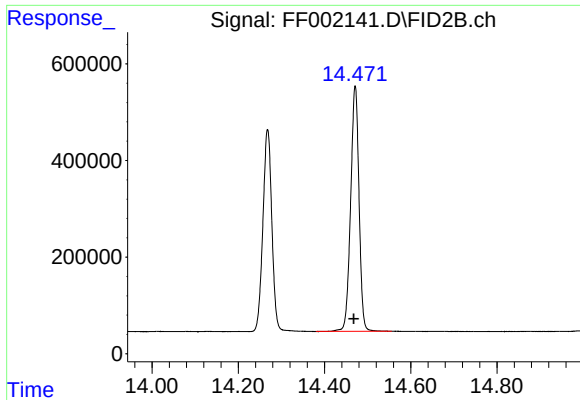


#10 N-TETRACOSANE

R.T.: 14.471 min
Delta R.T.: 0.003 min
Response: 6852539
Conc: 48.29 ug/ml

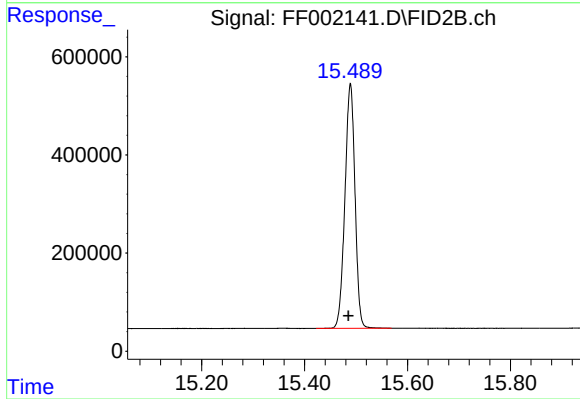

#11 N-HEXACOSANE

R.T.: 15.489 min
Delta R.T.: 0.004 min
Response: 6774412
Conc: 47.63 ug/ml

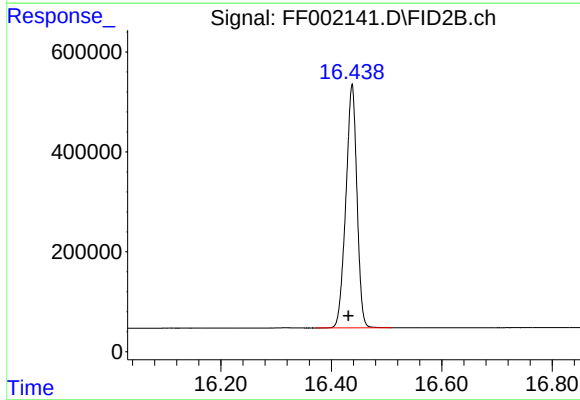

#12 N-OCTACOSANE

R.T.: 16.438 min
Delta R.T.: 0.007 min
Response: 6796030
Conc: 47.37 ug/ml