

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091919\
Data File : FF005632.D
Signal(s) : FID2B.ch
Acq On : 19 Sep 2019 16:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 20 01:18:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.623	2052986	19.185 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.540	47758	0.385 ug/ml
15) N-TETRATRIACONTANE	19.333	131581	1.092 ug/ml
16) N-HEXATRIACONTANE	20.080	334213	2.785 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091919\
Data File : FF005632.D
Signal(s) : FID2B.ch
Acq On : 19 Sep 2019 16:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 20 01:18:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

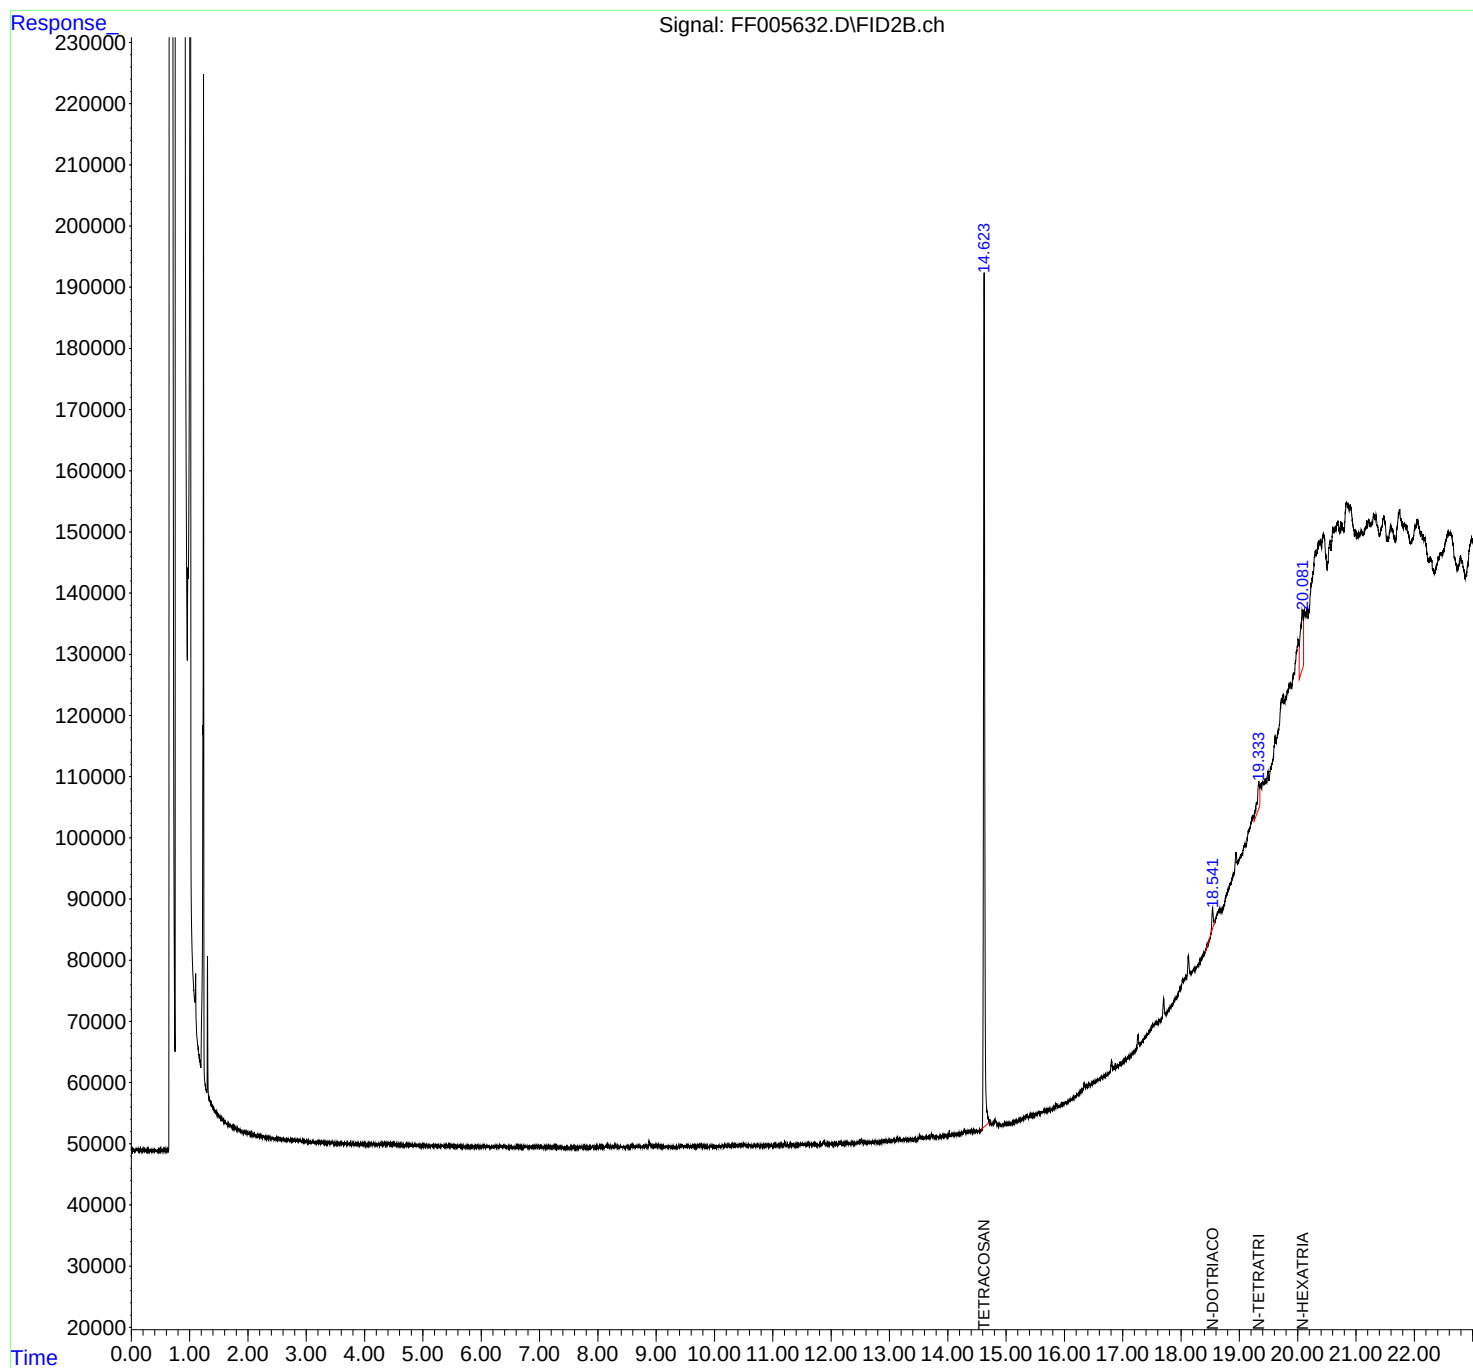


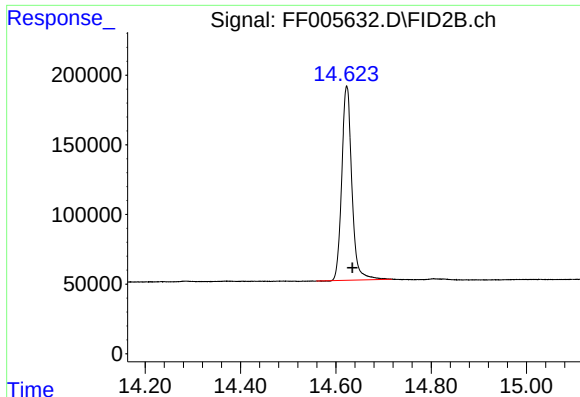

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.623 min
Delta R.T.: -0.011 min
Response: 2052986
Conc: 19.19 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

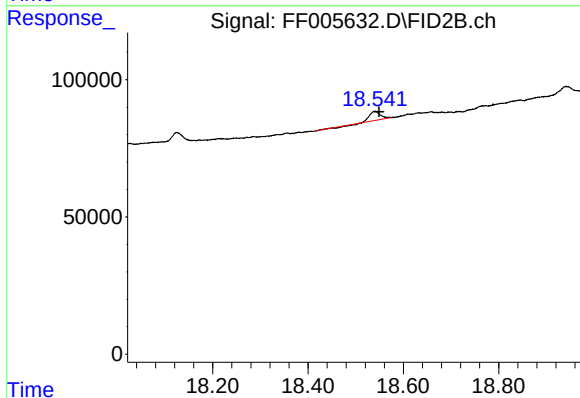


#14 N-DOTRIACONTANE

R.T.: 18.540 min
Delta R.T.: -0.009 min
Response: 47758
Conc: 0.39 ug/ml

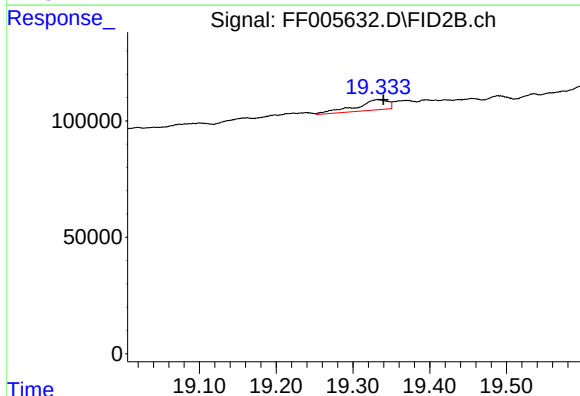

#15 N-TETRATRIACONTANE

R.T.: 19.333 min
Delta R.T.: -0.006 min
Response: 131581
Conc: 1.09 ug/ml

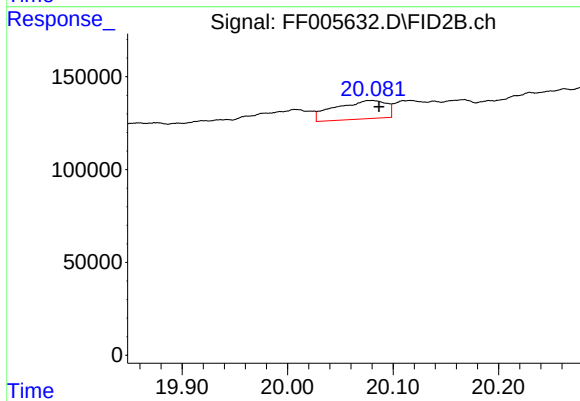

#16 N-HEXATRIACONTANE

R.T.: 20.080 min
Delta R.T.: -0.007 min
Response: 334213
Conc: 2.78 ug/ml